

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036986.D
 Acq On : 12 Oct 2022 16:30
 Operator : CG/JU
 Sample : N5024-04DL 5X
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BF1DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
 Supervised By :mohammad ahmed 10/14/2022

Quant Time: Oct 12 23:11:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	10138	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	36169	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	18256	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	32817	0.400	ng/ul	0.00
17) Chrysene-d12	21.484	240	17814	0.400	ng/ul	0.00
23) Perylene-d12	23.884	264	16738	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	12226	0.855	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	4218	0.077	ng/ul	0.00
18) Fluoranthene-d10	19.337	212	6323	0.119	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.803	128	40814	0.395	ng/ul	97
7) 2-Methylnaphthalene	12.409	142	24909	0.394	ng/ul	92
8) 1-Methylnaphthalene	12.629	142	21173	0.330	ng/ul	99
10) Acenaphthylene	14.298	152	28175	0.371	ng/ul	99
11) Acenaphthene	14.636	153	7958	0.121	ng/ul	99
12) Fluorene	15.621	166	8925	0.120	ng/ul#	97
15) Phenanthrene	17.356	178	323982	3.092	ng/ul	99
16) Anthracene	17.445	178	32821	0.375	ng/ul	99
19) Fluoranthene	19.364	202	432129	6.099	ng/ul	98
20) Pyrene	19.727	202	329585	4.461	ng/ul	97
21) Benzo(a)anthracene	21.470	228	100707	1.565	ng/ul	98
22) Chrysene	21.522	228	122421	1.772	ng/ul	98
24) Benzo(b)fluoranthene	23.150	252	177050	2.368	ng/ul	88
25) Benzo(k)fluoranthene	23.197	252	54735m	0.751	ng/ul	
26) Benzo(a)pyrene	23.776	252	110952	1.829	ng/ul#	79
27) Indeno(1,2,3-cd)pyrene	26.372	276	97027	1.129	ng/ul#	92
28) Dibenzo(a,h)anthracene	26.382	278	19968	0.288	ng/ul#	93
29) Benzo(g,h,i)perylene	27.144	276	92785	1.225	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036986.D
Acq On : 12 Oct 2022 16:30
Operator : CG/JU
Sample : N5024-04DL 5X
Misc :
ALS Vial : 90 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0BF1DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022


Quant Time: Oct 12 23:11:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

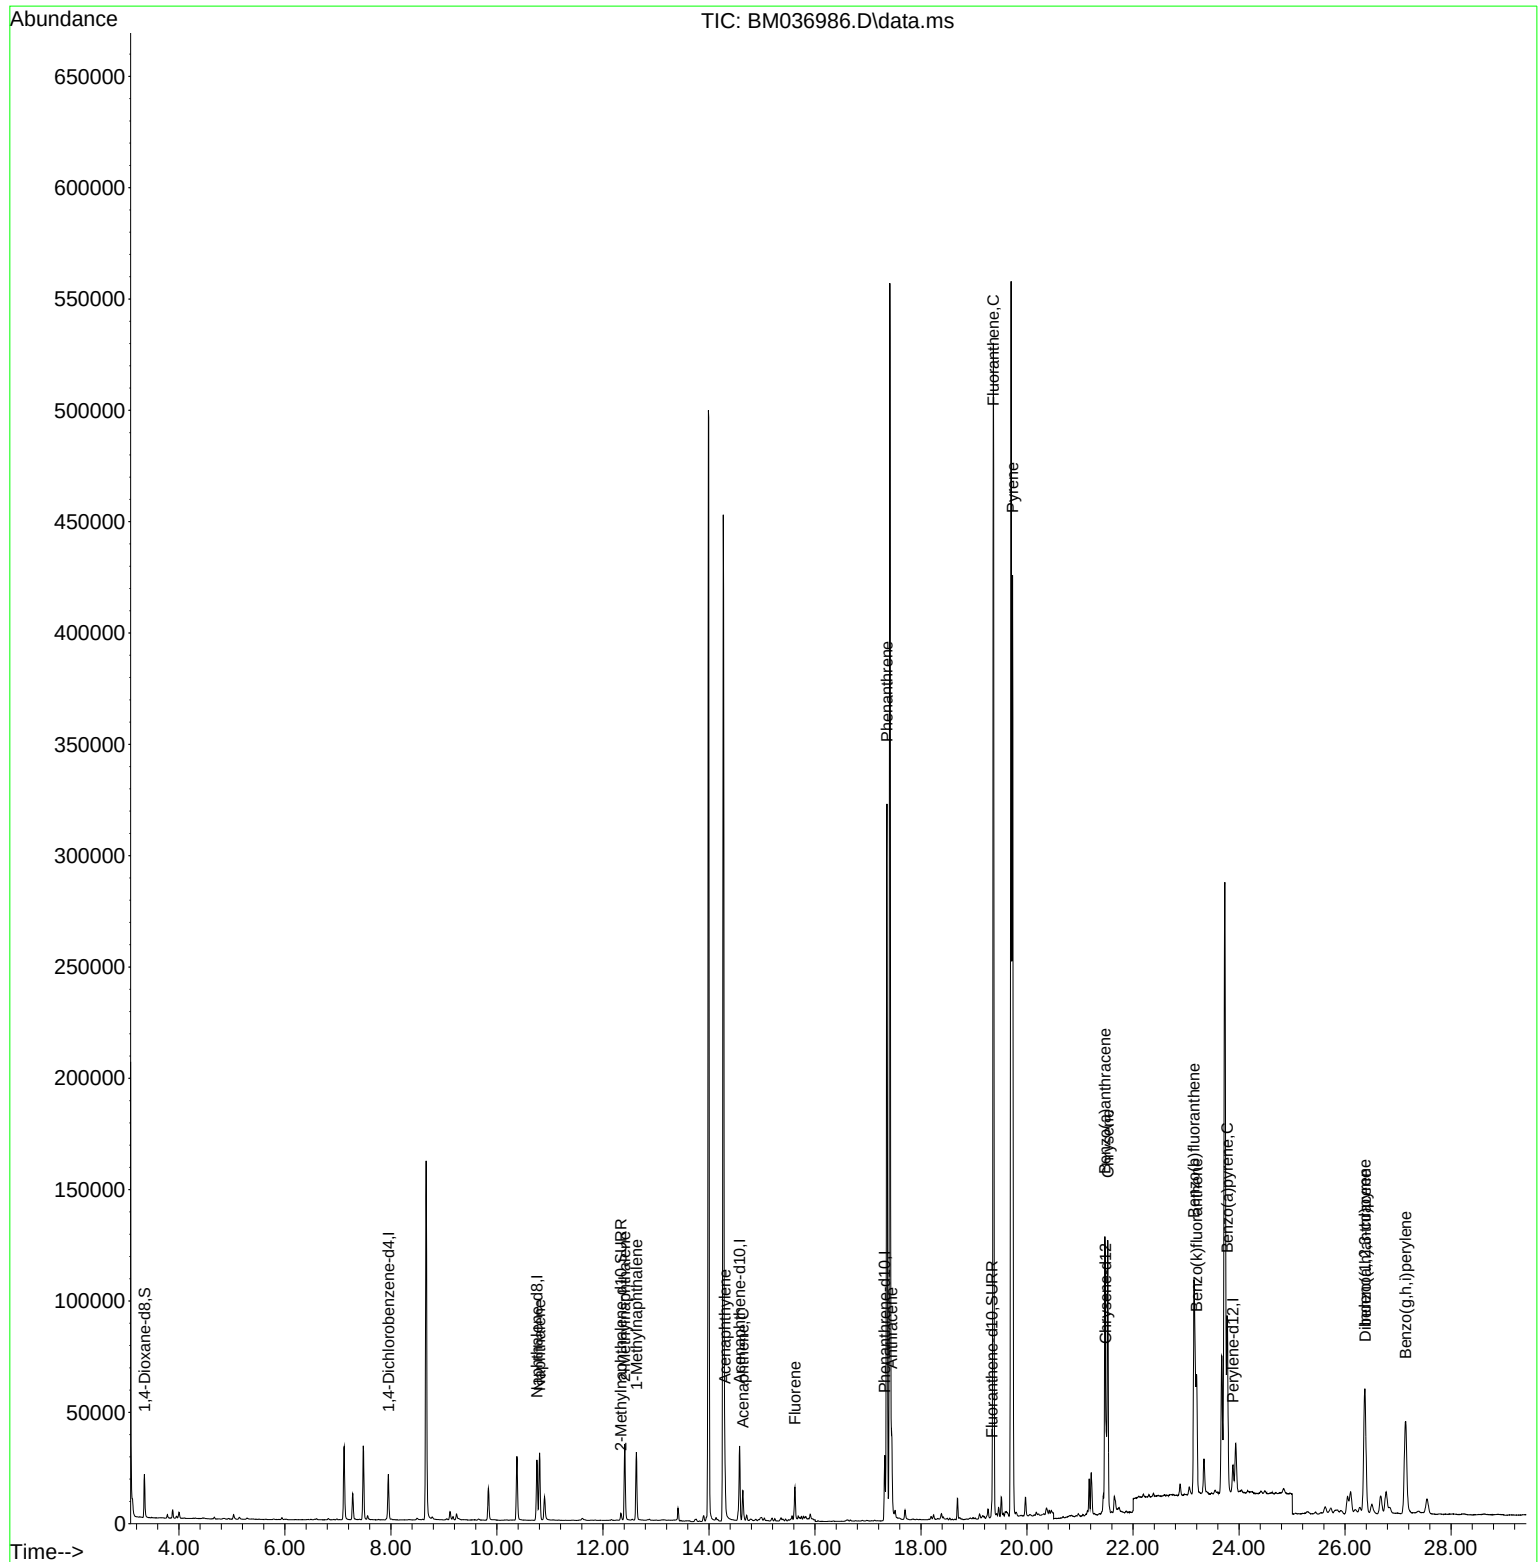

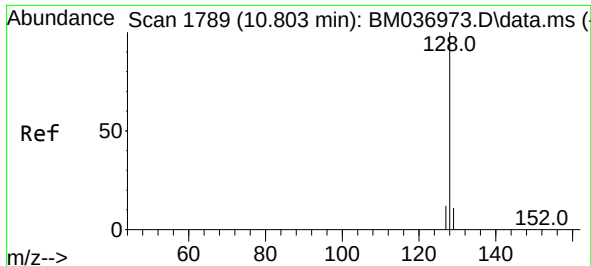

#5
Naphthalene
Concen: 0.395 ng/ul
RT: 10.803 min Scan# 1789
Delta R.T. 0.000 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:128 Resp: 40814
Ion Ratio Lower Upper
128 100
129 11.4 10.2 15.2
127 13.2 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

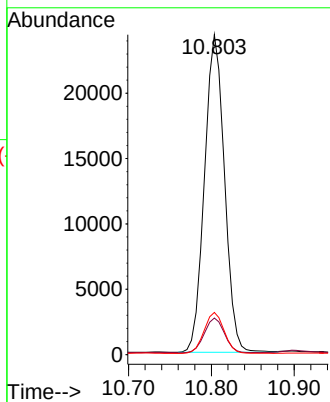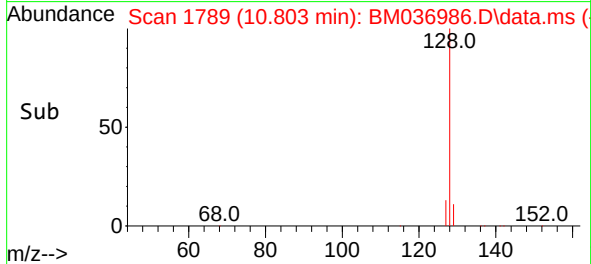

#7
2-Methylnaphthalene
Concen: 0.394 ng/ul
RT: 12.409 min Scan# 2081
Delta R.T. -0.005 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:142 Resp: 24909
Ion Ratio Lower Upper
142 100
141 88.5 77.4 116.0

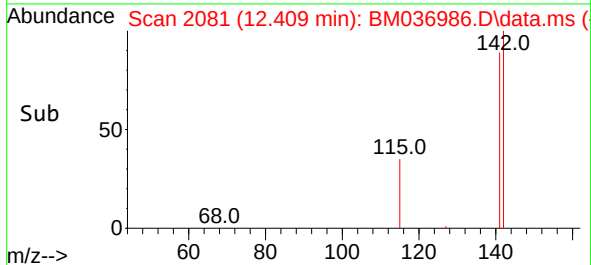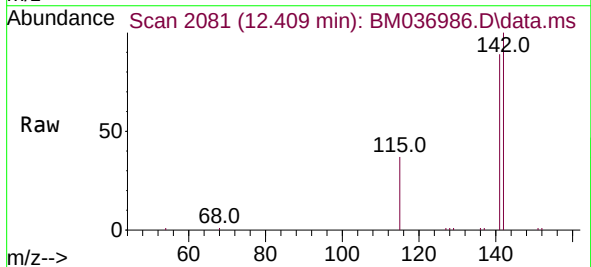

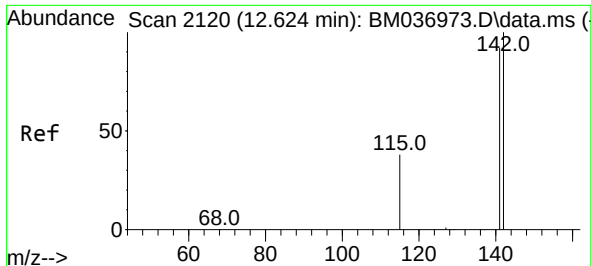

#8
1-Methylnaphthalene
Concen: 0.330 ng/ul
RT: 12.629 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:142 Resp: 21173
Ion Ratio Lower Upper
142 100
141 91.2 74.1 111.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

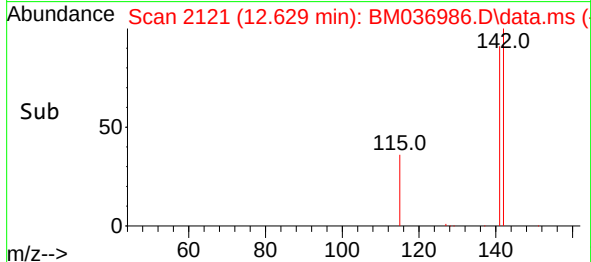

#10
Acenaphthylene
Concen: 0.371 ng/ul
RT: 14.298 min Scan# 2455
Delta R.T. 0.001 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:152 Resp: 28175
Ion Ratio Lower Upper
152 100
151 20.3 16.6 24.8
153 14.9 11.4 17.0

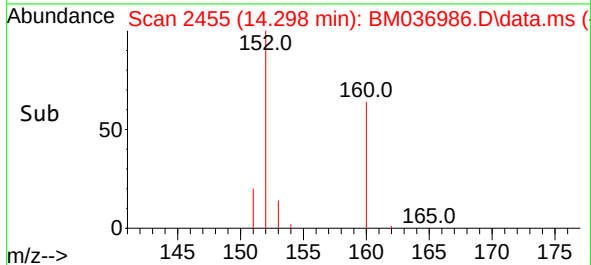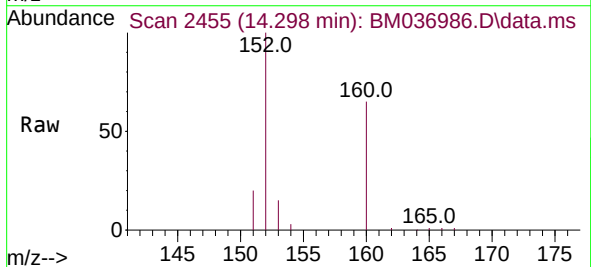

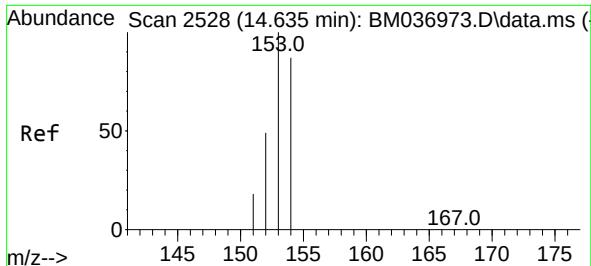

#11
Acenaphthene
Concen: 0.121 ng/ul
RT: 14.636 min Scan# 2528
Delta R.T. -0.004 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:153 Resp: 7958
Ion Ratio Lower Upper
153 100
152 51.4 40.2 60.4
154 86.9 69.7 104.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

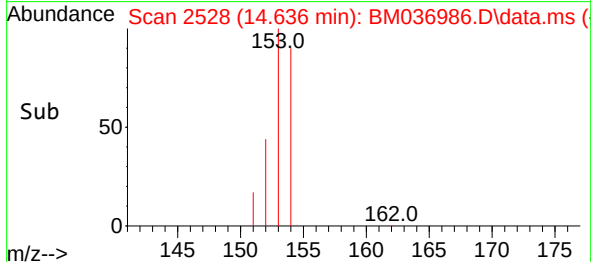

#12
Fluorene
Concen: 0.120 ng/ul
RT: 15.621 min Scan# 2741
Delta R.T. 0.001 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:166 Resp: 8925
Ion Ratio Lower Upper
166 100
165 100.2 78.9 118.3
167 17.9 11.3 16.9#

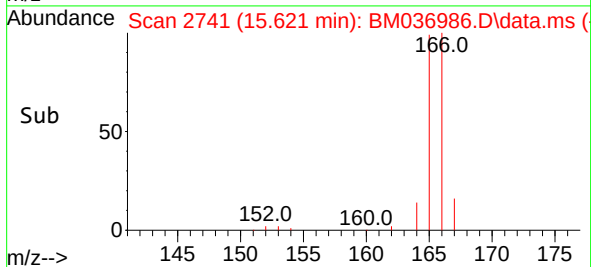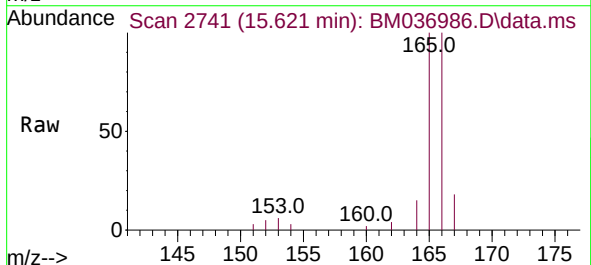

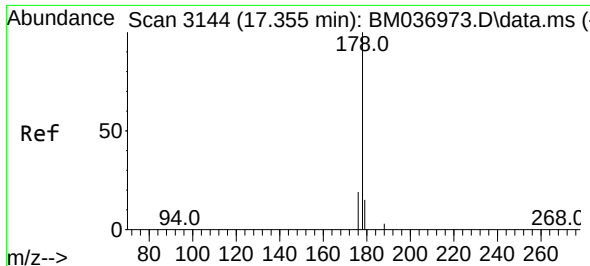

#15
Phenanthrene
Concen: 3.092 ng/ul
RT: 17.356 min Scan# 3144
Delta R.T. 0.001 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL

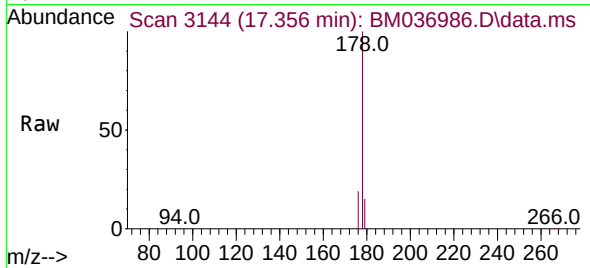

Tgt Ion:178 Resp: 323982
Ion Ratio Lower Upper
178 100
179 15.4 13.0 19.6
176 19.1 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

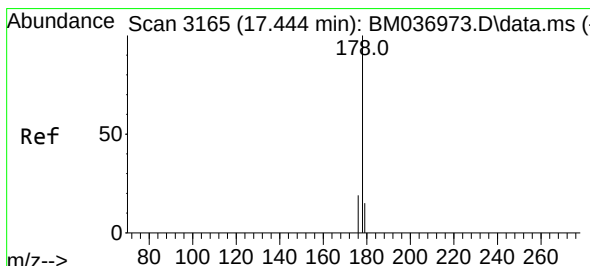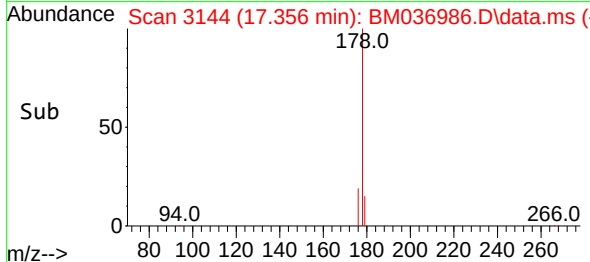

#16
Anthracene
Concen: 0.375 ng/ul
RT: 17.445 min Scan# 3165
Delta R.T. -0.003 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:178 Resp: 32821
Ion Ratio Lower Upper
178 100
179 16.9 13.6 20.4
176 19.2 15.6 23.4

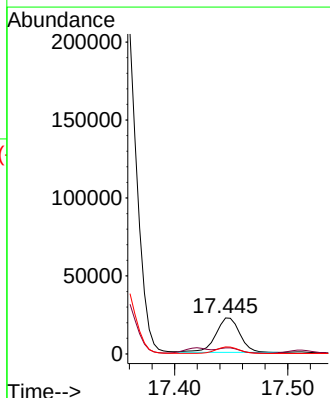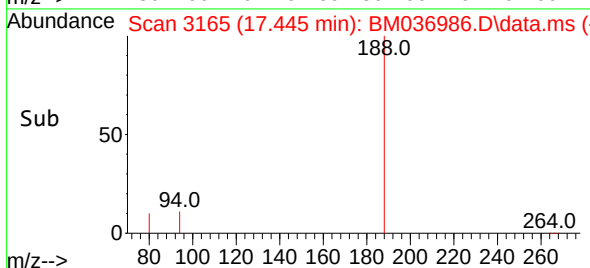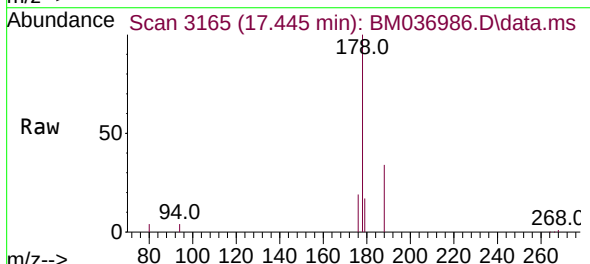



#19
Fluoranthene
Concen: 6.099 ng/u1
RT: 19.364 min Scan# 3601
Delta R.T. 0.001 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL




Tgt Ion:202 Resp: 432129
Ion Ratio Lower Upper
202 100
101 12.1 10.1 15.1
100 8.9 7.9 11.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

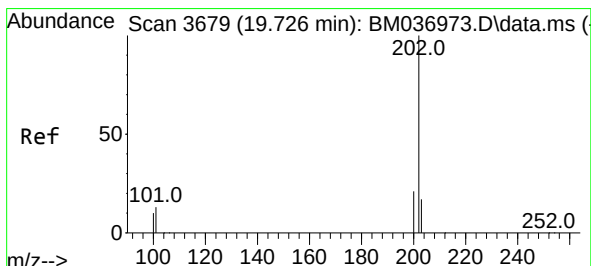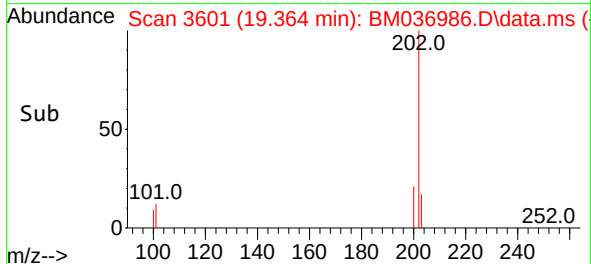


#20
Pyrene
Concen: 4.461 ng/u1
RT: 19.727 min Scan# 3679
Delta R.T. 0.001 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30

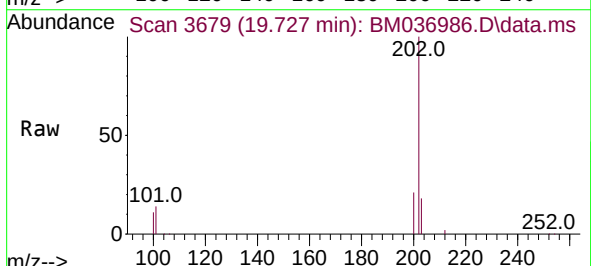


Tgt Ion:202 Resp: 329585
Ion Ratio Lower Upper
202 100
101 13.9 12.0 18.0
100 11.1 9.8 14.6

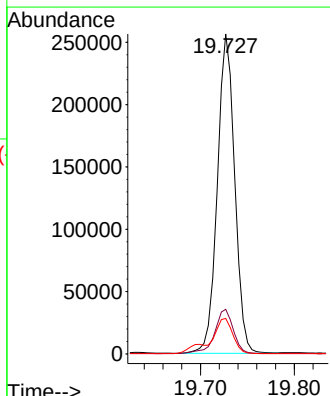

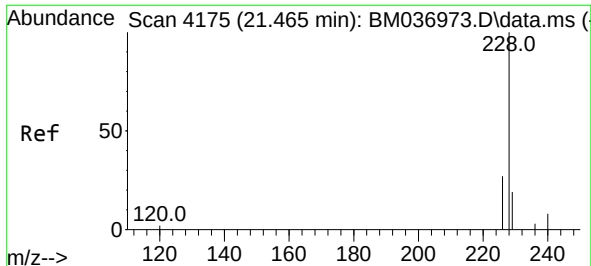

#21
Benzo(a)anthracene
Concen: 1.565 ng/ul
RT: 21.470 min Scan# 4177
Delta R.T. 0.002 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL




Tgt Ion:228 Resp: 100707
Ion Ratio Lower Upper
228 100
229 21.1 16.2 24.2
226 29.0 22.5 33.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

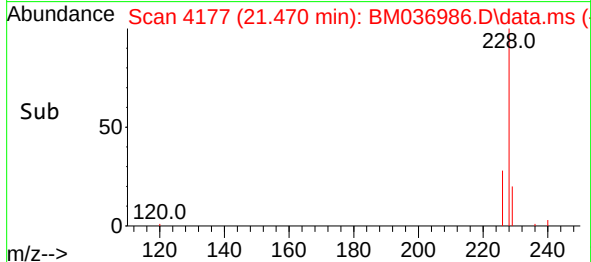


#22
Chrysene
Concen: 1.772 ng/ul
RT: 21.522 min Scan# 4195
Delta R.T. 0.002 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30

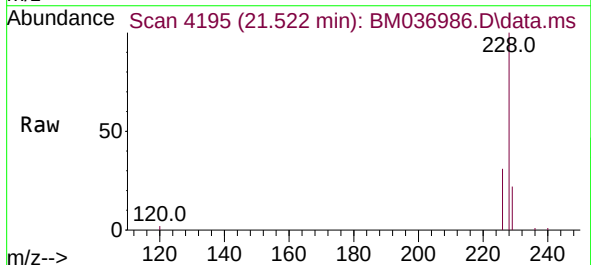


Tgt Ion:228 Resp: 122421
Ion Ratio Lower Upper
228 100
226 30.6 24.6 37.0
229 22.4 16.4 24.6

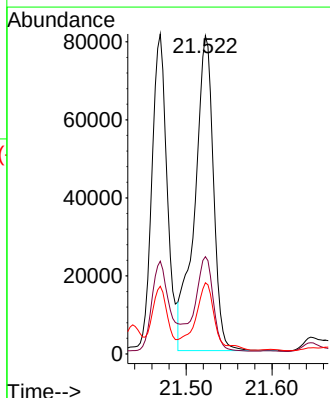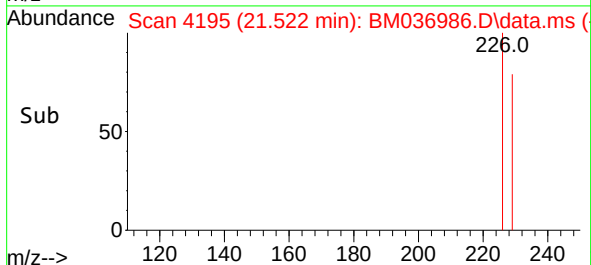

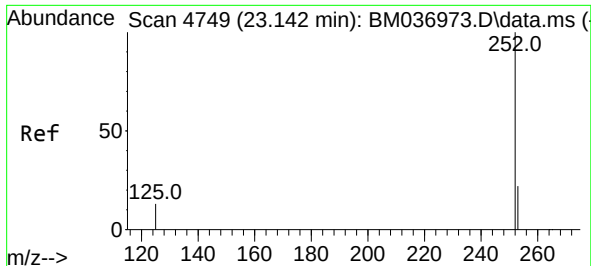

#24
Benzo(b)fluoranthene
Concen: 2.368 ng/ul
RT: 23.150 min Scan# 4752
Delta R.T. 0.005 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:252 Resp: 177050
Ion Ratio Lower Upper
252 100
253 24.2 0.0 61.4
125 16.0 0.0 42.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

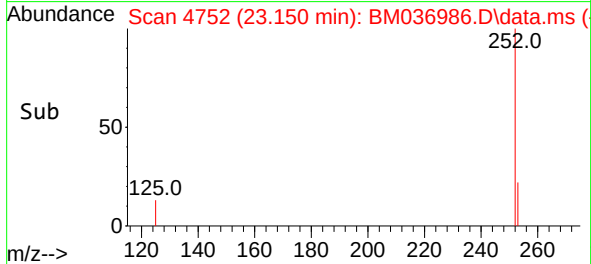

#25
Benzo(k)fluoranthene
Concen: 0.751 ng/ul m
RT: 23.197 min Scan# 4768
Delta R.T. 0.002 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:252 Resp: 54735
Ion Ratio Lower Upper
252 100
253 26.5 25.2 37.8
125 19.5 18.3 27.5

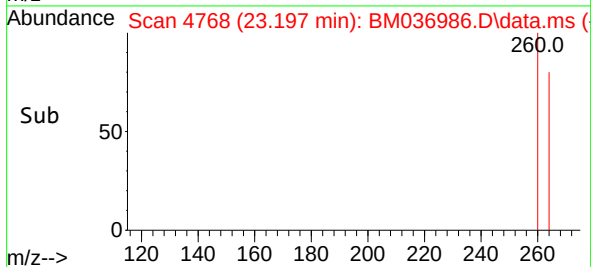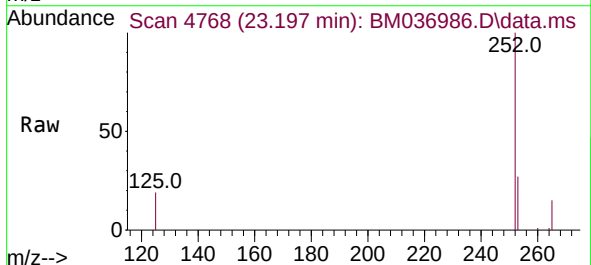

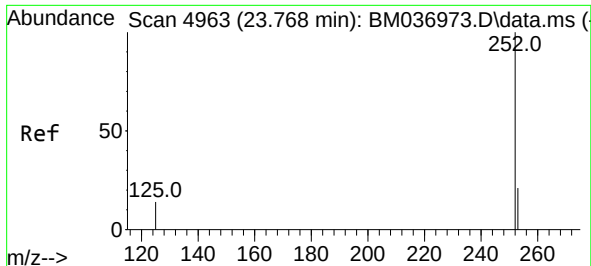

#26
Benzo(a)pyrene
Concen: 1.829 ng/ul
RT: 23.776 min Scan# 4963
Delta R.T. 0.005 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:252 Resp: 110952
Ion Ratio Lower Upper
252 100
253 24.9 29.7 44.5
125 17.6 23.6 35.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

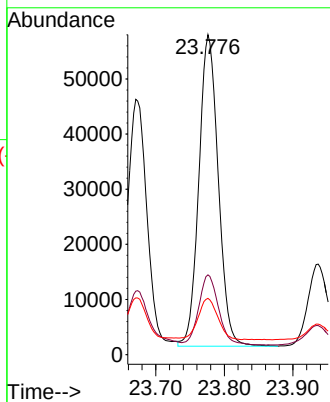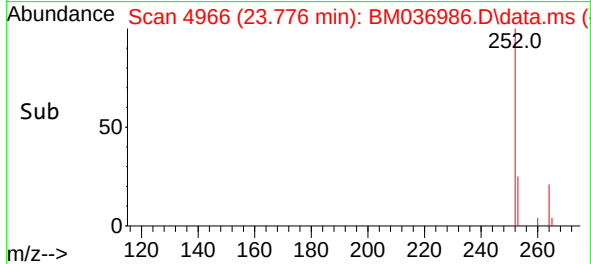

#27
Indeno(1,2,3-cd)pyrene
Concen: 1.129 ng/ul
RT: 26.372 min Scan# 5794
Delta R.T. 0.009 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30


Tgt Ion:276 Resp: 97027
Ion Ratio Lower Upper
276 100
138 25.5 23.9 35.9
227 0.4 0.1 0.1

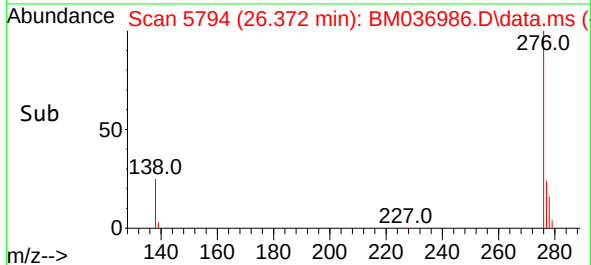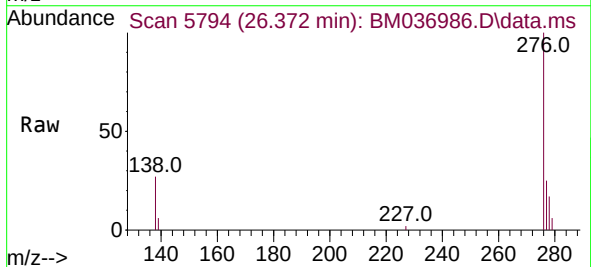

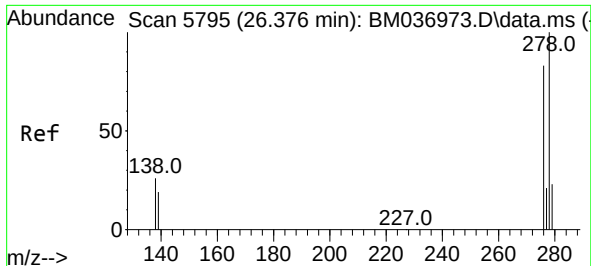

#28
Dibenzo(a,h)anthracene
Concen: 0.288 ng/ul
RT: 26.382 min Scan# 51
Delta R.T. 0.003 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30




Instrument :
BNA_M
ClientSampleId :
C0BF1DL



Tgt Ion:278 Resp: 19968
Ion Ratio Lower Upper
278 100
139 32.0 19.8 29.6
279 35.7 27.7 41.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

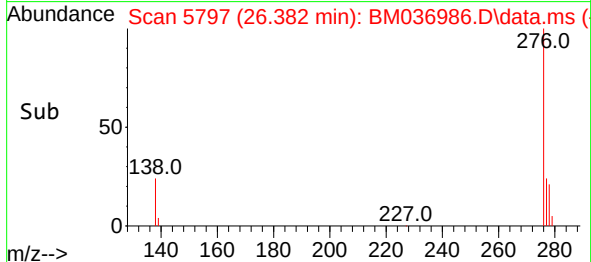

#29
Benzo(g,h,i)perylene
Concen: 1.225 ng/ul
RT: 27.144 min Scan# 6024
Delta R.T. 0.016 min
Lab File: BM036986.D
Acq: 12 Oct 2022 16:30

Tgt Ion:276 Resp: 92785
Ion Ratio Lower Upper
276 100
138 28.0 23.4 35.0
277 25.0 21.0 31.4

