

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036999.D
 Acq On : 13 Oct 2022 00:56
 Operator : CG/JU
 Sample : N4980-09
 Misc :
 ALS Vial : 104 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y7

Quant Time: Oct 13 01:57:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	8808	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	31122	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	18023	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	28478	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.481	240	16214	0.400	ng/ul	# 0.00
23) Perylene-d12	23.878	264	16767	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	46342	3.731	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	14524	0.309	ng/ul	0.00
18) Fluoranthene-d10	19.332	212	21154	0.436	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.382	88	381424	31.413	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036999.D
Acq On : 13 Oct 2022 00:56
Operator : CG/JU
Sample : N4980-09
Misc :
ALS Vial : 104 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Y7


Quant Time: Oct 13 01:57:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

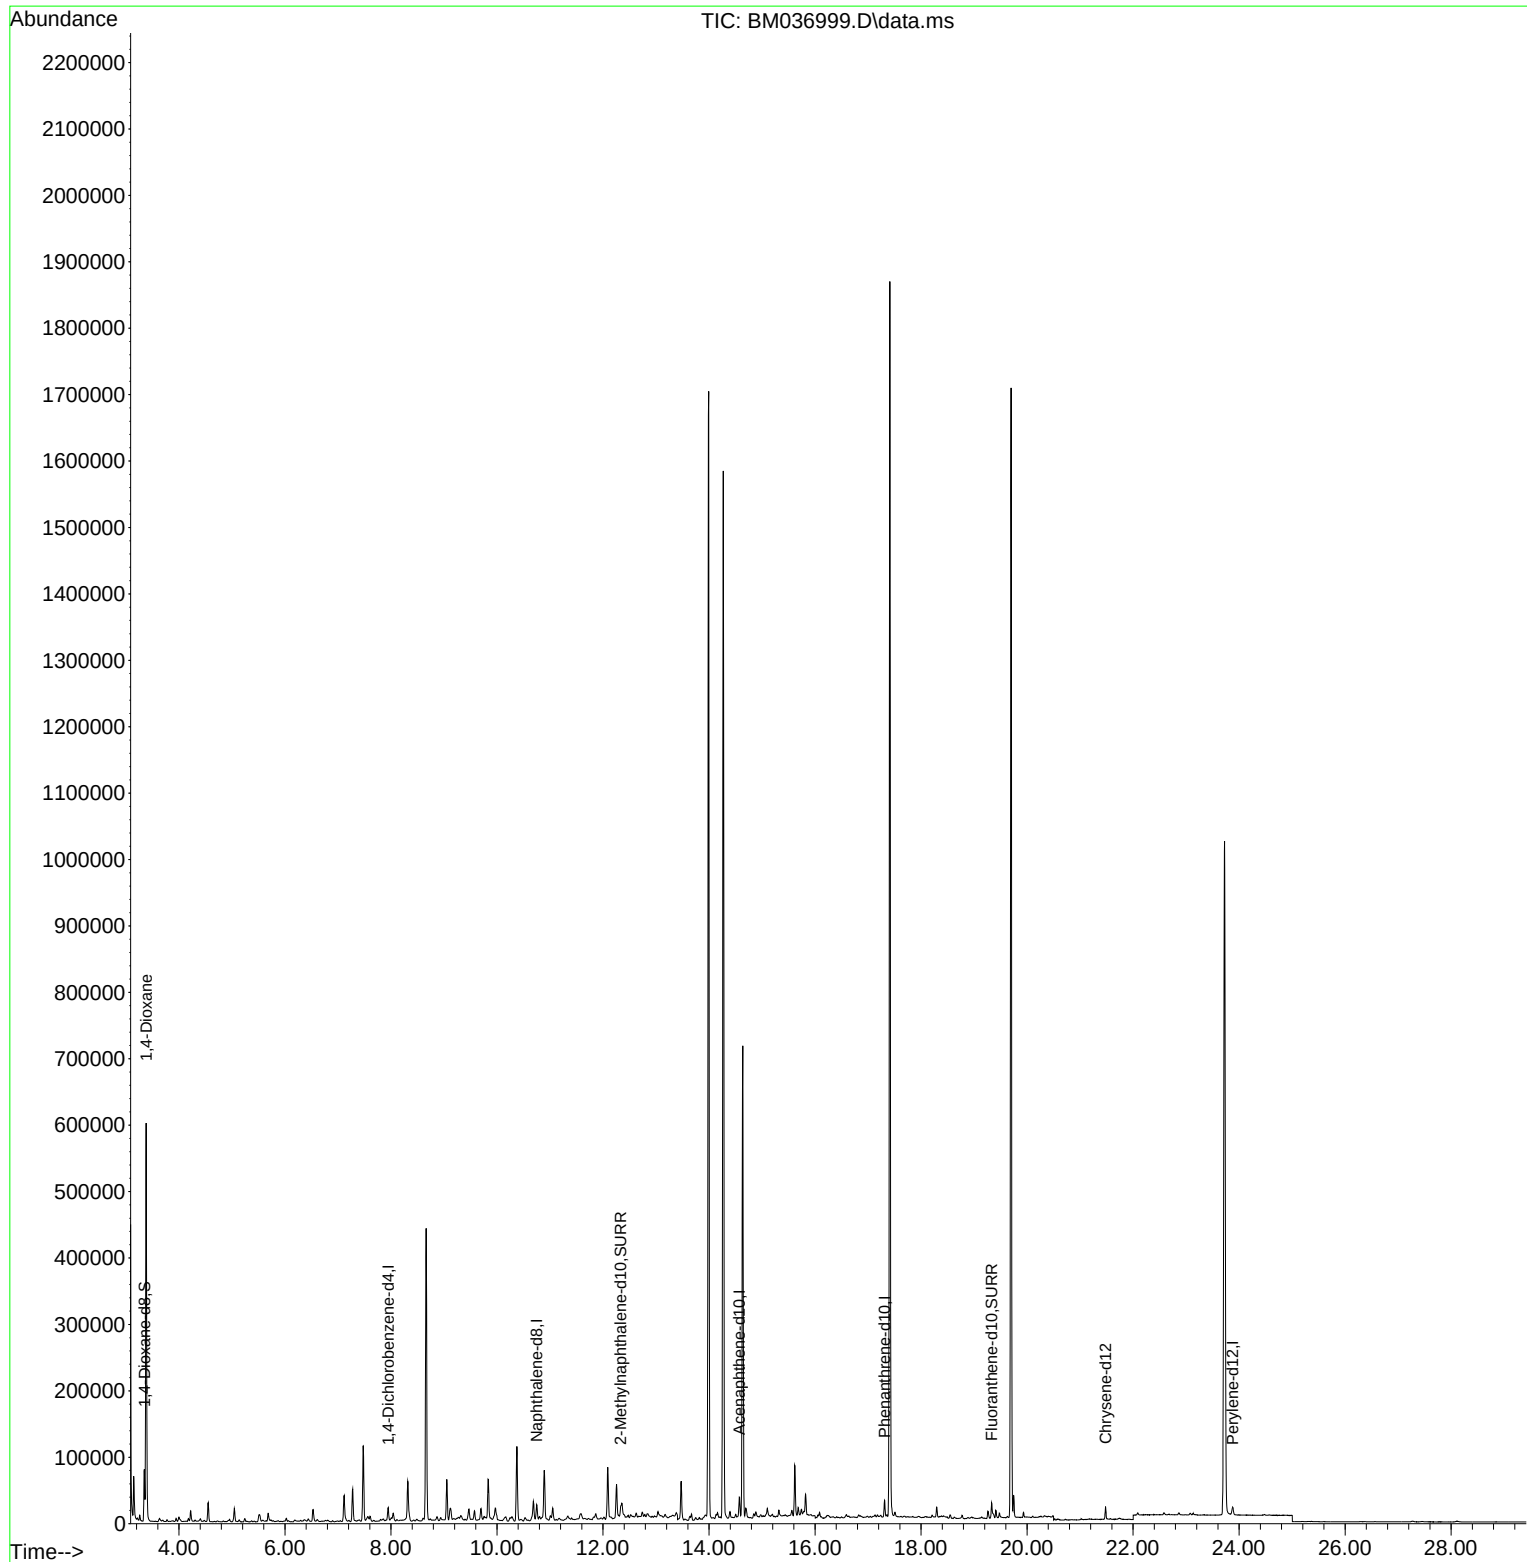

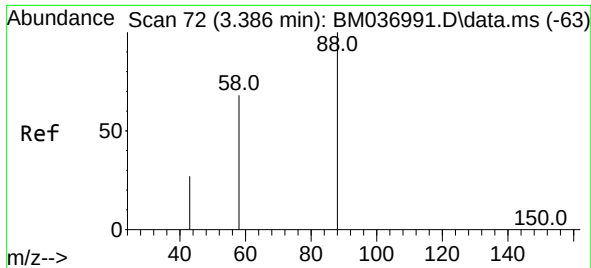

#2
 1,4-Dioxane
 Concen: 31.413 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM036999.D
 Acq: 13 Oct 2022 00:56

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y7

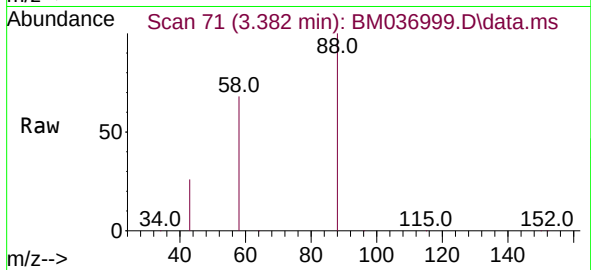

Tgt Ion: 88 Resp: 381424

Ion	Ratio	Lower	Upper
88	100		
43	26.2	37.8	56.6#
58	68.0	42.6	63.8#

