

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM037001.D
 Acq On : 13 Oct 2022 02:08
 Operator : CG/JU
 Sample : N4980-07
 Misc :
 ALS Vial : 106 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y3

Quant Time: Oct 13 03:48:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	9487	0.400	ng/ul	0.00
4) Naphthalene-d8	10.749	136	33927	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.575	164	20010	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.309	188	33272	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.482	240	17599	0.400	ng/ul	# 0.00
23) Perylene-d12	23.876	264	17316	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	37650	2.814	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	10706	0.209	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	16845	0.320	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.382	88	294672	22.531	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM037001.D
Acq On : 13 Oct 2022 02:08
Operator : CG/JU
Sample : N4980-07
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Y3


Quant Time: Oct 13 03:48:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

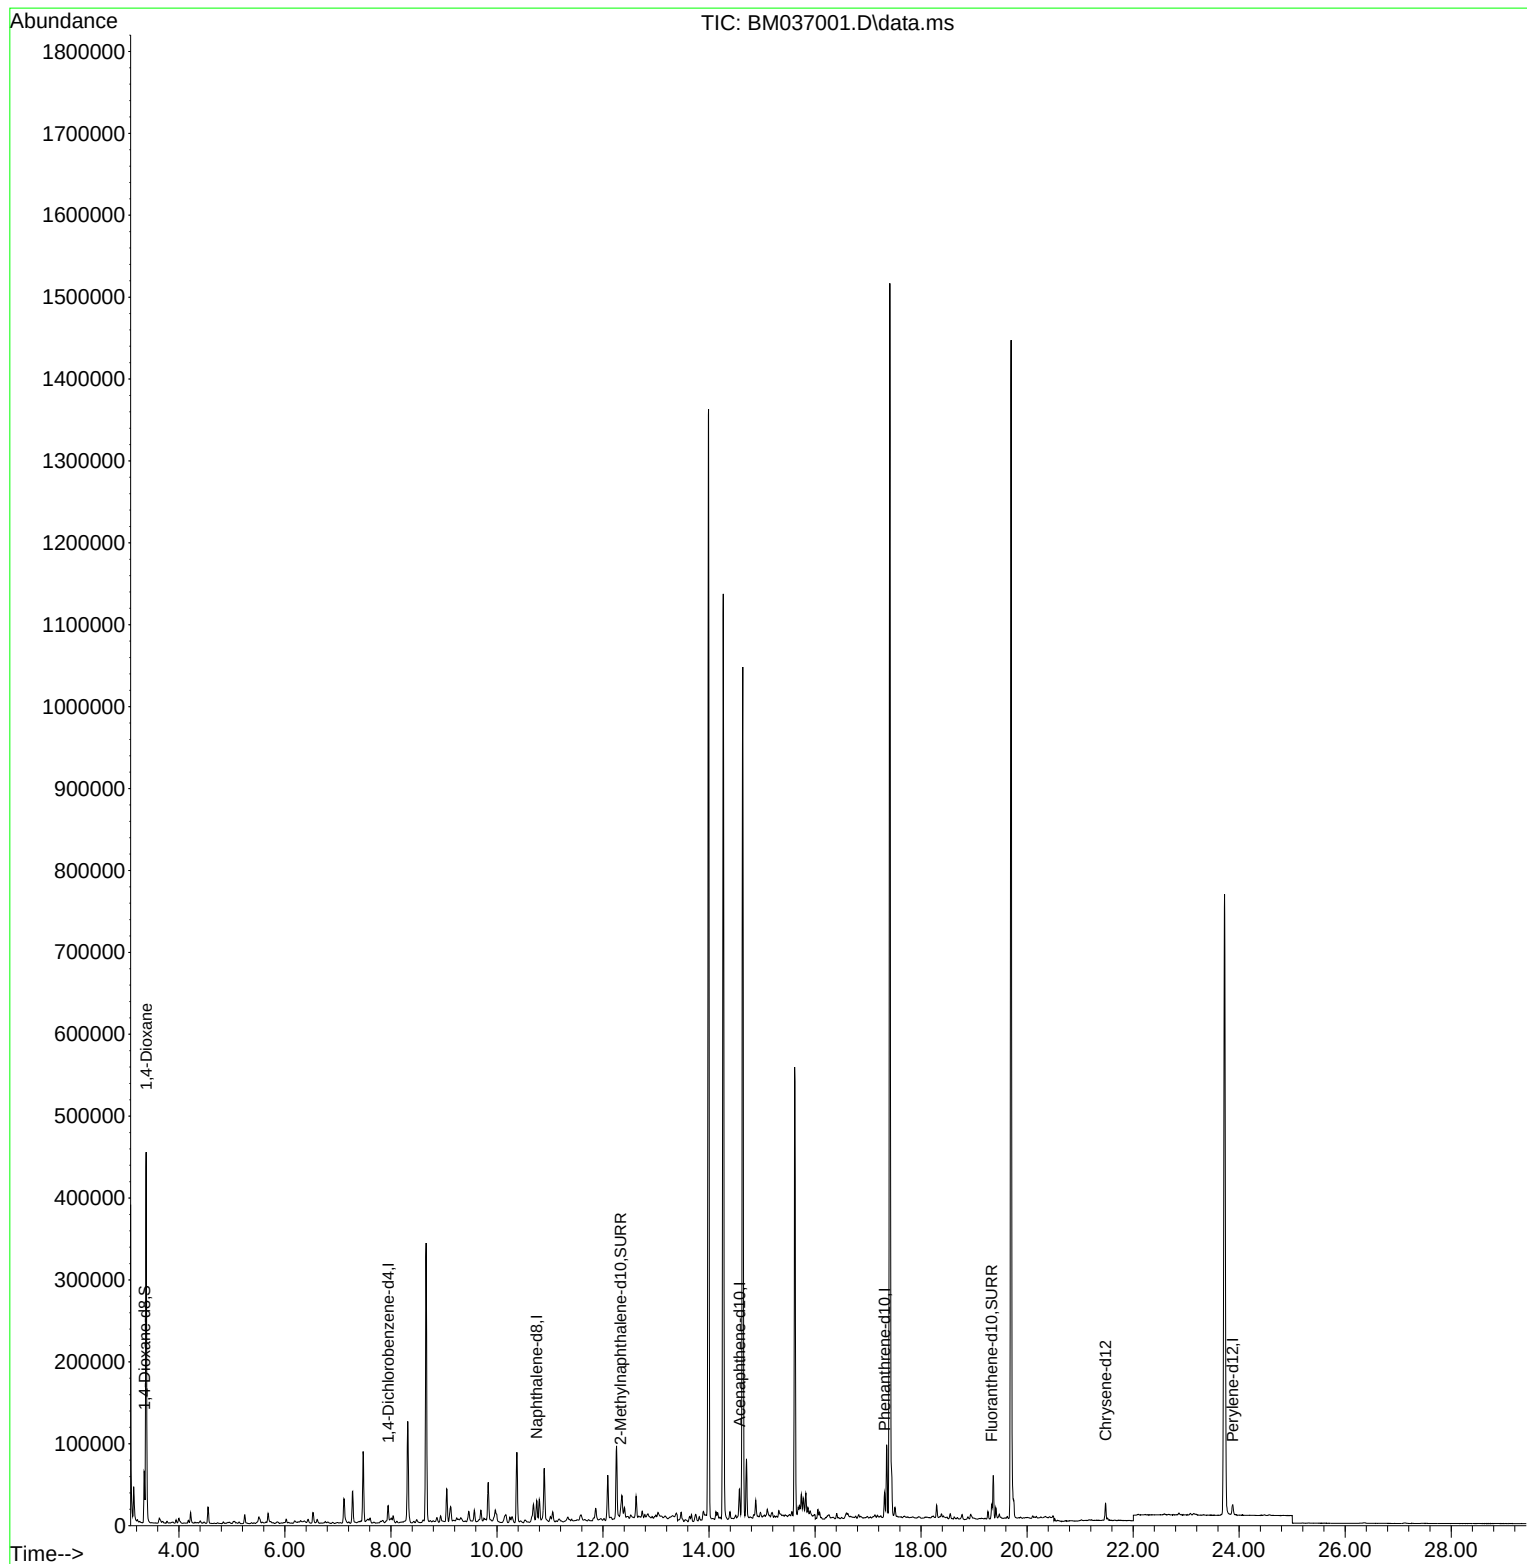

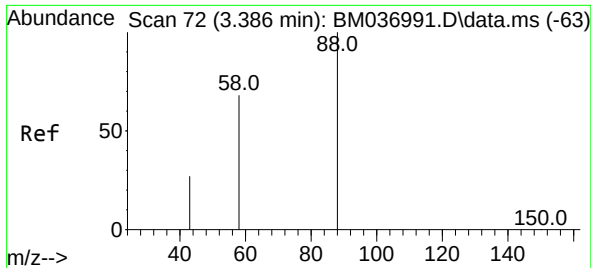

#2
 1,4-Dioxane
 Concen: 22.531 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM037001.D
 Acq: 13 Oct 2022 02:08

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y3

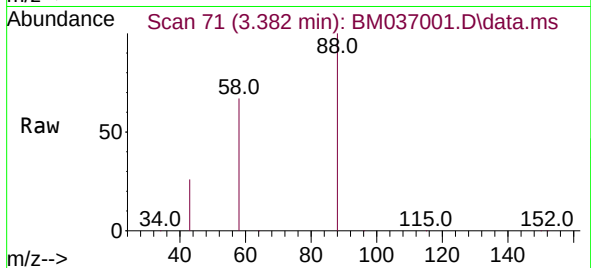

Tgt Ion: 88 Resp: 294672
 Ion Ratio Lower Upper
 88 100
 43 26.0 37.8 56.6#
 58 67.3 42.6 63.8#

