

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM037003.D
 Acq On : 13 Oct 2022 03:19
 Operator : CG/JU
 Sample : N4980-10
 Misc :
 ALS Vial : 108 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y9

Quant Time: Oct 13 03:51:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	9013	0.400	ng/ul	0.00
4) Naphthalene-d8	10.749	136	32130	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.570	164	20068	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	35713	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.479	240	19912	0.400	ng/ul	# 0.00
23) Perylene-d12	23.879	264	18884	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	47725	3.755	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	14317	0.295	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	27605	0.464	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.382	88	393207	31.647	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM037003.D
Acq On : 13 Oct 2022 03:19
Operator : CG/JU
Sample : N4980-10
Misc :
ALS Vial : 108 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Y9


Quant Time: Oct 13 03:51:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

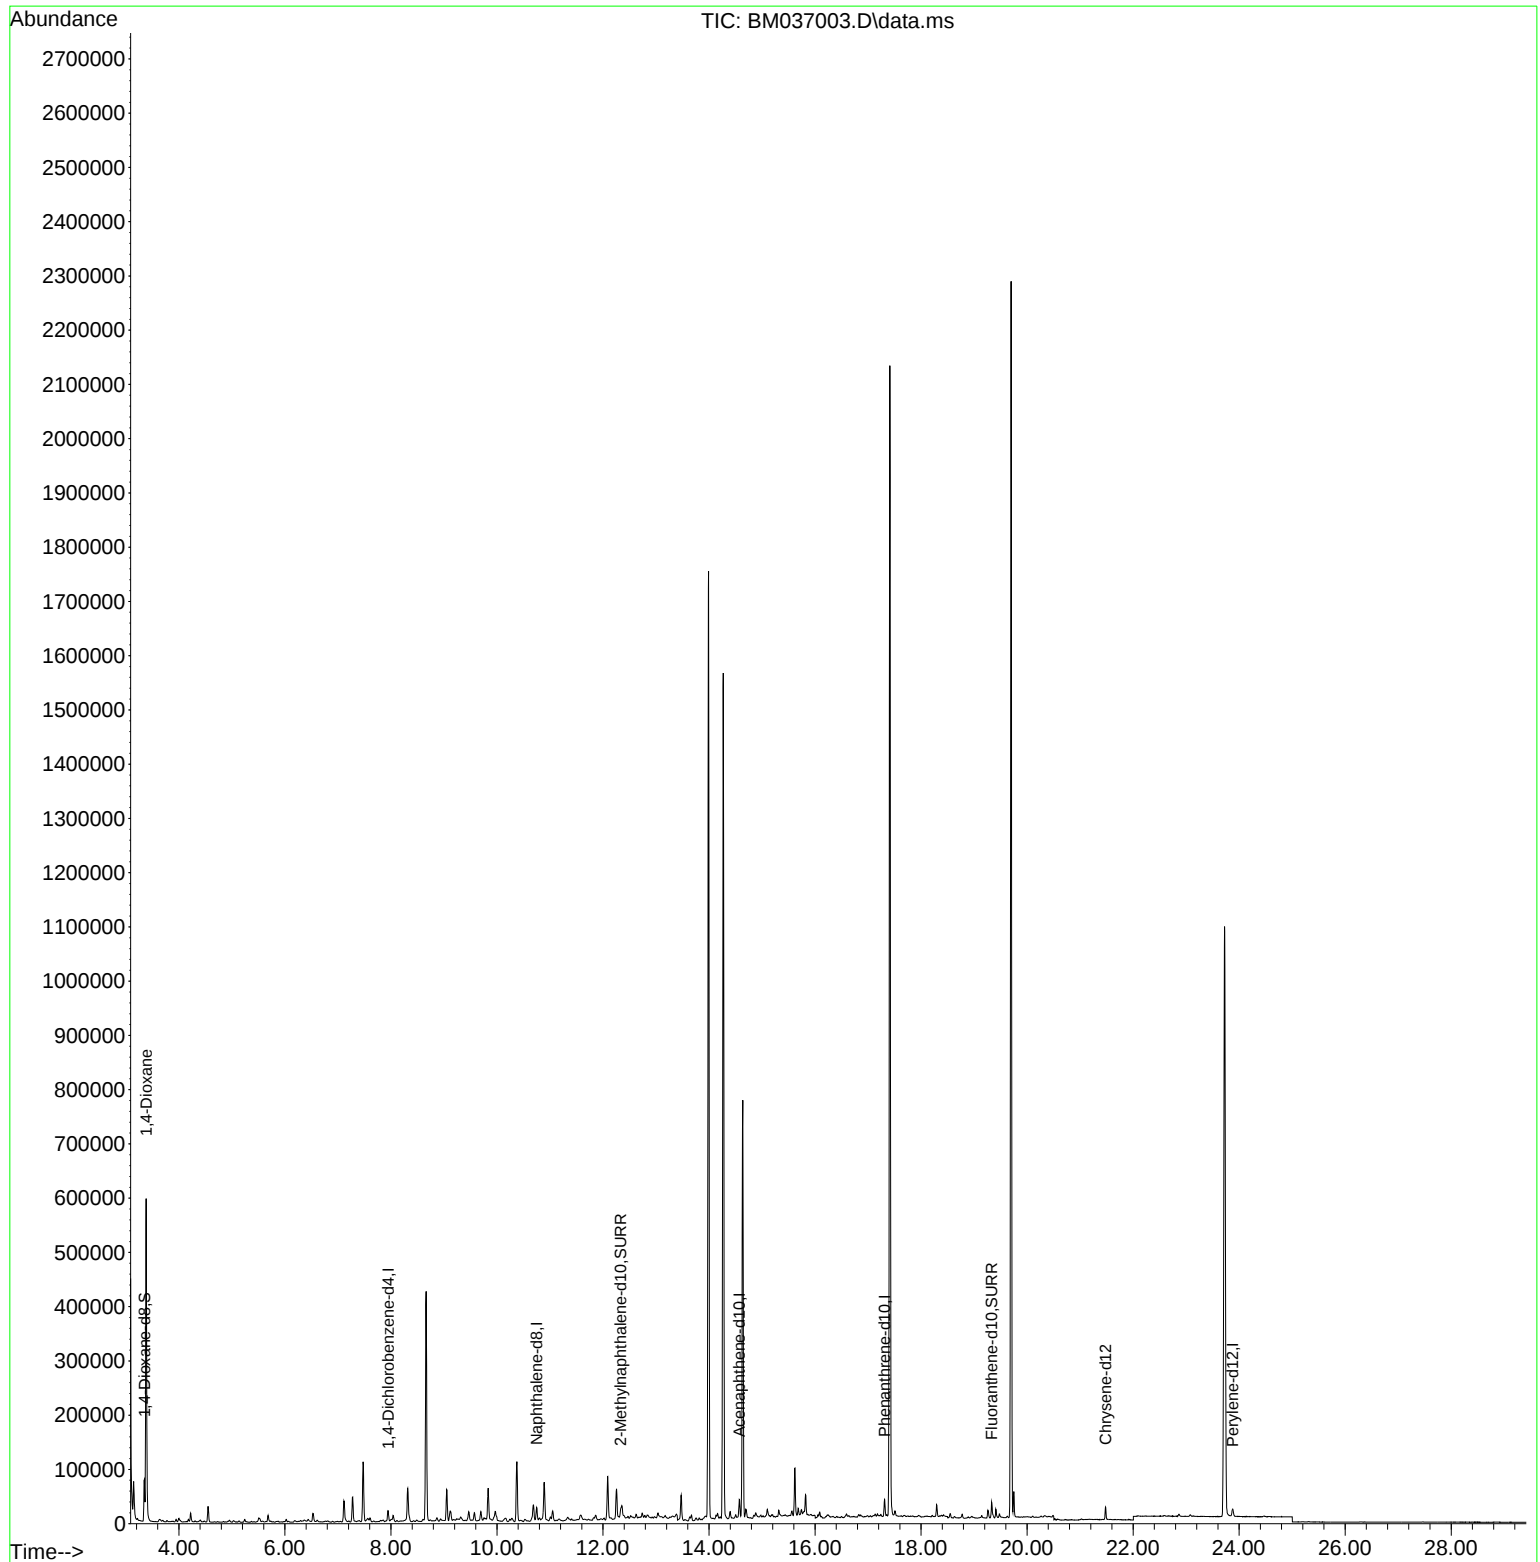

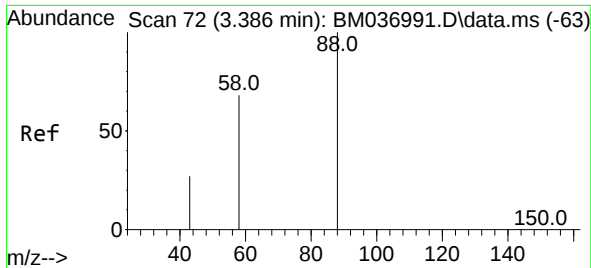

#2
 1,4-Dioxane
 Concen: 31.647 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM037003.D
 Acq: 13 Oct 2022 03:19

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y9

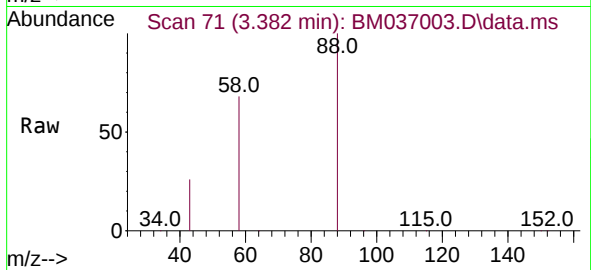

Tgt Ion: 88 Resp: 393207
 Ion Ratio Lower Upper
 88 100
 43 26.0 37.8 56.6#
 58 67.6 42.6 63.8#

