




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
Data File : BM047983.D
Acq On : 10 Oct 2024 18:11
Operator : RC/JU
Sample : PB163727BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 10 18:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 18:01:13 2024
Response via : Initial Calibration

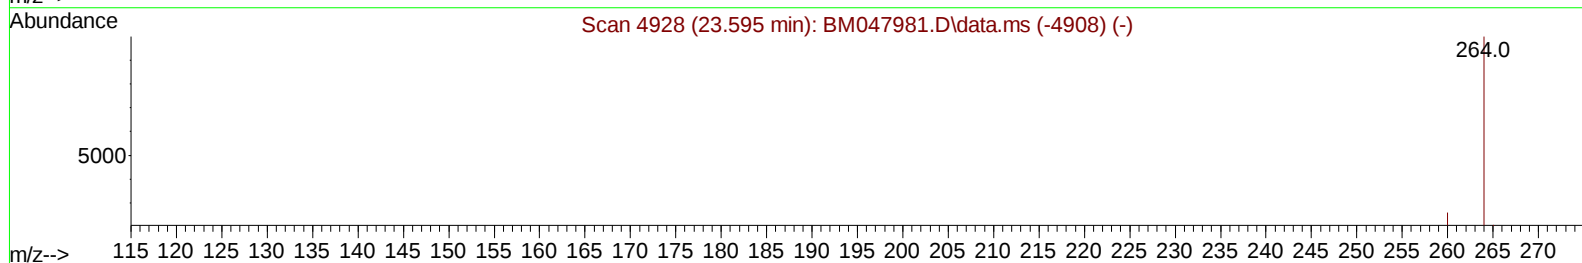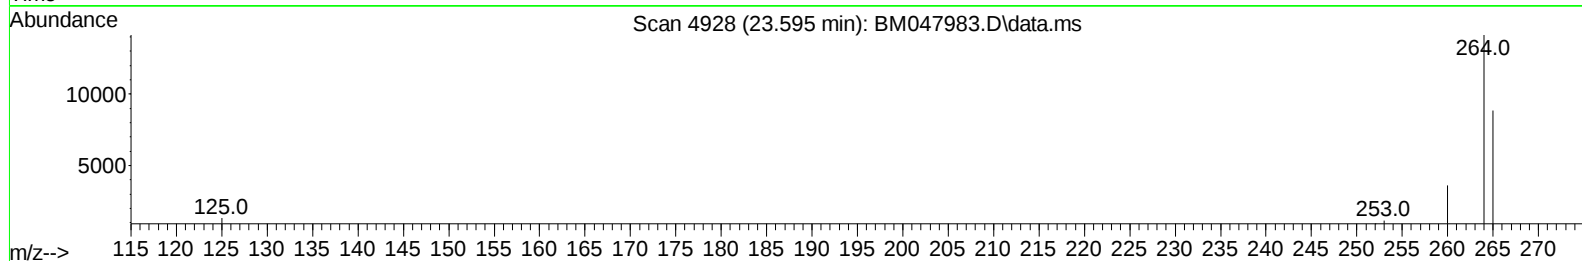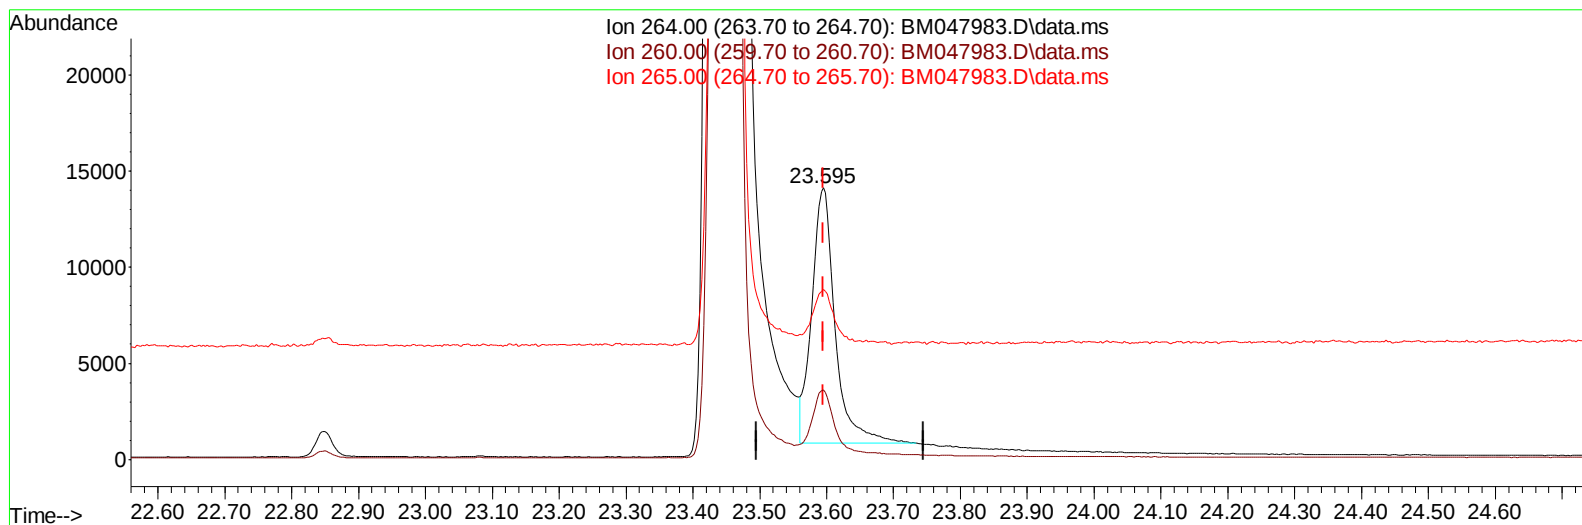

TIC: BM047983.D\data.ms

(23) Perylene-d12 (I)

23.595min (-0.000) 0.40 ng/u1

response 32115

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.64
265.00	85.70	62.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
Data File : BM047983.D
Acq On : 10 Oct 2024 18:11
Operator : RC/JU
Sample : PB163727BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 10 18:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 18:01:13 2024
Response via : Initial Calibration

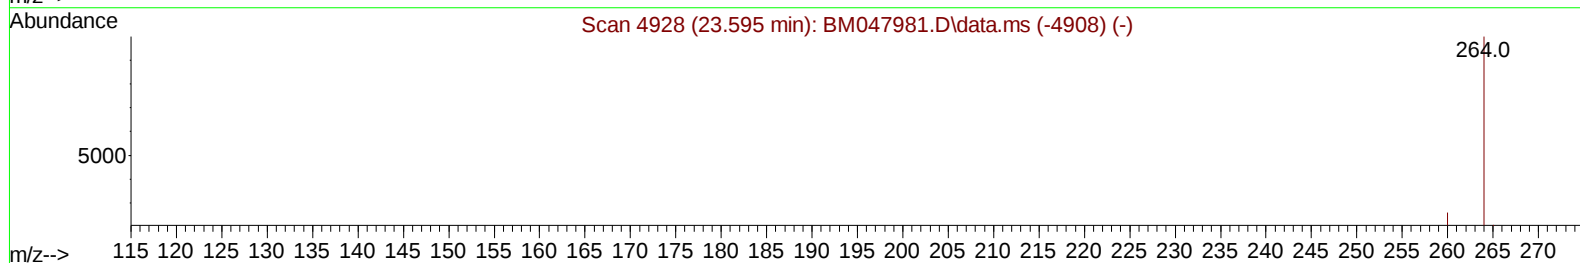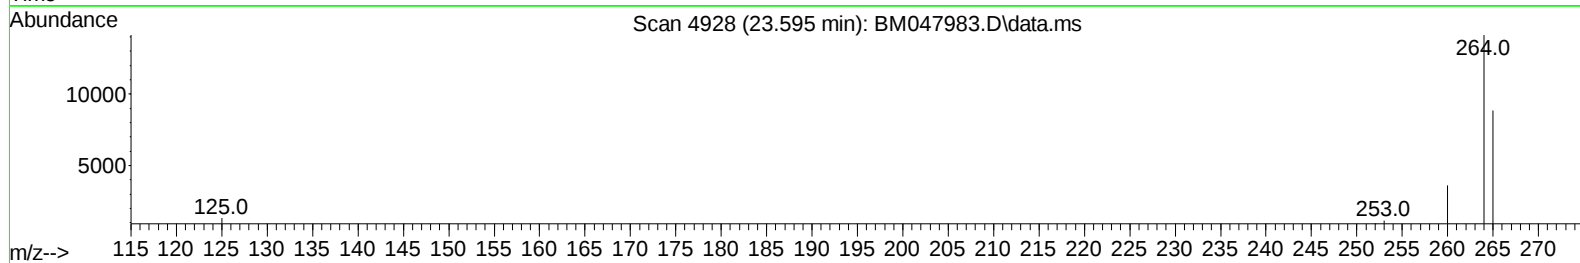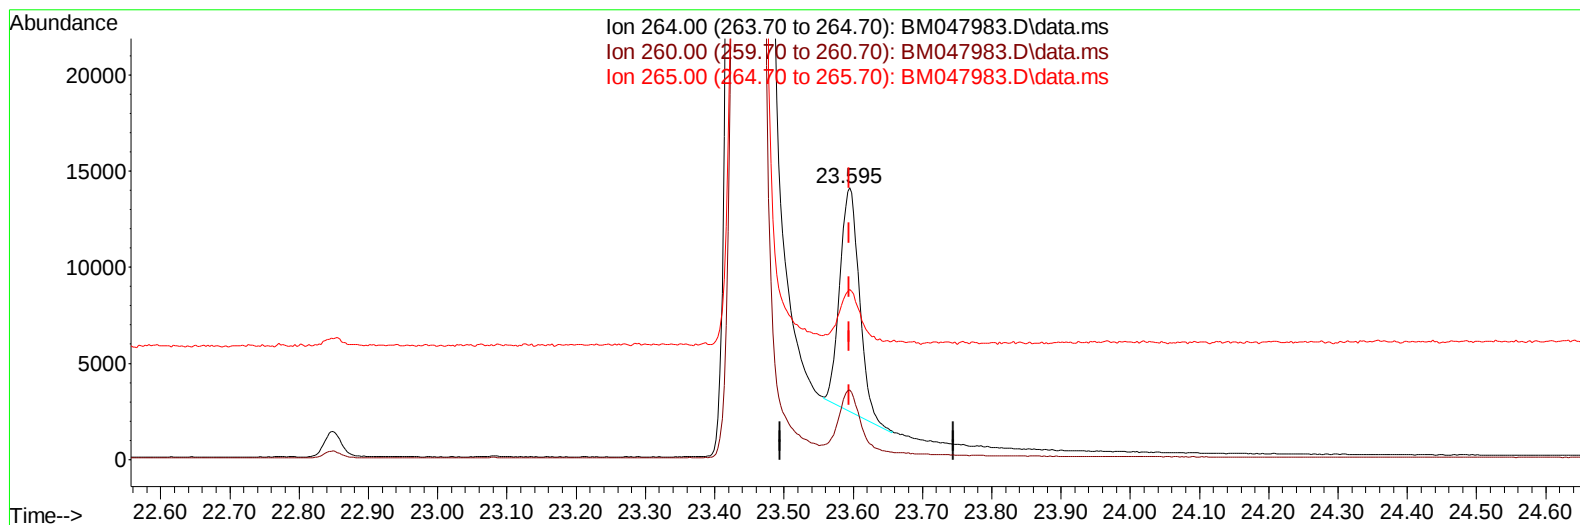

TIC: BM047983.D\data.ms

(23) Perylene-d12 (I)

23.595min (-0.000) 0.40 ng/ul m

response 22798

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.64
265.00	85.70	62.67#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM047983.D
 Acq On : 10 Oct 2024 18:11
 Operator : RC/JU
 Sample : PB163727BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK727

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 10 18:44:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	11262	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	34103	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	17494	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.158	188	34829	0.400	ng/ul	0.00
17) Chrysene-d12	21.333	240	27856	0.400	ng/ul	0.00
23) Perylene-d12	23.595	264	22798m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.273	96	66315	4.583	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	11428	0.251	ng/ul	0.00
18) Fluoranthene-d10	19.183	212	19558	0.229	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
Data File : BM047983.D
Acq On : 10 Oct 2024 18:11
Operator : RC/JU
Sample : PB163727BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Manual IntegrationsAPPROVED

Quant Time: Oct 10 18:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 18:01:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :mohammad ahmed 10/14/2024

