

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :

BNA_M




ClientSampleId :

SBLK719

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

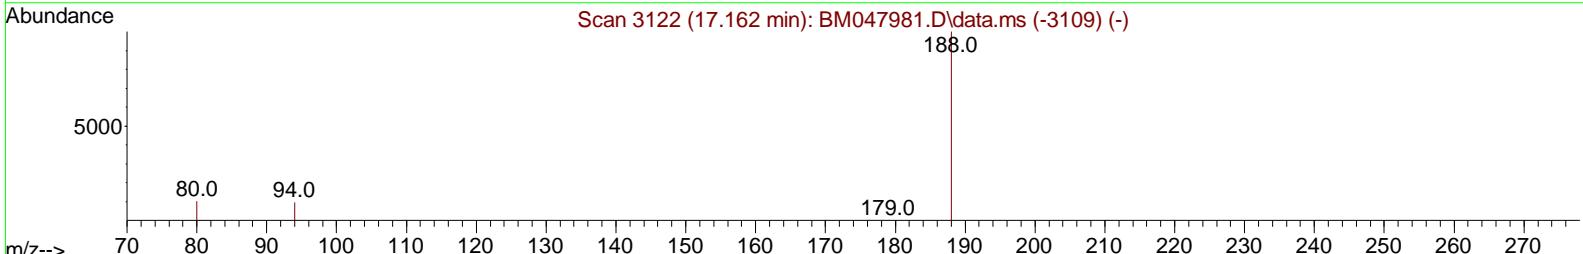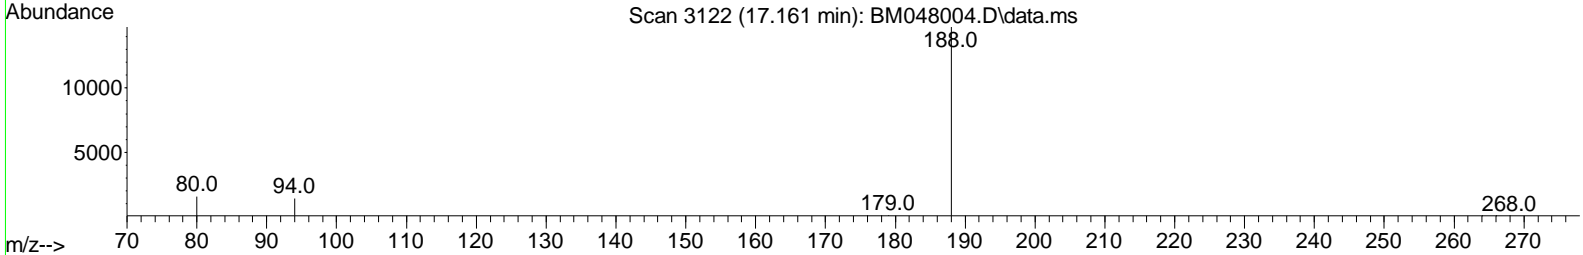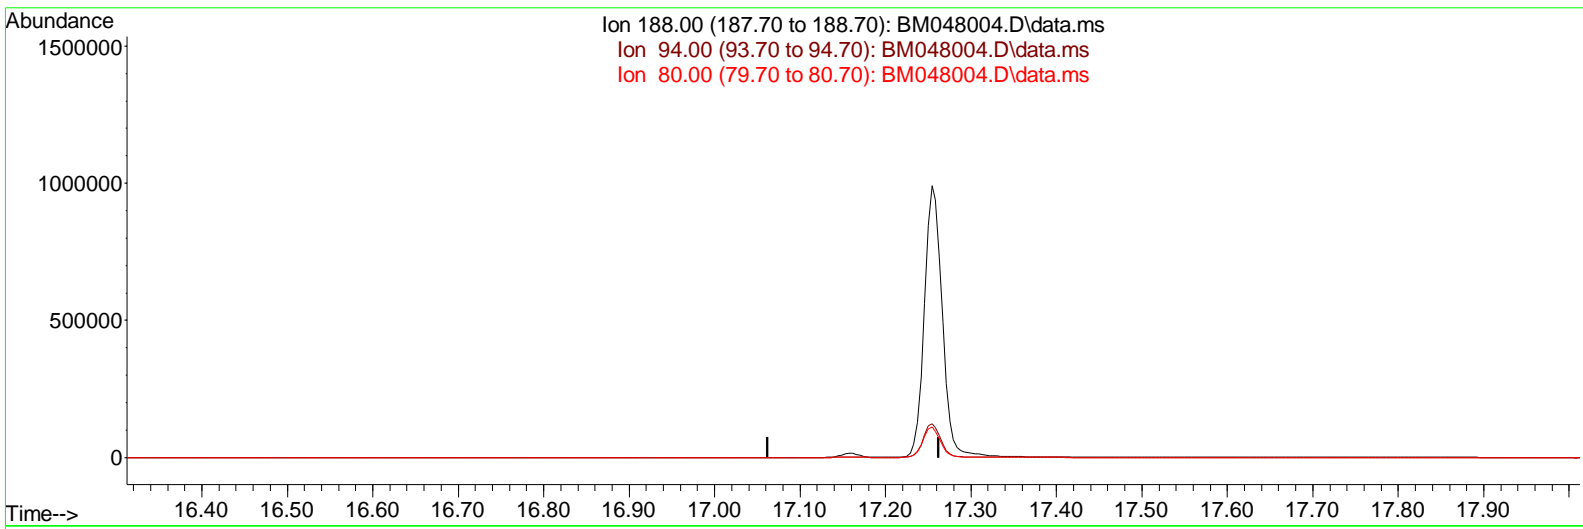

TIC: BM048004.D\data.ms

(13) Phenanthrene-d10 (I)

17.162min (-17.162) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.20	0.00#
80.00	13.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK719

Manual IntegrationsAPPROVED

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

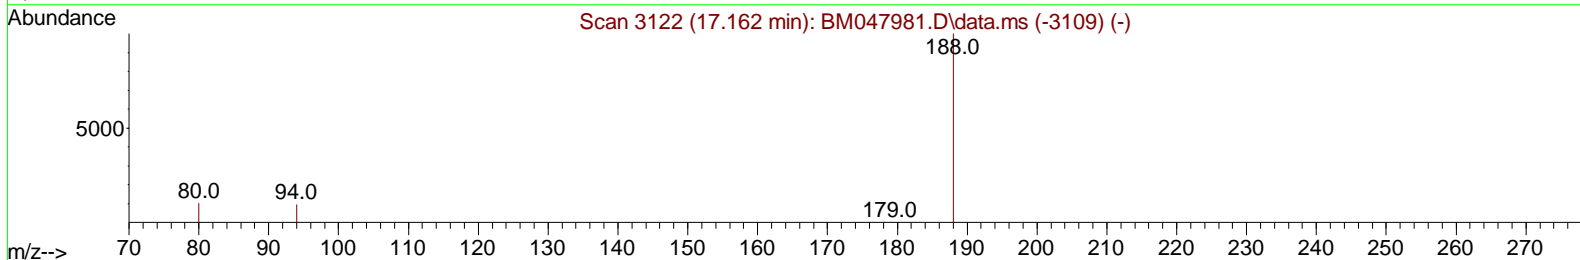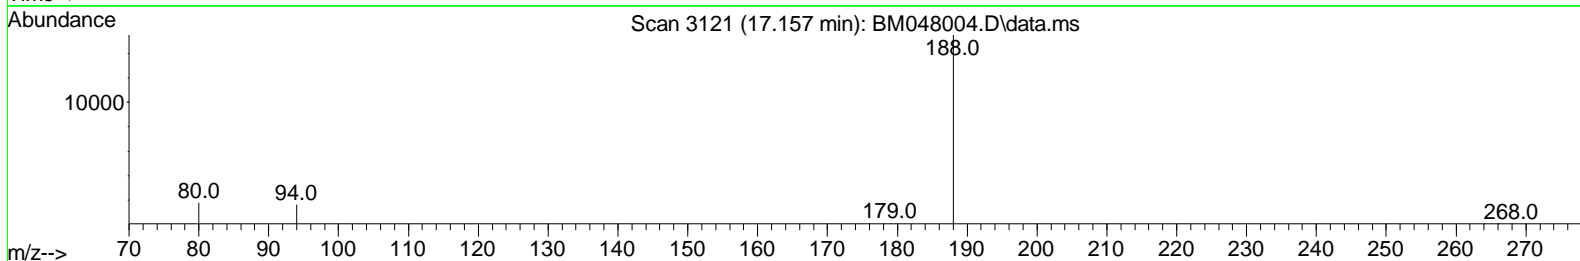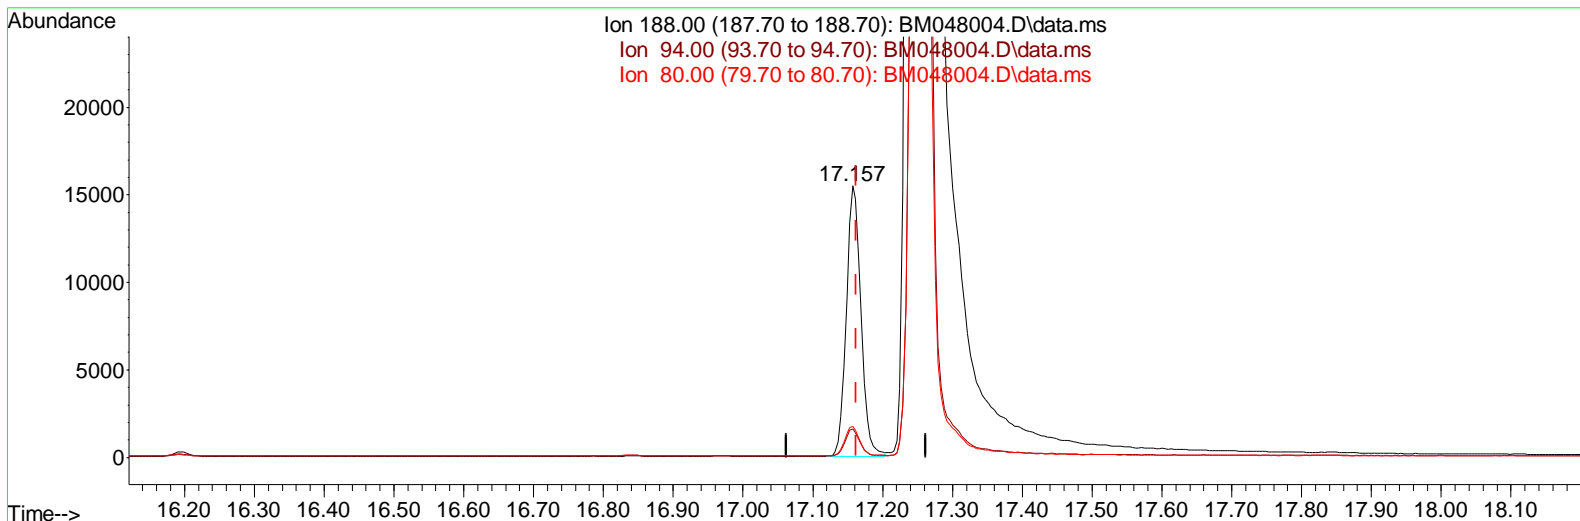

TIC: BM048004.D\data.ms

(13) Phenanthrene-d10 (I)

17.157min (-0.005) 0.40 ng/ul m

response 22519

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.20	10.42
80.00	13.00	11.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK719

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

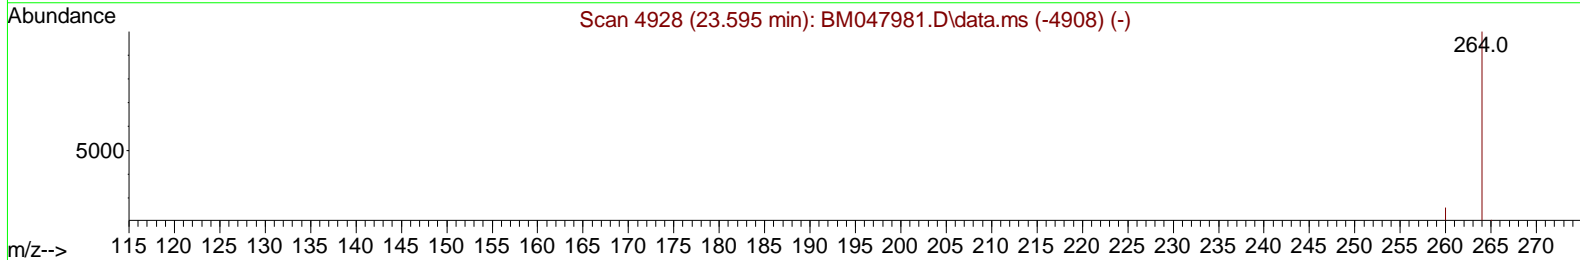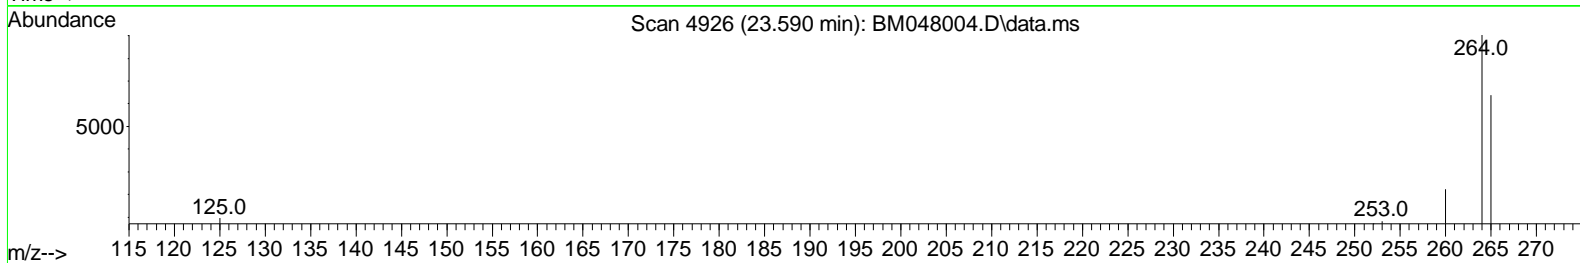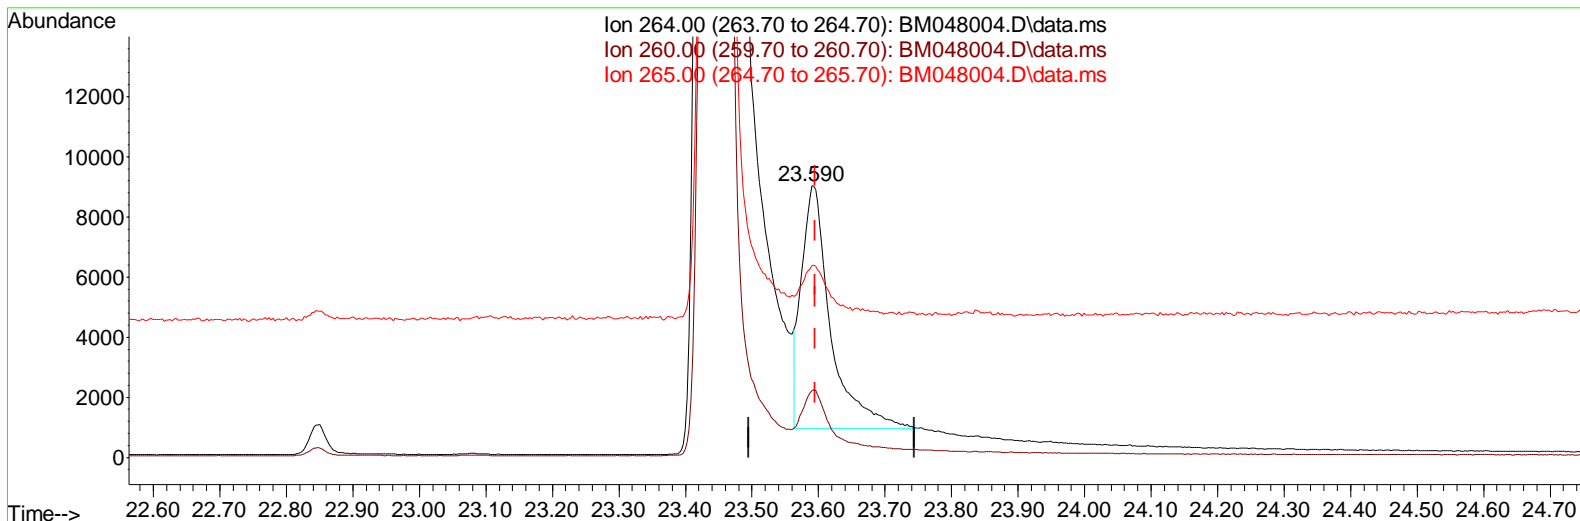

TIC: BM048004.D\data.ms

(23) Perylene-d12 (I)

23.590min (-0.005) 0.40 ng/ul

response 24629

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.58
265.00	85.70	70.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK719

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

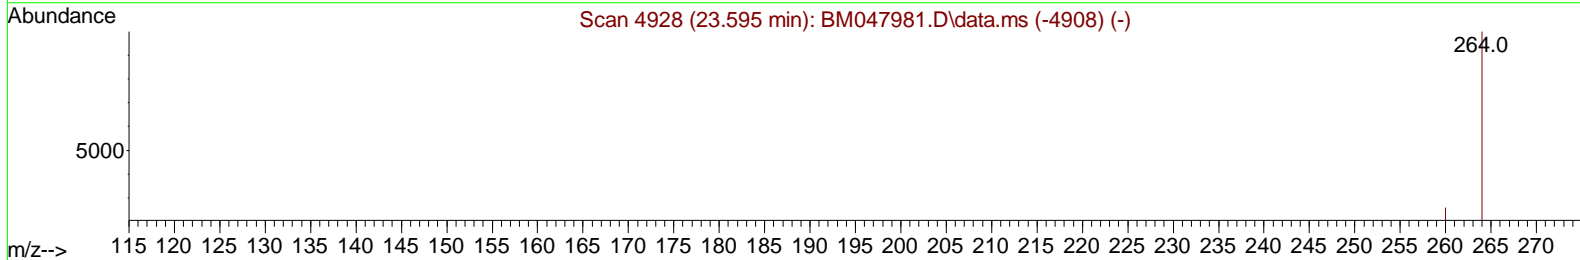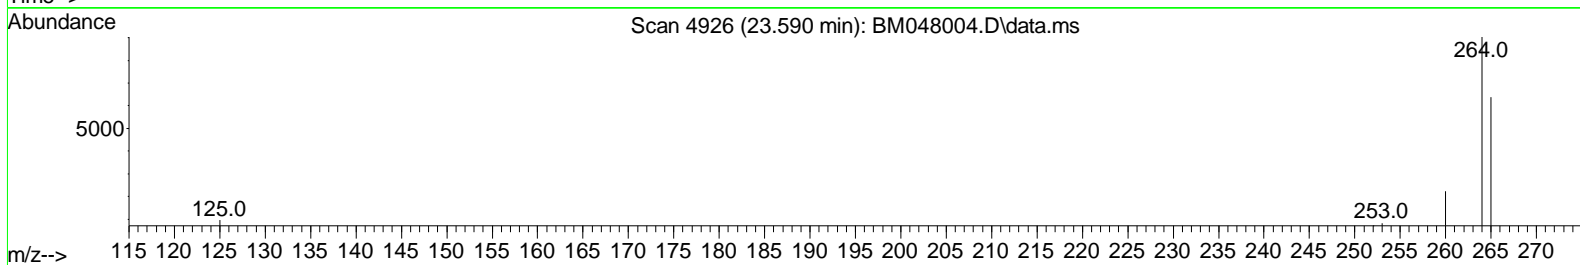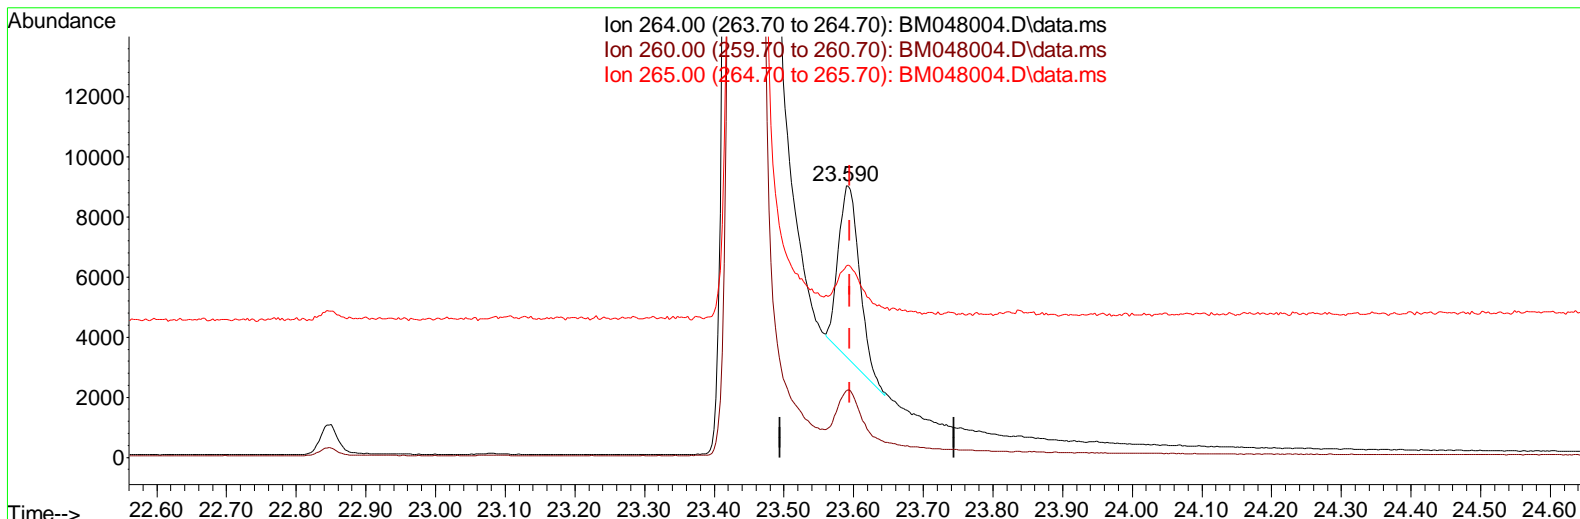

TIC: BM048004.D\data.ms

(23) Perylene-d12 (I)		
23.590min (-0.005)	0.40 ng/ul m	
response	12006	
Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.58
265.00	85.70	70.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK719

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	8370	0.400	ng/ul	0.00
4) Naphthalene-d8	10.578	136	24843	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.422	164	12151	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.157	188	22519m	0.400	ng/ul	0.00
17) Chrysene-d12	21.342	240	15315	0.400	ng/ul	0.01
23) Perylene-d12	23.590	264	12006m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	57430	5.340	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.189	152	7951	0.240	ng/ul	0.02
18) Fluoranthene-d10	19.182	212	14607	0.311	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM048004.D
 Acq On : 11 Oct 2024 08:41
 Operator : RC/JU
 Sample : PB163719BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK719

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 09:16:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

