

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM047992.D
 Acq On : 10 Oct 2024 23:37
 Operator : RC/JU
 Sample : P4187-21
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY076

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 00:10:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	9717	0.400	ng/ul	0.00
4) Naphthalene-d8	10.578	136	29615	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.422	164	14859	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.157	188	35393m	0.400	ng/ul	0.00
17) Chrysene-d12	21.327	240	27470	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	22452m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.273	96	44529	3.567	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.172	152	10199	0.258	ng/ul	0.00
18) Fluoranthene-d10	19.182	212	23428	0.279	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.307	88	6100	0.408	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
Data File : BM047992.D
Acq On : 10 Oct 2024 23:37
Operator : RC/JU
Sample : P4187-21
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EY076

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :mohammad ahmed 10/14/2024


Quant Time: Oct 11 00:10:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 18:01:13 2024
Response via : Initial Calibration

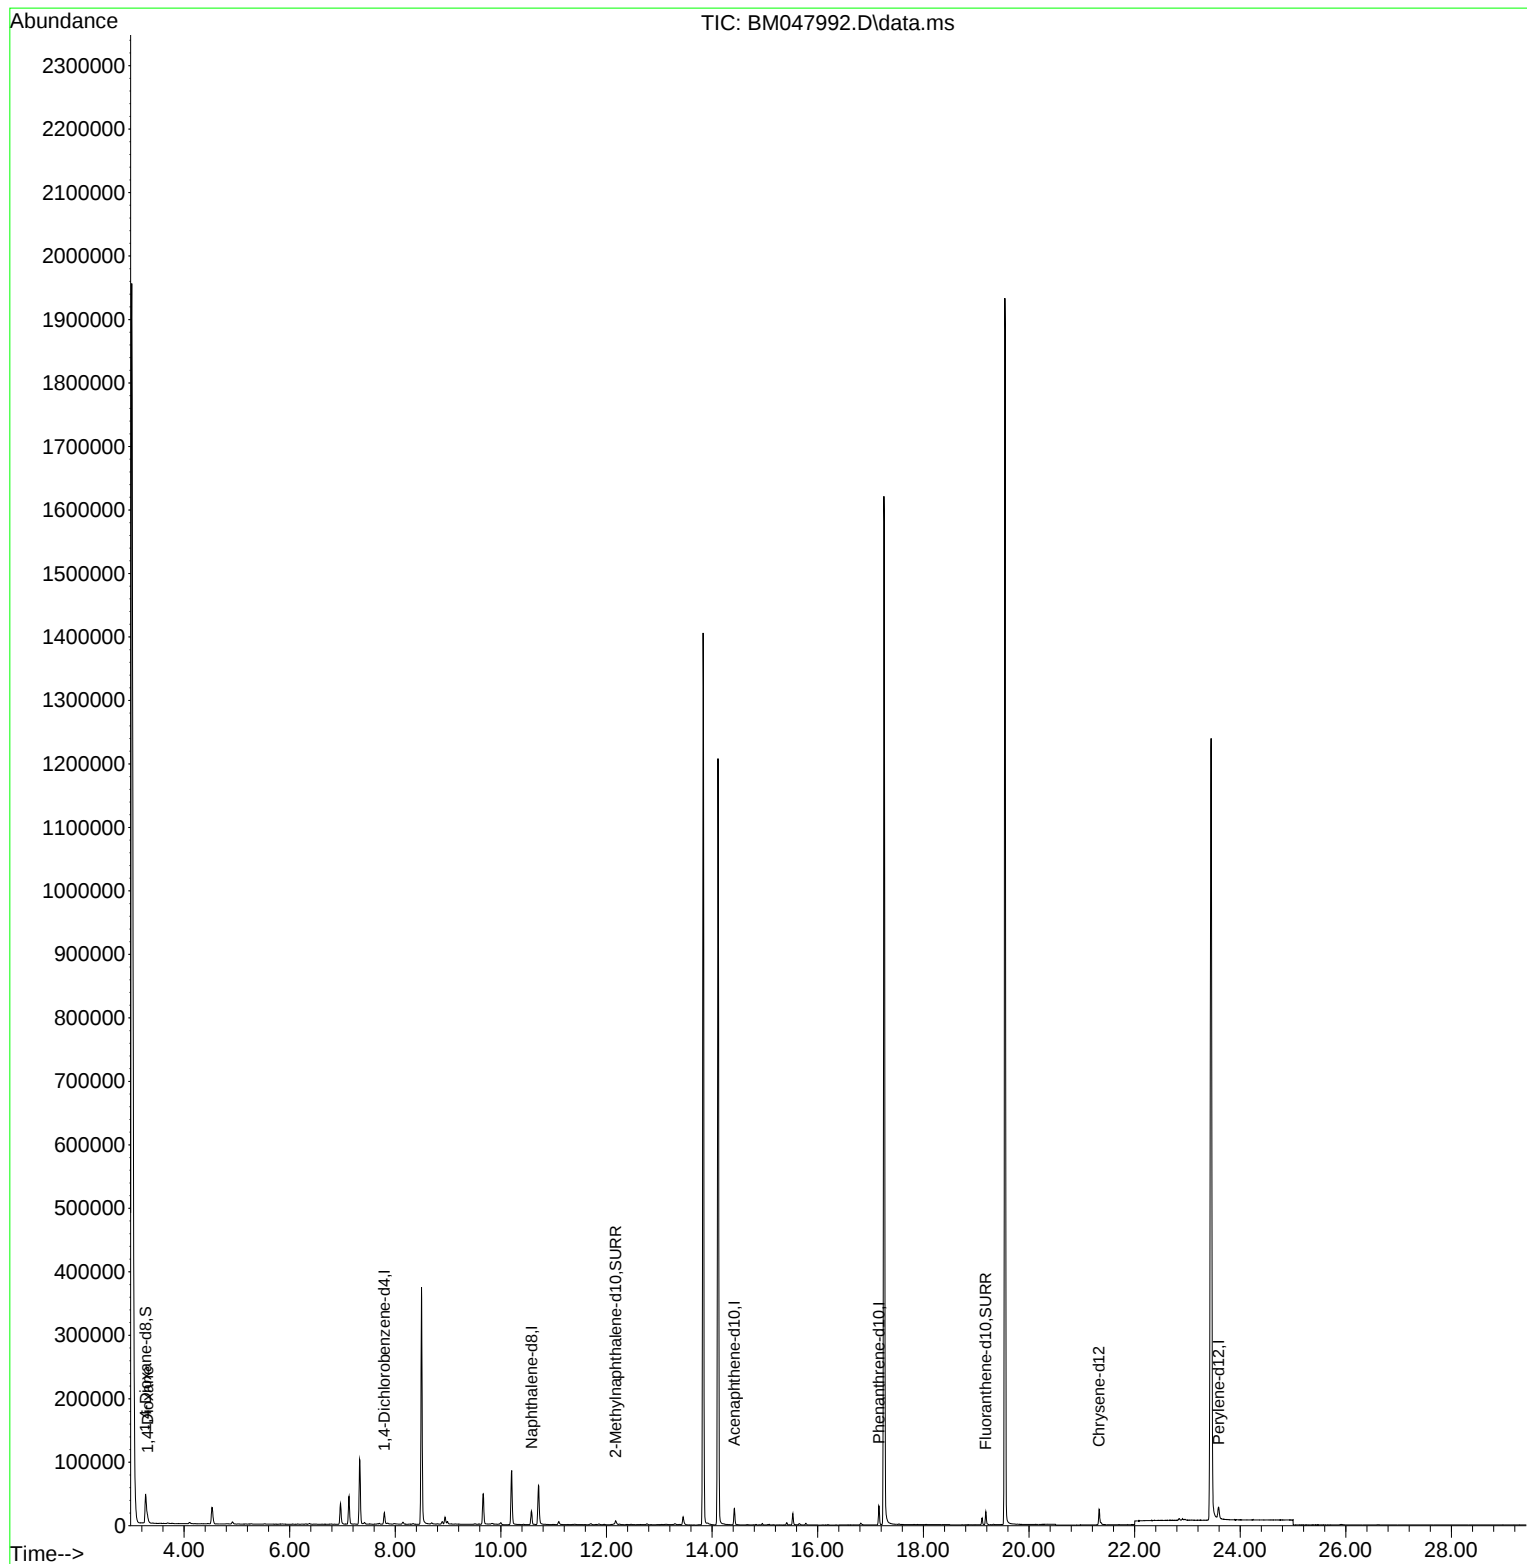

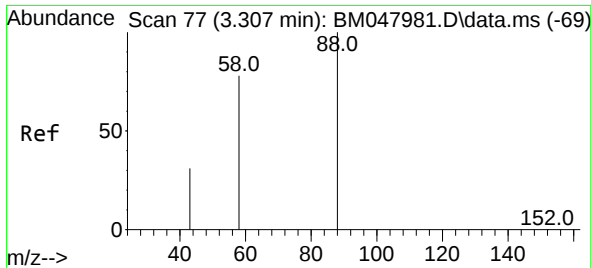

#2
 1,4-Dioxane
 Concen: 0.408 ng/ul
 RT: 3.307 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM047992.D
 Acq: 10 Oct 2024 23:37

Instrument :
 BNA_M
 ClientSampleId :
 EY076

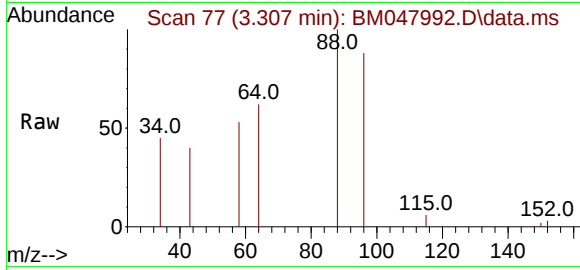

Tgt Ion: 88 Resp: 6100

Ion	Ratio	Lower	Upper
88	100		
43	40.1	30.9	46.3
58	53.4	42.5	63.7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

