

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
 Data File : BM047996.D
 Acq On : 11 Oct 2024 02:02
 Operator : RC/JU
 Sample : P4207-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY052

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

Quant Time: Oct 11 02:34:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 10 18:01:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	9602	0.400	ng/ul	0.00
4) Naphthalene-d8	10.578	136	29439	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.422	164	14448	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.157	188	28069m	0.400	ng/ul	0.00
17) Chrysene-d12	21.330	240	20720	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	18262m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.273	96	43311	3.511	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.178	152	8391	0.214	ng/ul	0.00
18) Fluoranthene-d10	19.182	212	21586	0.340	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.307	88	25877	1.753	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101024\
Data File : BM047996.D
Acq On : 11 Oct 2024 02:02
Operator : RC/JU
Sample : P4207-09
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EY052

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :mohammad ahmed 10/14/2024


Quant Time: Oct 11 02:34:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 18:01:13 2024
Response via : Initial Calibration

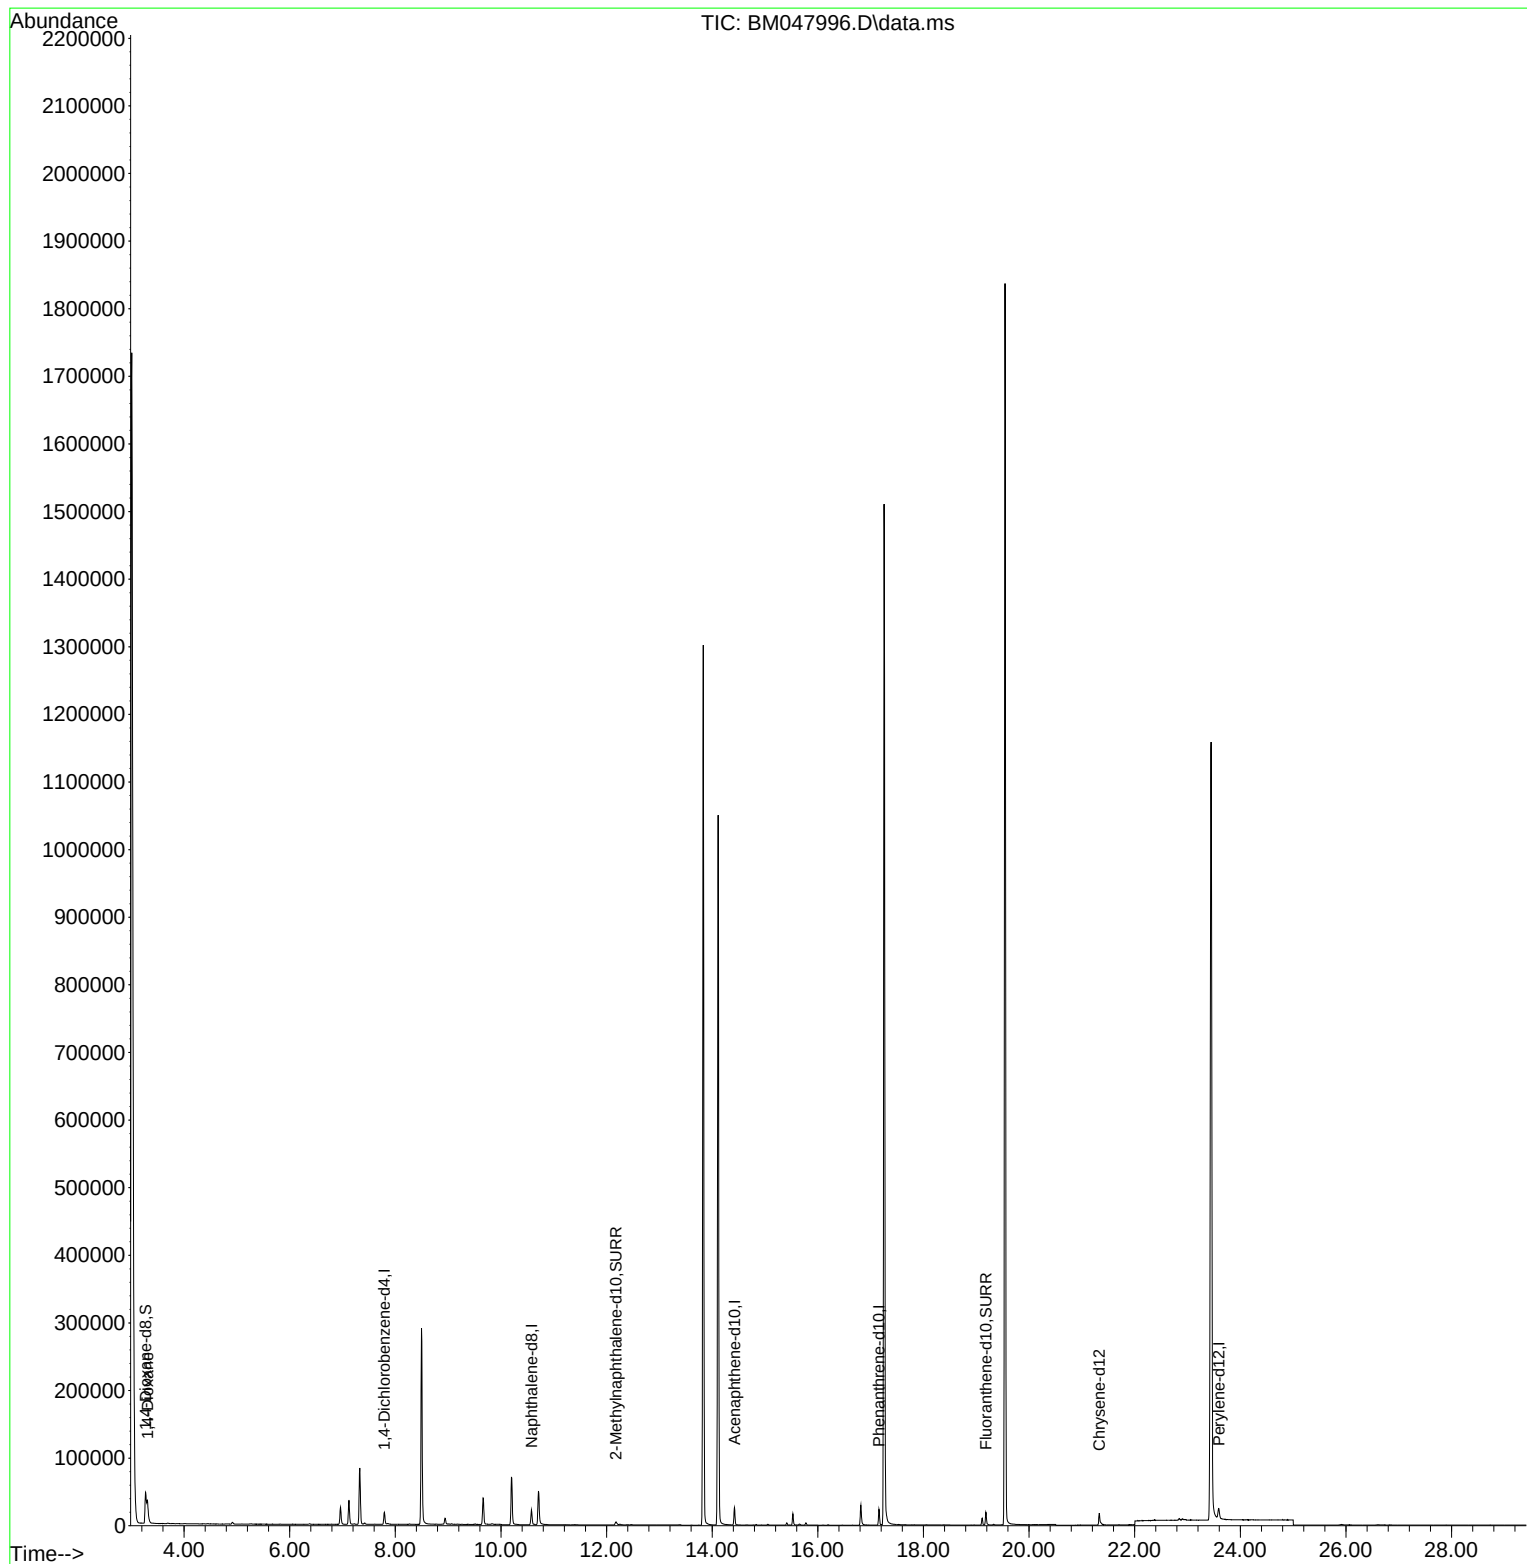

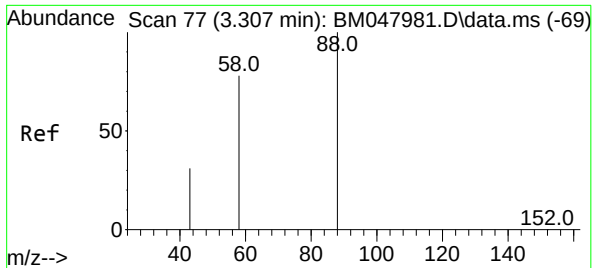

#2
 1,4-Dioxane
 Concen: 1.753 ng/ul
 RT: 3.307 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM047996.D
 Acq: 11 Oct 2024 02:02

Instrument :
 BNA_M
 ClientSampleId :
 EY052

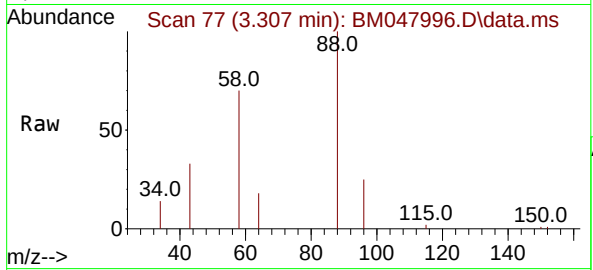

Tgt Ion: 88 Resp: 2587

Ion	Ratio	Lower	Upper
88	100		
43	32.8	30.9	46.3
58	70.3	42.5	63.7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :mohammad ahmed 10/14/2024

