

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032467.D
 Acq On : 12 Oct 2021 20:46
 Operator : CG/JU
 Sample : M4128-12
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA3

Quant Time: Oct 13 01:10:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 12 09:54:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	227942	20.000	ng/ul	0.00
20) Naphthalene-d8	10.395	136	1021801	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.260	164	697084	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.983	188	1485024	20.000	ng/ul	0.00
79) Chrysene-d12	21.147	240	1458033	20.000	ng/ul	0.00
88) Perylene-d12	23.289	264	1451415	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.955	96	29695	5.223	ng/uL	0.00
4) Pyridine-d5	3.390	84	156621	9.752	ng/ul	0.00
7) Phenol-d5	6.801	99	156260	8.062	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.937	67	336703	30.254	ng/ul	0.00
11) 2-Chlorophenol-d4	7.148	132	394058	26.627	ng/ul	0.00
15) 4-Methylphenol-d8	8.337	113	293397	18.741	ng/ul	0.00
21) Nitrobenzene-d5	8.760	128	245047	33.990	ng/ul	0.00
24) 2-Nitrophenol-d4	9.484	143	273229	35.160	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.031	165	474022	30.642	ng/ul	0.00
31) 4-Chloroaniline-d4	10.531	131	610206	26.742	ng/ul	0.00
46) Dimethylphthalate-d6	13.660	166	1920176	39.803	ng/ul	0.00
49) Acenaphthylene-d8	13.948	160	2101684	35.861	ng/ul	0.00
54) 4-Nitrophenol-d4	14.466	143	75181	7.935	ng/ul	0.00
60) Fluorene-d10	15.248	176	1619766	39.589	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.366	200	301811	35.661	ng/ul	0.00
73) Anthracene-d10	17.083	188	2667497	41.266	ng/ul	0.00
81) Pyrene-d10	19.371	212	3051839	41.606	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.159	264	2846629	39.164	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.695	107	56026	3.343	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032467.D
Acq On : 12 Oct 2021 20:46
Operator : CG/JU
Sample : M4128-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA3

Quant Time: Oct 13 01:10:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 12 09:54:27 2021
Response via : Initial Calibration

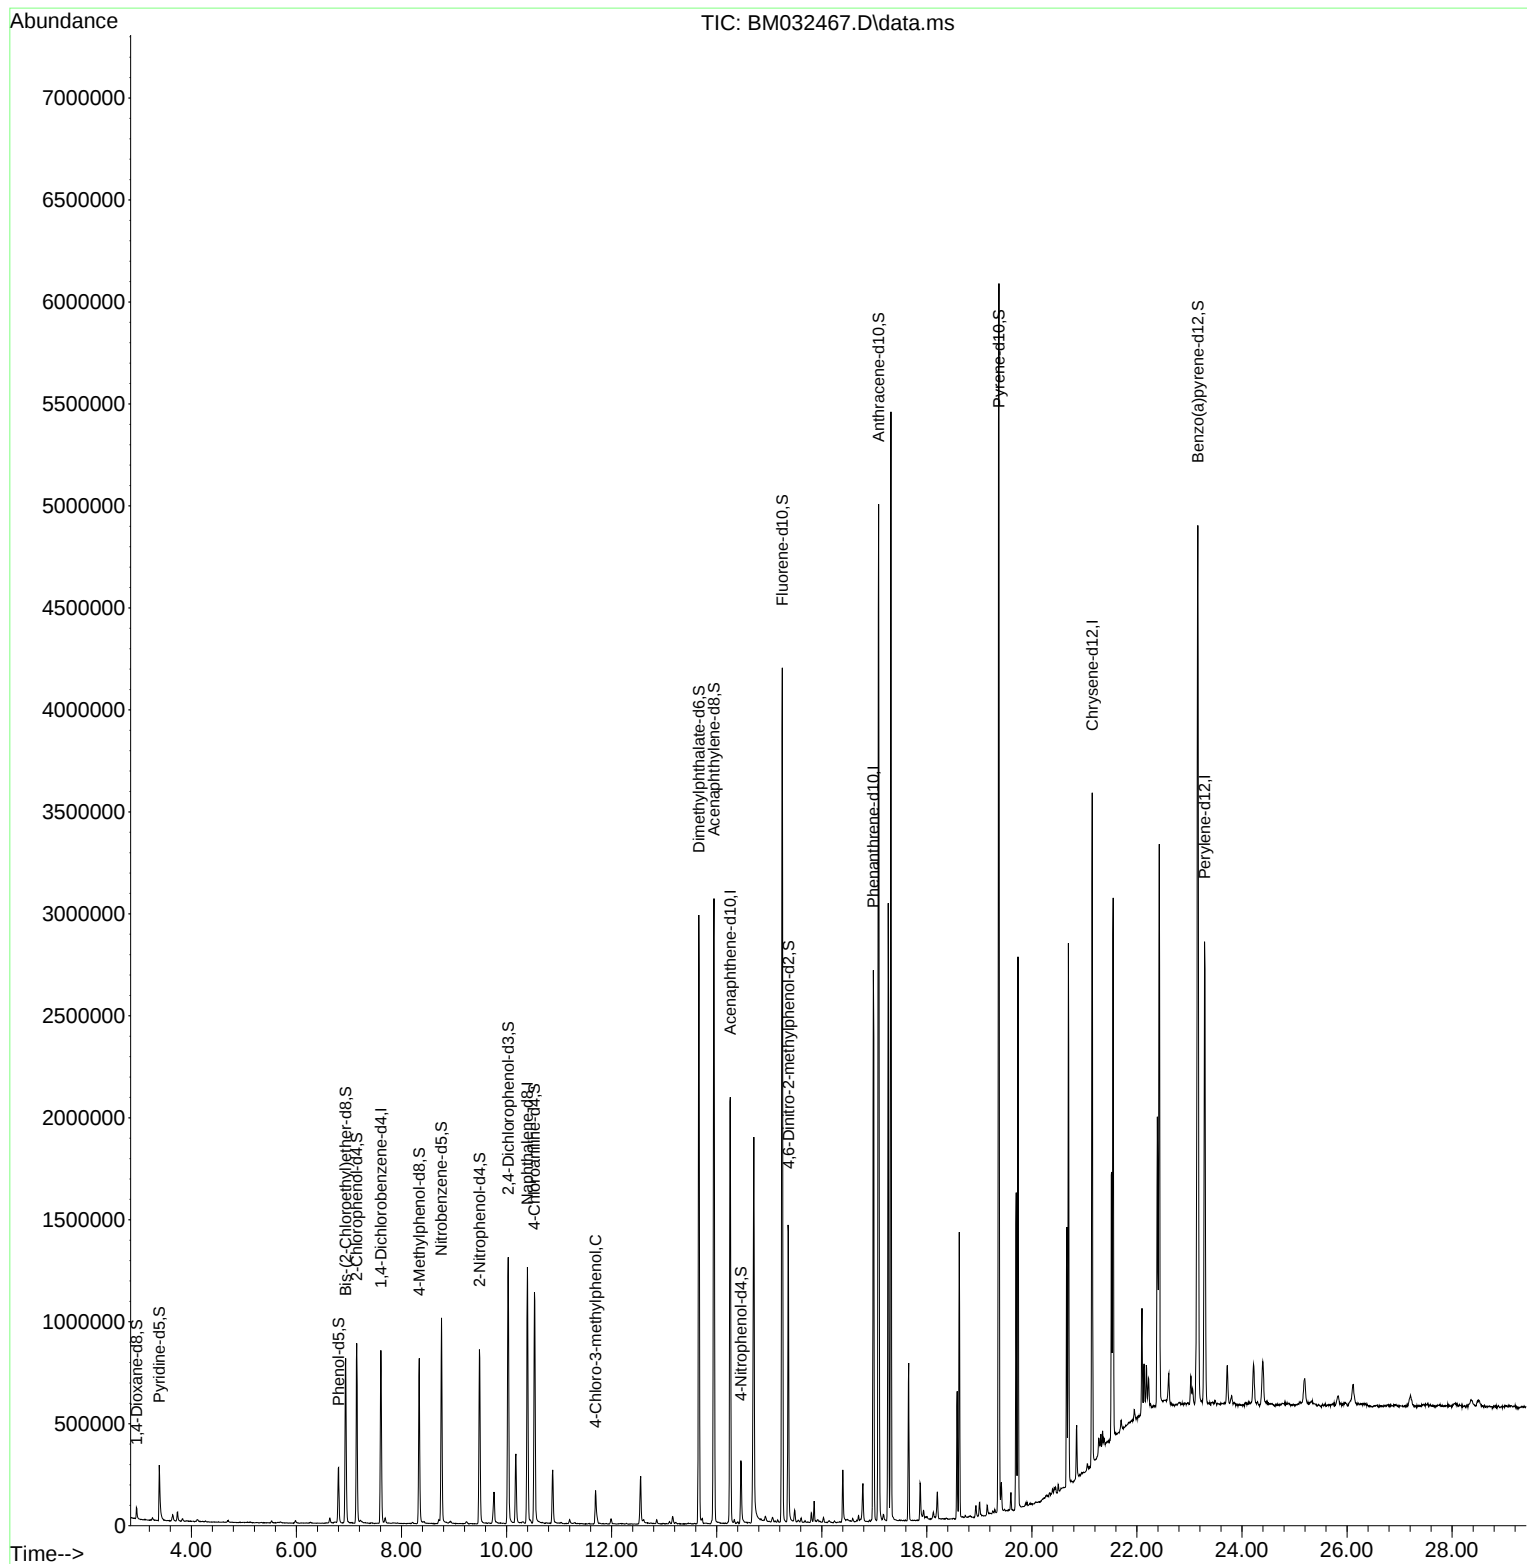

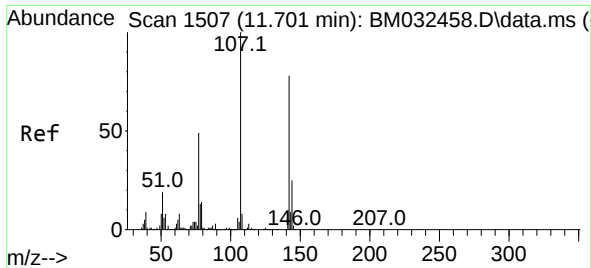

#35
 4-Chloro-3-methylphenol
 Concen: 3.343 ng/ul
 RT: 11.695 min Scan# 1506
 Delta R.T. -0.006 min
 Lab File: BM032467.D
 Acq: 12 Oct 2021 20:46

Instrument :
 BNA_M
 ClientSampleId :
 C0AA3

Tgt Ion:107	Resp:	56026
Ion	Ratio	Lower Upper
107	100	
144	26.6	20.4 30.6
142	79.4	62.4 93.6

