

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032468.D
 Acq On : 12 Oct 2021 21:22
 Operator : CG/JU
 Sample : M4110-06
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00U8

Quant Time: Oct 13 01:10:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 12 09:54:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	208457	20.000	ng/ul	0.00
20) Naphthalene-d8	10.395	136	925357	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.254	164	649278	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.983	188	1379435	20.000	ng/ul	0.00
79) Chrysene-d12	21.148	240	1354786	20.000	ng/ul	0.00
88) Perylene-d12	23.289	264	1342590	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.955	96	27777	5.342	ng/uL	0.00
4) Pyridine-d5	3.390	84	138761	9.447	ng/ul	0.00
7) Phenol-d5	6.796	99	135488	7.643	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.937	67	303160	29.786	ng/ul	0.00
11) 2-Chlorophenol-d4	7.148	132	348607	25.757	ng/ul	0.00
15) 4-Methylphenol-d8	8.337	113	249265	17.410	ng/ul	0.00
21) Nitrobenzene-d5	8.760	128	217942	33.381	ng/ul	0.00
24) 2-Nitrophenol-d4	9.484	143	237148	33.697	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.031	165	402993	28.765	ng/ul	0.00
31) 4-Chloroaniline-d4	10.531	131	578674	28.004	ng/ul	0.00
46) Dimethylphthalate-d6	13.660	166	1663118	37.013	ng/ul	0.00
49) Acenaphthylene-d8	13.948	160	1845660	33.811	ng/ul	0.00
54) 4-Nitrophenol-d4	14.460	143	63235	7.166	ng/ul	-0.01
60) Fluorene-d10	15.248	176	1439903	37.785	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.366	200	255157	32.456	ng/ul	0.00
73) Anthracene-d10	17.083	188	2506339	41.740	ng/ul	0.00
81) Pyrene-d10	19.371	212	2820636	41.385	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.153	264	2616541	38.916	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.053	149	159463	3.499	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032468.D
Acq On : 12 Oct 2021 21:22
Operator : CG/JU
Sample : M4110-06
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00U8

Quant Time: Oct 13 01:10:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 12 09:54:27 2021
Response via : Initial Calibration

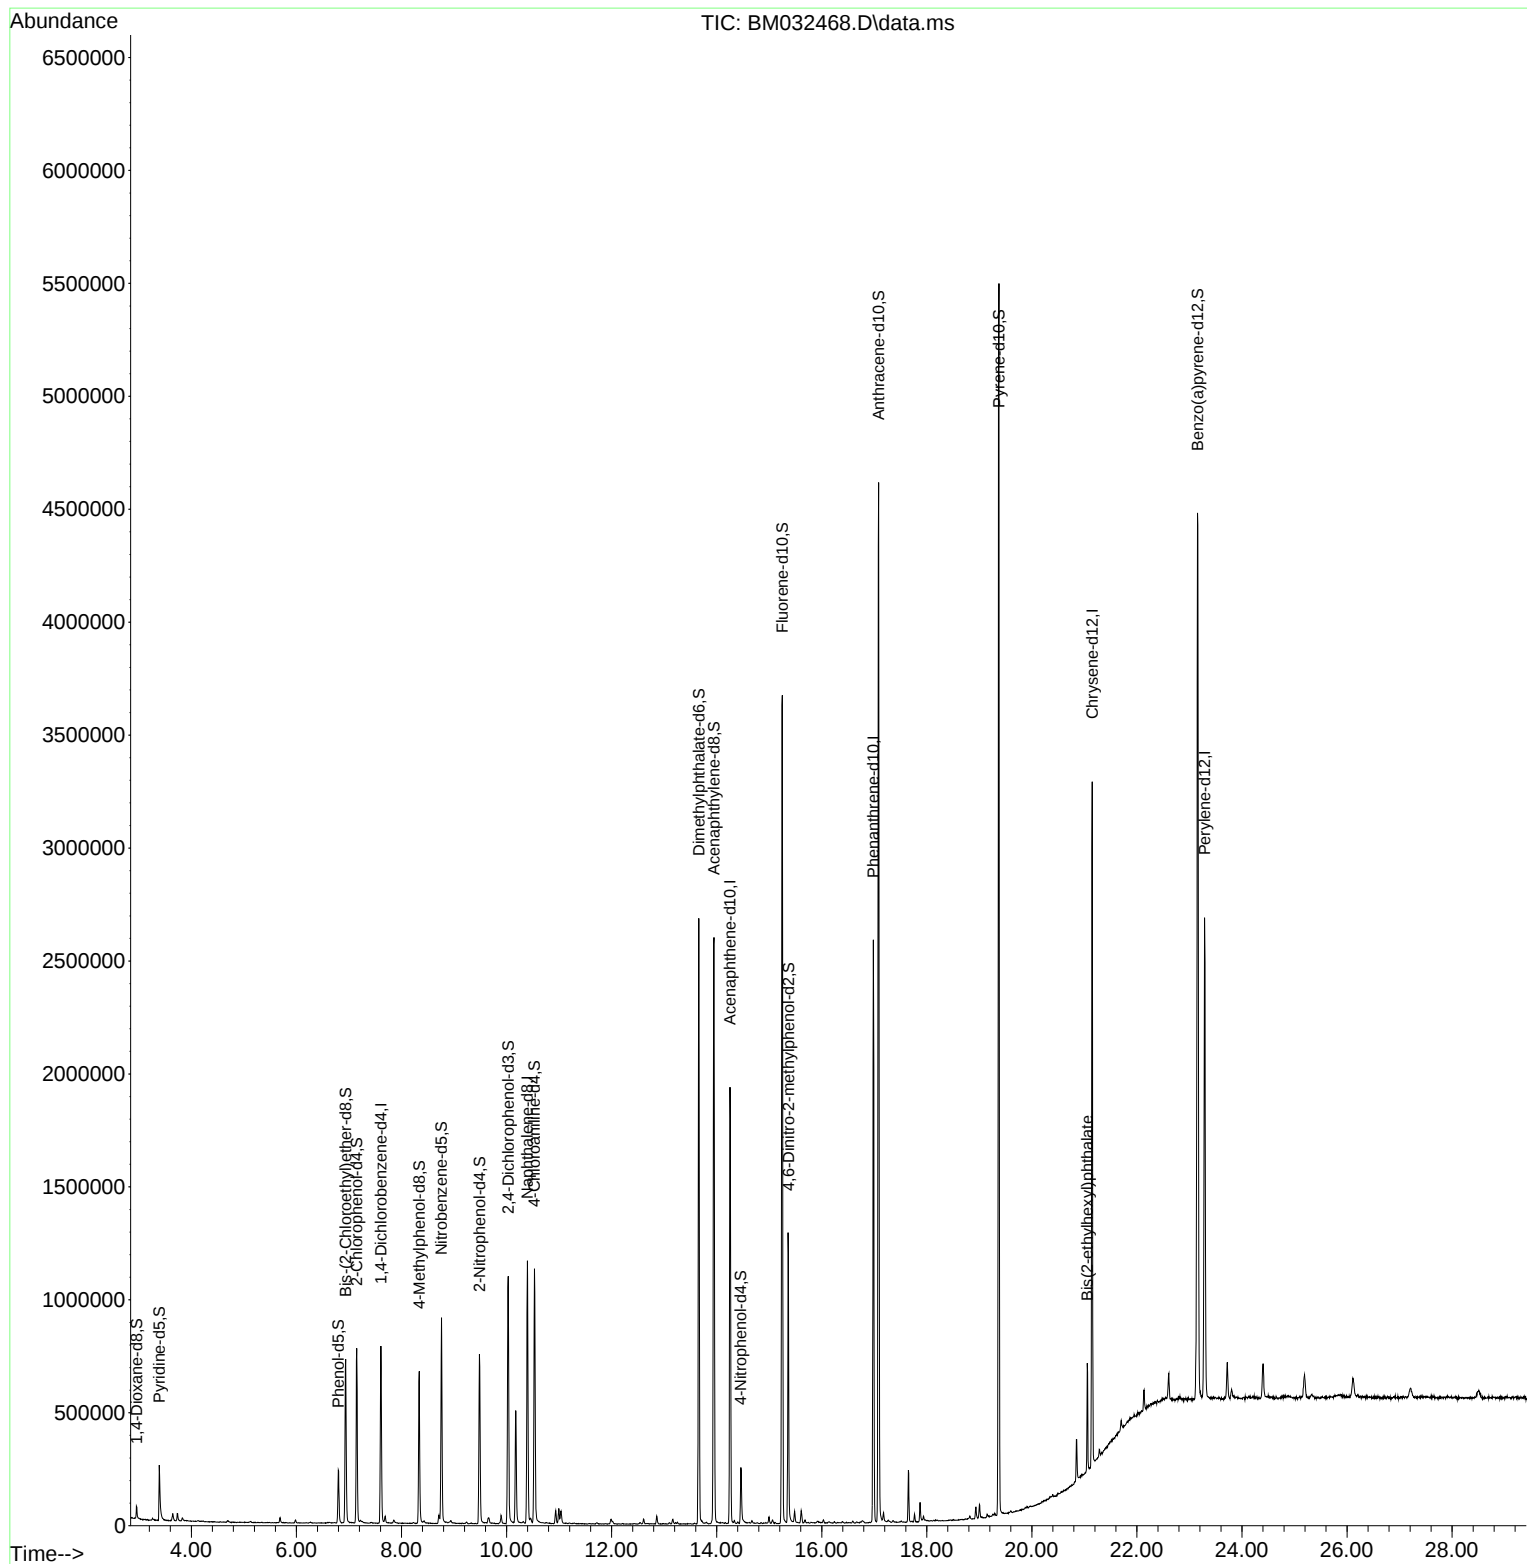

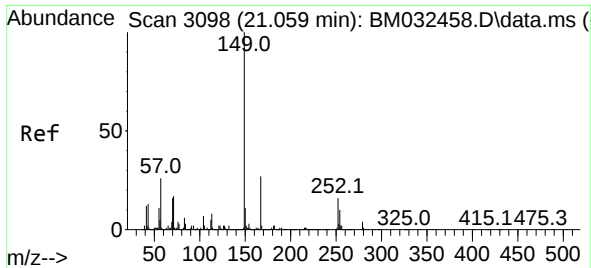

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.499 ng/ul
 RT: 21.053 min Scan# 3097
 Delta R.T. -0.006 min
 Lab File: BM032468.D
 Acq: 12 Oct 2021 21:22

Instrument :
 BNA_M
 ClientSampleId :
 C00U8

Tgt Ion:149 Resp: 159463
 Ion Ratio Lower Upper
 149 100
 167 26.7 22.0 33.0
 279 3.6 3.3 4.9

