

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032415.D
 Acq On : 11 Oct 2021 10:55
 Operator : CG/JU
 Sample : PB139762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.954	17	20	29	rVB	53728	72874	1.25%	0.127%
2	3.384	89	93	115	rBV	697922	1053280	18.08%	1.840%
3	3.737	148	153	164	rVB	109610	155894	2.68%	0.272%
4	6.807	668	675	684	rBV	846642	1275905	21.90%	2.228%
5	6.942	689	698	708	rVV	680678	1023192	17.56%	1.787%
6	7.154	726	734	743	rBV	864556	1324510	22.74%	2.313%
7	7.613	805	812	826	rBV	668159	1055470	18.12%	1.843%
8	8.342	929	936	951	rBV	1091261	1688371	28.98%	2.949%
9	8.460	954	956	962	rVB7	3327	6320	0.11%	0.011%
10	8.766	1000	1008	1017	rBV	810826	1297332	22.27%	2.266%
11	9.495	1124	1132	1144	rBV	706687	1123371	19.28%	1.962%
12	10.036	1217	1224	1237	rBV	1071109	1695922	29.11%	2.962%
13	10.407	1280	1287	1299	rBV	1005688	1637466	28.11%	2.860%
14	10.542	1302	1310	1329	rBV	1079921	1790490	30.74%	3.127%
15	11.183	1411	1419	1420	rBV6	3498	7640	0.13%	0.013%
16	11.995	1552	1557	1564	rVB	21559	35673	0.61%	0.062%
17	12.995	1722	1727	1732	rBV8	3944	7938	0.14%	0.014%
18	13.230	1760	1767	1772	rBV7	3696	7751	0.13%	0.014%
19	13.624	1828	1834	1835	rBV5	5616	8996	0.15%	0.016%
20	13.666	1835	1841	1851	rVV	2164374	2873453	49.33%	5.019%
21	13.954	1883	1890	1896	rBV	2314837	3250081	55.79%	5.676%
22	14.077	1906	1911	1915	rVB2	13180	18755	0.32%	0.033%
23	14.266	1936	1943	1951	rBV	1705234	2378021	40.82%	4.153%
24	14.471	1971	1978	1992	rBV	1034413	1489592	25.57%	2.602%
25	14.683	2011	2014	2020	rVB6	12304	17414	0.30%	0.030%
26	14.830	2035	2039	2045	rVB2	8166	12242	0.21%	0.021%
27	15.254	2104	2111	2123	rBV	3002455	4133172	70.95%	7.219%
28	15.371	2125	2131	2146	rVV	1117028	1423249	24.43%	2.486%
29	15.489	2147	2151	2158	rVB2	38466	56129	0.96%	0.098%
30	15.918	2221	2224	2227	rBV5	6452	6866	0.12%	0.012%
31	16.036	2237	2244	2249	rBV6	15224	28556	0.49%	0.050%
32	16.124	2254	2259	2263	rBV8	3842	7691	0.13%	0.013%
33	16.777	2364	2370	2376	rBV	11148	16969	0.29%	0.030%
34	16.989	2400	2406	2416	rBV	2097751	2928362	50.27%	5.115%
35	17.089	2416	2423	2436	rBV	3522139	4629241	79.46%	8.085%
36	17.359	2465	2469	2473	rBV2	5103	8443	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032415.D
 Acq On : 11 Oct 2021 10:55
 Operator : CG/JU
 Sample : PB139762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	17.659	2516	2520	2524	rBV6	13352	17058	0.29%	0.030%
38	17.877	2550	2557	2566	rBV	124558	213423	3.66%	0.373%
39	18.942	2733	2738	2745	rBV3	43678	72205	1.24%	0.126%
40	19.012	2745	2750	2754	rBV	50473	67400	1.16%	0.118%
41	19.153	2771	2774	2780	rBV4	31004	47291	0.81%	0.083%
42	19.377	2806	2812	2823	rBV	4194260	5470811	93.91%	9.555%
43	21.153	3109	3114	3122	rBV	2771771	3398683	58.34%	5.936%
44	23.171	3450	3457	3469	rVB	3302662	5825537	100.00%	10.175%
45	23.306	3473	3480	3488	rVB2	2075874	3596666	61.74%	6.282%




Sum of corrected areas: 57255705

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032415.D
Acq On : 11 Oct 2021 10:55
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

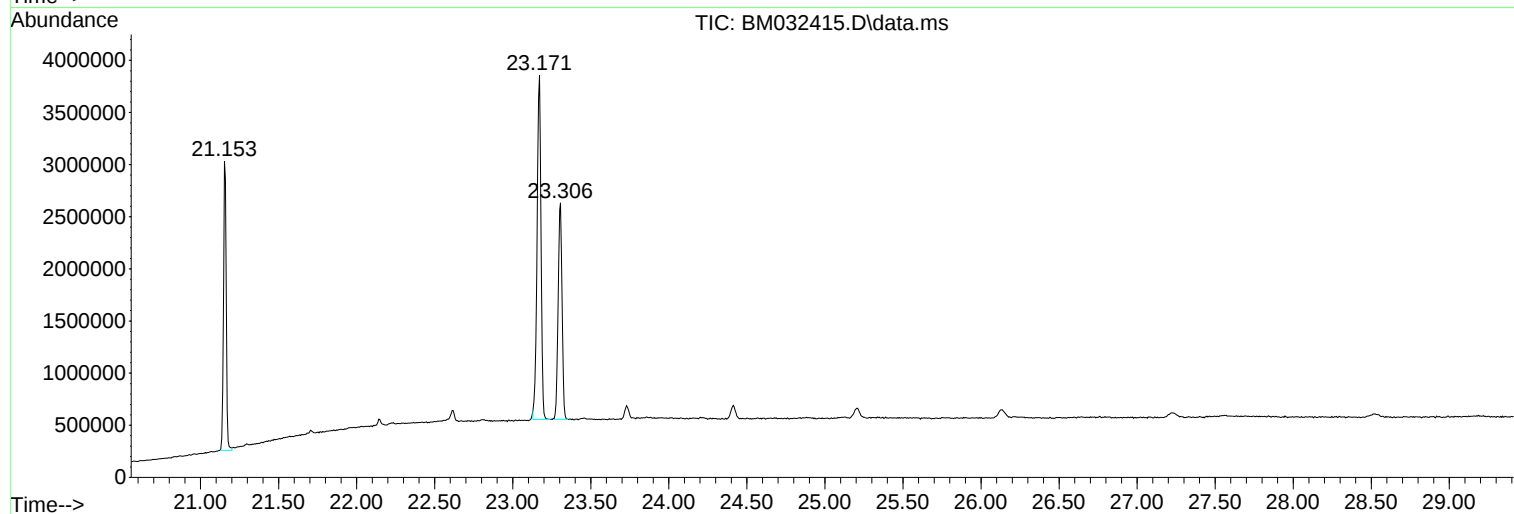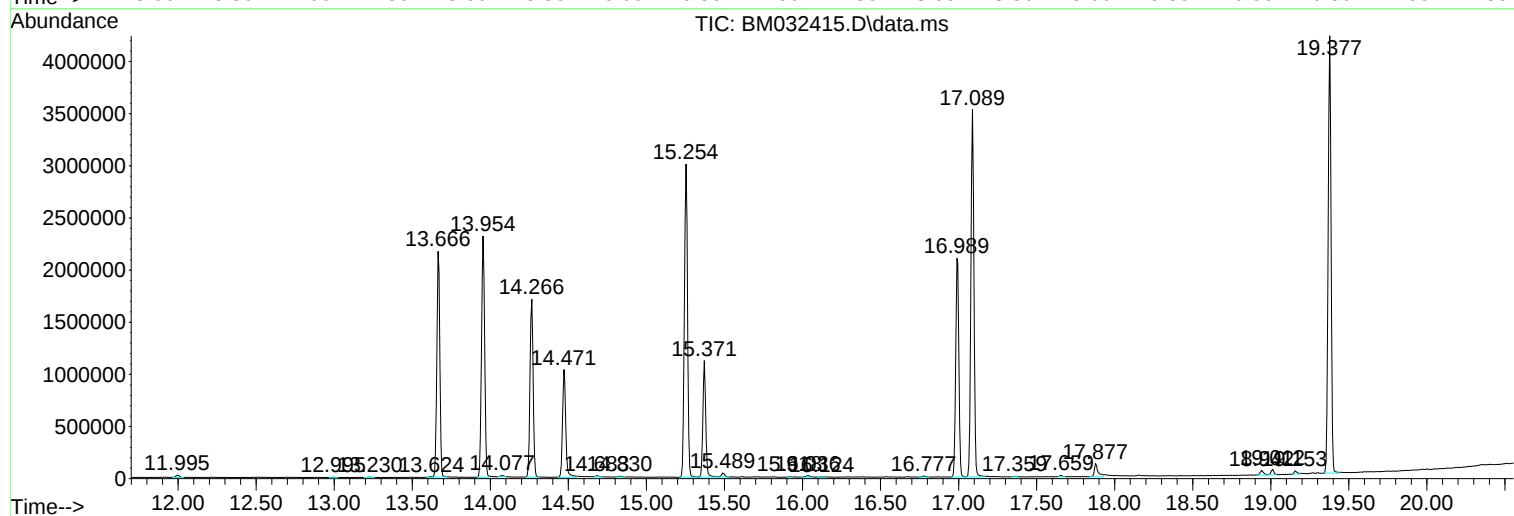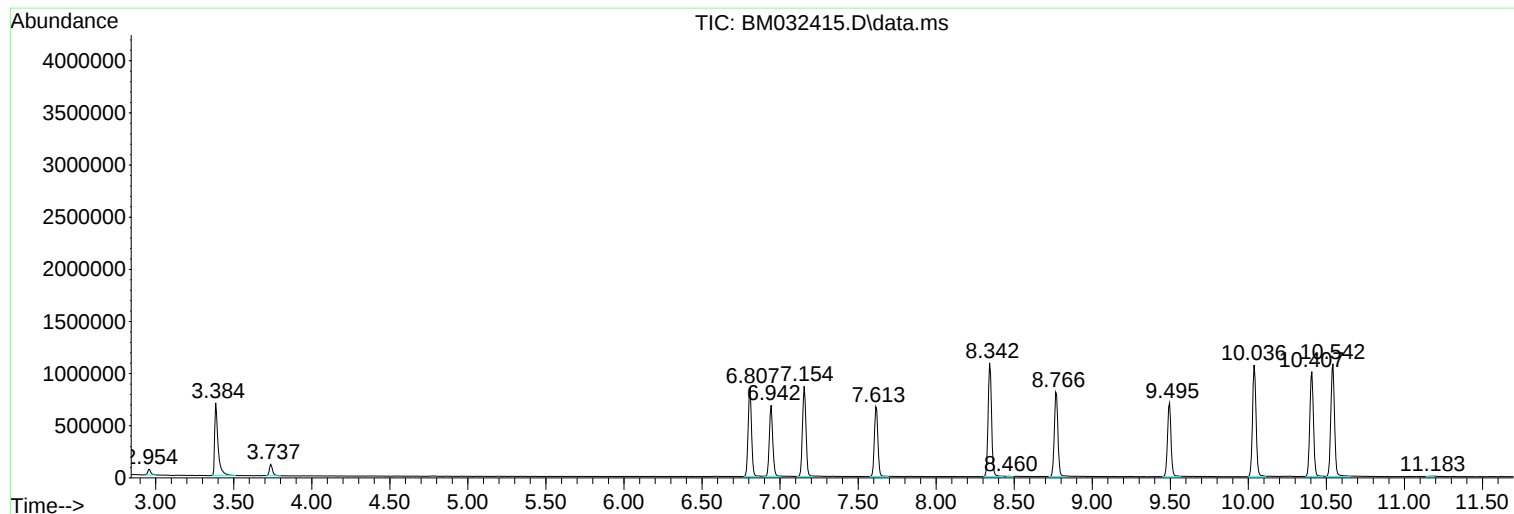

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032415.D
Acq On : 11 Oct 2021 10:55
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032415.D
Acq On : 11 Oct 2021 10:55
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
