

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032423.D
 Acq On : 11 Oct 2021 16:22
 Operator : CG/JU
 Sample : M4029-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00R4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.961	17	21	26	rVB	15140	20678	0.66%	0.084%
2	3.402	93	96	106	rBV	52344	84848	2.70%	0.343%
3	3.508	110	114	118	rVB4	8783	11103	0.35%	0.045%
4	3.649	130	138	143	rBV	36971	63681	2.03%	0.258%
5	3.737	149	153	160	rVB	14547	19690	0.63%	0.080%
6	3.925	182	185	189	rVB6	3067	4382	0.14%	0.018%
7	3.984	192	195	200	rVB	20971	27146	0.87%	0.110%
8	4.131	215	220	225	rVB8	5759	10291	0.33%	0.042%
9	4.314	248	251	256	rVB7	3655	5803	0.18%	0.023%
10	4.414	265	268	272	rVB	12774	16257	0.52%	0.066%
11	4.696	311	316	323	rBV	10531	17668	0.56%	0.071%
12	4.796	330	333	338	rVB5	5584	9847	0.31%	0.040%
13	4.855	338	343	347	rBV8	2862	6884	0.22%	0.028%
14	5.319	418	422	427	rBV6	2576	4937	0.16%	0.020%
15	5.631	472	475	481	rVB7	4518	7585	0.24%	0.031%
16	6.631	641	645	651	rVB8	4869	7119	0.23%	0.029%
17	6.743	659	664	669	rBV5	8990	14850	0.47%	0.060%
18	6.802	669	674	688	rVB	190746	308672	9.84%	1.249%
19	6.943	692	698	710	rVB	153567	244456	7.79%	0.989%
20	7.155	726	734	742	rBV	203731	315191	10.05%	1.275%
21	7.260	748	752	759	rVB4	11411	19428	0.62%	0.079%
22	7.437	779	782	787	rVB6	4000	5036	0.16%	0.020%
23	7.613	805	812	823	rBV	668104	1025988	32.71%	4.151%
24	7.866	849	855	862	rVB10	6267	11998	0.38%	0.049%
25	8.178	903	908	911	rBV5	4992	9220	0.29%	0.037%
26	8.343	925	936	944	rBV	209019	336477	10.73%	1.361%
27	8.437	947	952	960	rVB	19634	36796	1.17%	0.149%
28	8.766	1001	1008	1016	rBV	183831	294284	9.38%	1.191%
29	8.860	1019	1024	1029	rVB9	4387	9173	0.29%	0.037%
30	9.237	1085	1088	1095	rVB6	4465	8310	0.26%	0.034%
31	9.490	1126	1131	1140	rBV	143479	234217	7.47%	0.948%
32	9.972	1208	1213	1216	rBV6	5150	8326	0.27%	0.034%
33	10.037	1218	1224	1233	rVV	240095	379573	12.10%	1.536%
34	10.178	1240	1248	1261	rBV	130007	207235	6.61%	0.838%
35	10.284	1264	1266	1269	rVB3	3953	4101	0.13%	0.017%
36	10.401	1278	1286	1293	rBV	957346	1563637	49.85%	6.327%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032423.D
 Acq On : 11 Oct 2021 16:22
 Operator : CG/JU
 Sample : M4029-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00R4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	10.537	1302	1309	1316	rBV	222664	365843	11.66%	1.480%
38	11.178	1413	1418	1420	rBV4	4478	7400	0.24%	0.030%
39	11.201	1420	1422	1428	rVB6	5533	8731	0.28%	0.035%
40	11.431	1458	1461	1468	rVB8	3021	6824	0.22%	0.028%
41	11.843	1526	1531	1535	rBV6	6450	9808	0.31%	0.040%
42	11.895	1535	1540	1542	rBV5	4877	5947	0.19%	0.024%
43	11.990	1552	1556	1564	rVB7	6407	12751	0.41%	0.052%
44	12.072	1564	1570	1574	rBV3	7552	14596	0.47%	0.059%
45	12.295	1602	1608	1610	rBV4	3950	6144	0.20%	0.025%
46	12.613	1656	1662	1670	rBV8	7931	16064	0.51%	0.065%
47	12.701	1674	1677	1680	rBV4	3151	4127	0.13%	0.017%
48	12.866	1700	1705	1709	rBV4	7932	11402	0.36%	0.046%
49	13.095	1737	1744	1749	rBV7	7329	13640	0.43%	0.055%
50	13.160	1749	1755	1760	rVV6	5273	8551	0.27%	0.035%
51	13.225	1762	1766	1771	rVV5	2686	4118	0.13%	0.017%
52	13.584	1822	1827	1830	rBV6	5479	8498	0.27%	0.034%
53	13.666	1830	1841	1847	rBV	484216	665257	21.21%	2.692%
54	13.907	1877	1882	1884	rBV5	6416	8790	0.28%	0.036%
55	13.954	1884	1890	1899	rVV	510967	745529	23.77%	3.016%
56	14.072	1903	1910	1915	rBV3	21264	42265	1.35%	0.171%
57	14.172	1923	1927	1932	rVB4	7144	9643	0.31%	0.039%
58	14.260	1936	1942	1951	rBV	1530467	2234752	71.24%	9.042%
59	14.407	1964	1967	1972	rBV7	5136	7720	0.25%	0.031%
60	14.472	1972	1978	1989	rBV	120871	205646	6.56%	0.832%
61	14.672	2005	2012	2021	rBV8	20305	46142	1.47%	0.187%
62	15.066	2074	2079	2085	rBV5	9512	17036	0.54%	0.069%
63	15.119	2085	2088	2091	rVB3	7227	8556	0.27%	0.035%
64	15.248	2103	2110	2117	rBV	723744	1012855	32.29%	4.098%
65	15.366	2125	2130	2137	rBV	102073	149900	4.78%	0.607%
66	15.495	2144	2152	2155	rBV3	8344	17613	0.56%	0.071%
67	15.607	2167	2171	2177	rVB7	5822	10038	0.32%	0.041%
68	15.666	2177	2181	2185	rBV6	6498	13049	0.42%	0.053%
69	15.742	2191	2194	2201	rVB7	3241	5302	0.17%	0.021%
70	15.930	2222	2226	2229	rVV4	7430	9879	0.31%	0.040%
71	15.978	2229	2234	2236	rVV5	9590	13877	0.44%	0.056%
72	16.030	2240	2243	2247	rVB6	4664	6207	0.20%	0.025%
73	16.125	2256	2259	2266	rBV6	5501	11794	0.38%	0.048%
74	16.536	2325	2329	2332	rBV6	6393	8740	0.28%	0.035%
75	16.760	2364	2367	2369	rBV2	8127	10125	0.32%	0.041%
76	16.913	2387	2393	2397	rVB7	7345	11647	0.37%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032423.D
 Acq On : 11 Oct 2021 16:22
 Operator : CG/JU
 Sample : M4029-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00R4

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	16.989	2400	2406	2411	rVV	2023877	2712292	86.46%	10.974%
78	17.030	2411	2413	2417	rVV	38967	46367	1.48%	0.188%
79	17.083	2417	2422	2435	rVV	737594	1058801	33.75%	4.284%
80	17.183	2435	2439	2444	rVB3	37587	48225	1.54%	0.195%
81	17.366	2468	2470	2472	rBV3	5263	5127	0.16%	0.021%
82	17.489	2488	2491	2493	rVB3	7326	7115	0.23%	0.029%
83	17.577	2501	2506	2507	rBV5	3528	4840	0.15%	0.020%
84	17.654	2516	2519	2525	rBV	32000	39948	1.27%	0.162%
85	17.877	2551	2557	2566	rVV3	91935	172073	5.49%	0.696%
86	17.942	2566	2568	2573	rVB	9016	13175	0.42%	0.053%
87	18.042	2582	2585	2591	rBV5	9042	14335	0.46%	0.058%
88	18.172	2602	2607	2610	rBV5	14465	18603	0.59%	0.075%
89	18.354	2635	2638	2641	rBV4	9835	12268	0.39%	0.050%
90	18.442	2651	2653	2659	rVB7	6183	10098	0.32%	0.041%
91	18.771	2706	2709	2713	rBV6	15885	25875	0.82%	0.105%
92	18.824	2713	2718	2723	rVB5	21167	35828	1.14%	0.145%
93	19.007	2746	2749	2751	rBV	11470	14963	0.48%	0.061%
94	19.042	2751	2755	2762	rVB	83129	112850	3.60%	0.457%
95	19.154	2771	2774	2779	rBV7	19276	27030	0.86%	0.109%
96	19.371	2806	2811	2826	rBV	1003224	1457234	46.45%	5.896%
97	20.860	3061	3064	3068	rBV4	75850	85941	2.74%	0.348%
98	21.154	3109	3114	3119	rBV	2436724	3048226	97.17%	12.333%
99	23.165	3451	3456	3470	rVB	759097	1475670	47.04%	5.971%
100	23.301	3473	3479	3492	rVB2	1744684	3136892	100.00%	12.692%




Sum of corrected areas: 24715469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032423.D
Acq On : 11 Oct 2021 16:22
Operator : CG/JU
Sample : M4029-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00R4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

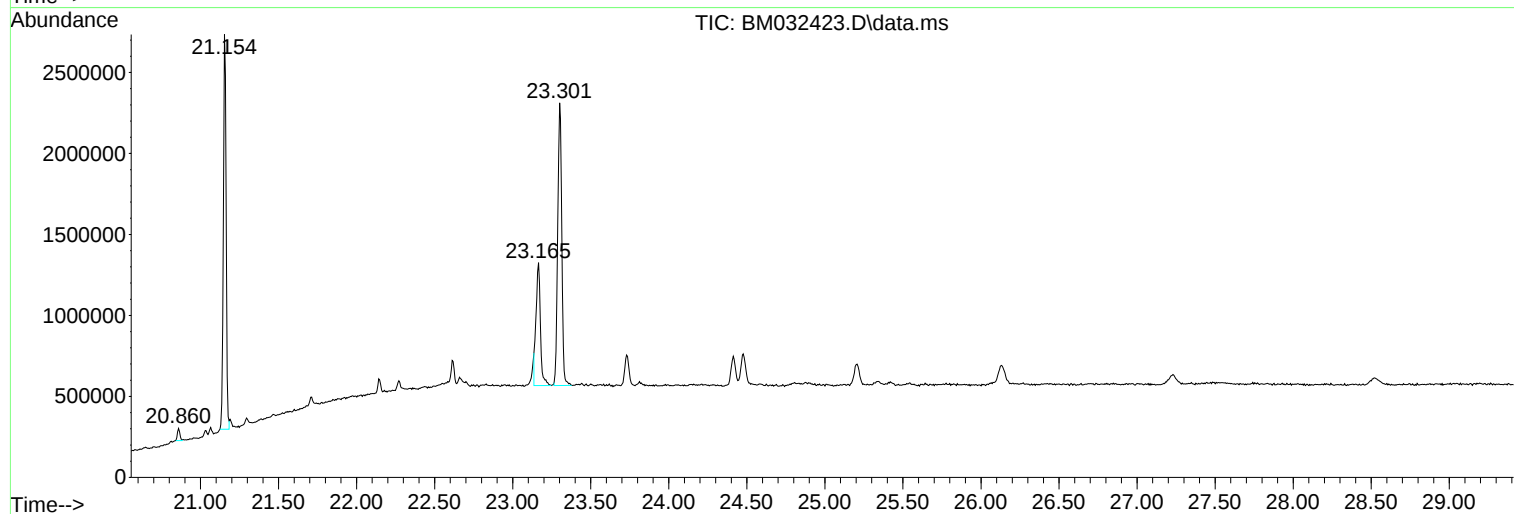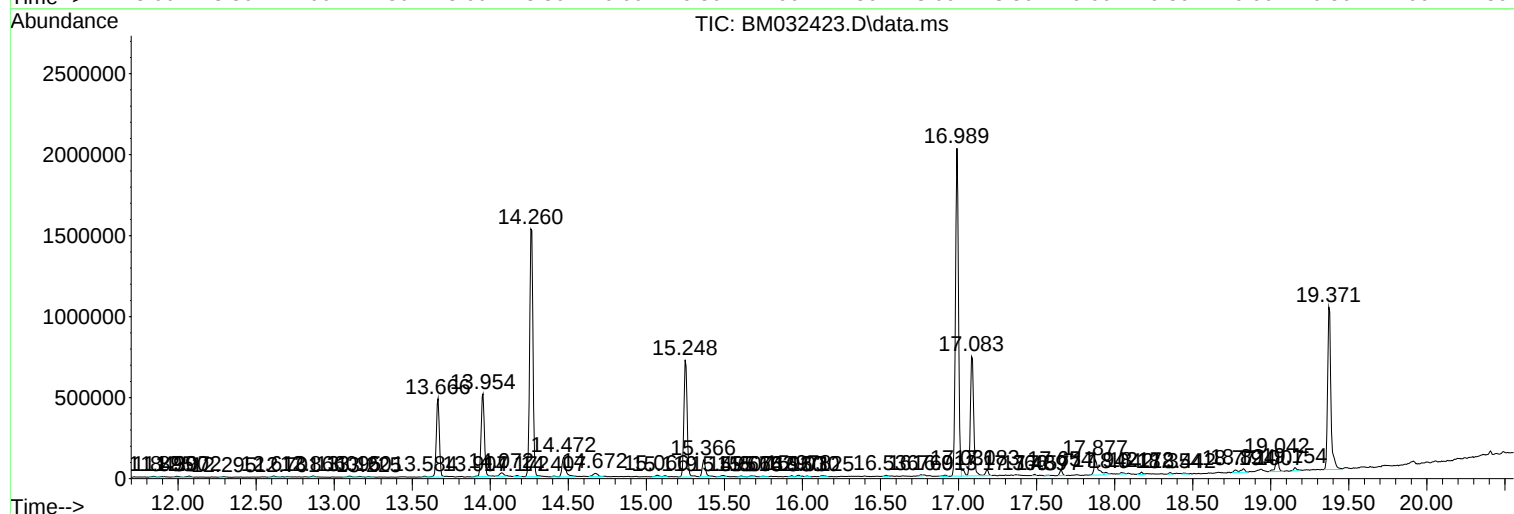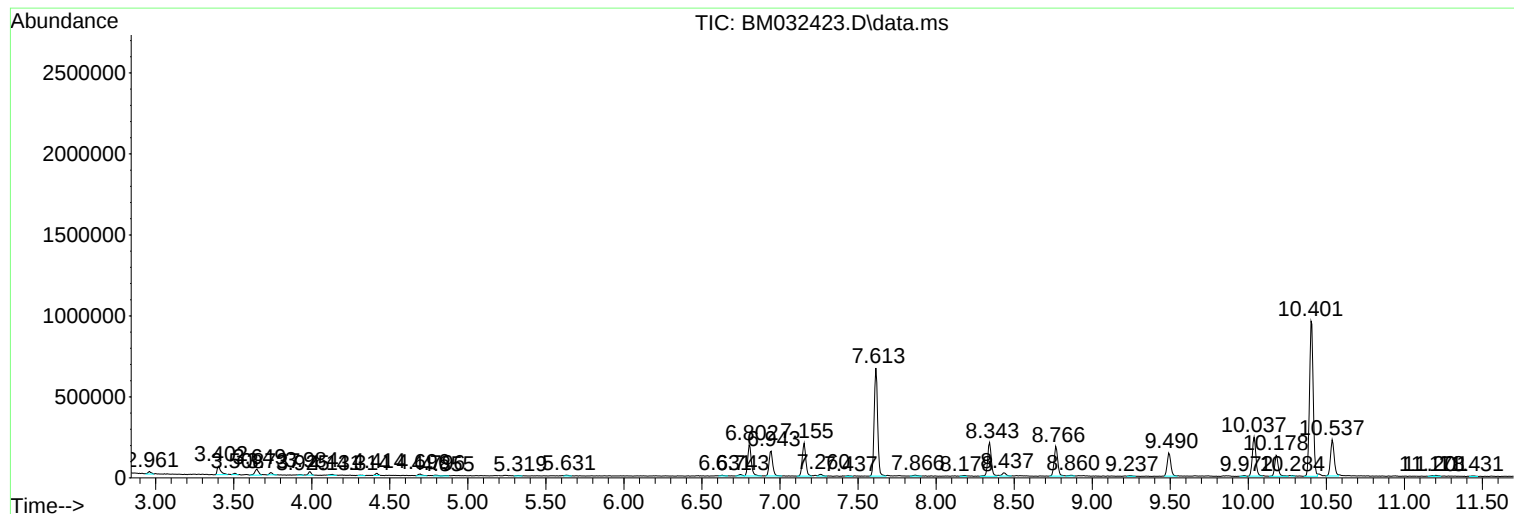

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032423.D
Acq On : 11 Oct 2021 16:22
Operator : CG/JU
Sample : M4029-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00R4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.178	2.65 ng/ul	207235	Naphthalene-d8	10.401

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

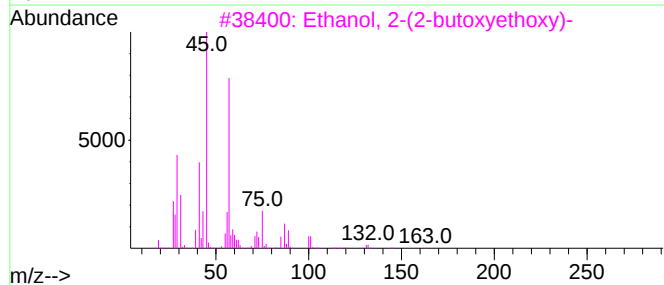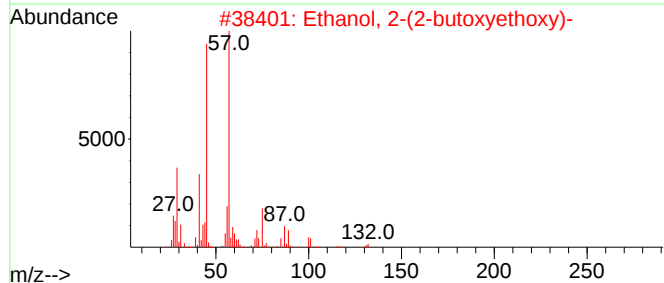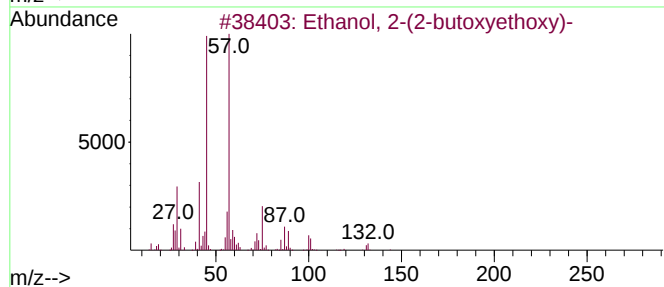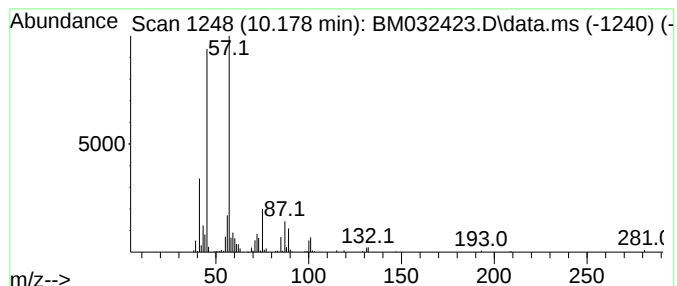

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032423.D
Acq On : 11 Oct 2021 16:22
Operator : CG/JU
Sample : M4029-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00R4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.178	2.6	ng/ul	207235	2	10.401	1563640	20.0