

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032425.D
 Acq On : 11 Oct 2021 18:12
 Operator : CG/JU
 Sample : PB139762BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.954	16	20	32	rVB	43633	66044	1.17%	0.122%
2	3.384	89	93	111	rBV	558755	853359	15.07%	1.581%
3	3.737	148	153	158	rBV	10685	14432	0.25%	0.027%
4	6.801	668	674	687	rBV	678986	1032606	18.24%	1.913%
5	6.942	691	698	711	rVB	538012	844788	14.92%	1.565%
6	7.154	726	734	745	rBV	687273	1073667	18.96%	1.990%
7	7.613	805	812	827	rBV	663070	1020975	18.03%	1.892%
8	8.342	929	936	946	rBV	914000	1392205	24.59%	2.580%
9	8.766	1000	1008	1024	rBV	687550	1088948	19.23%	2.018%
10	9.489	1125	1131	1143	rBV	584609	931021	16.44%	1.725%
11	10.036	1217	1224	1238	rBV	901297	1438130	25.40%	2.665%
12	10.401	1279	1286	1295	rBV	997272	1677357	29.62%	3.108%
13	10.536	1302	1309	1323	rBV	955444	1564399	27.63%	2.899%
14	11.995	1553	1557	1564	rVB	20394	31343	0.55%	0.058%
15	13.665	1835	1841	1855	rVB	1968586	2563863	45.28%	4.751%
16	13.954	1883	1890	1898	rBV	2049924	2952090	52.13%	5.470%
17	14.071	1905	1910	1918	rVB2	24868	48082	0.85%	0.089%
18	14.265	1936	1943	1960	rVB	1743916	2580776	45.58%	4.782%
19	14.471	1971	1978	1993	rBV	900928	1307224	23.09%	2.422%
20	14.671	2010	2012	2017	rVB6	4722	7917	0.14%	0.015%
21	15.254	2104	2111	2124	rBV	2710592	3801564	67.14%	7.044%
22	15.365	2124	2130	2146	rVV	875634	1217641	21.50%	2.256%
23	15.489	2147	2151	2157	rVB2	35177	50008	0.88%	0.093%
24	15.918	2221	2224	2229	rBV5	3863	6141	0.11%	0.011%
25	16.030	2239	2243	2247	rVB5	5311	7077	0.12%	0.013%
26	16.777	2366	2370	2375	rVB	8918	12639	0.22%	0.023%
27	16.989	2400	2406	2416	rBV	2340684	3213040	56.74%	5.954%
28	17.089	2416	2423	2443	rVV	3081905	4224078	74.60%	7.827%
29	17.653	2516	2519	2526	rVB9	4806	6541	0.12%	0.012%
30	17.877	2553	2557	2565	rBV2	37335	57053	1.01%	0.106%
31	18.942	2733	2738	2742	rBV2	34783	49742	0.88%	0.092%
32	19.006	2745	2749	2754	rBV	41161	56397	1.00%	0.105%
33	19.153	2771	2774	2780	rBV7	7825	16143	0.29%	0.030%
34	19.377	2806	2812	2821	rBV	3877290	4985351	88.04%	9.238%
35	21.153	3109	3114	3120	rBV	2977876	3732584	65.92%	6.916%
36	23.171	3448	3457	3468	rVB2	3034989	5662544	100.00%	10.493%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032425.D
Acq On : 11 Oct 2021 18:12
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Title : SVOA CALIBRATION

37	23.300	3473	3479	3488	rVB2	2278432	4014253	70.89%	7.438%
38	23.730	3549	3552	3561	rVB	211389	364375	6.43%	0.675%




Sum of corrected areas: 53966397

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032425.D
Acq On : 11 Oct 2021 18:12
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

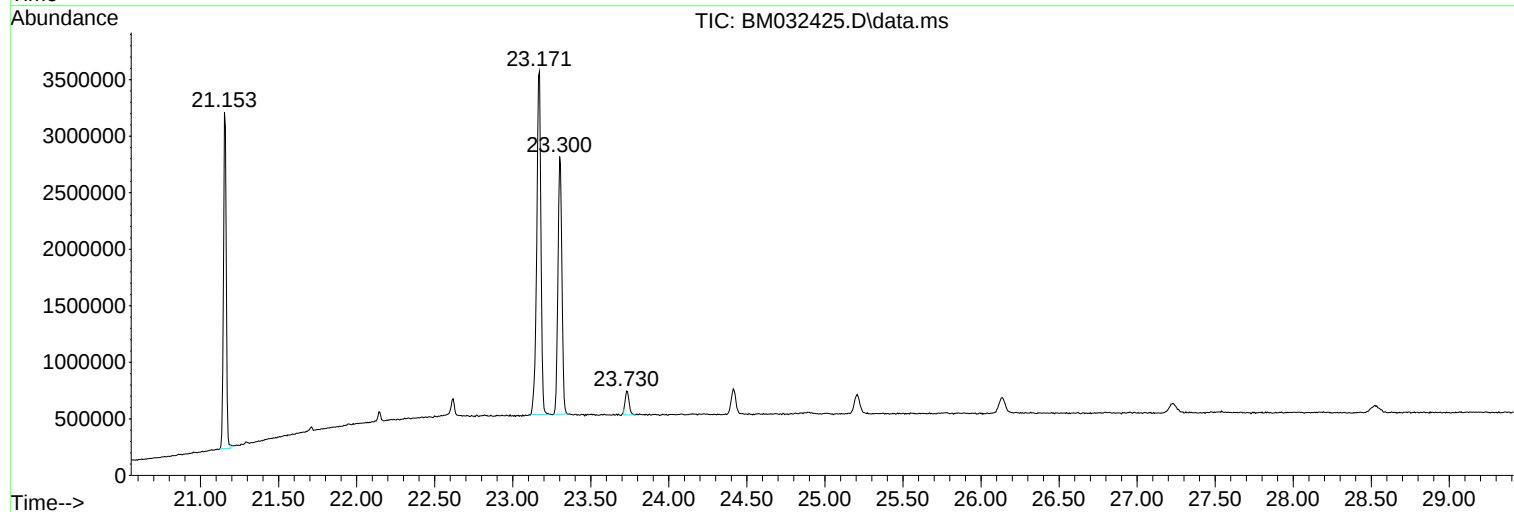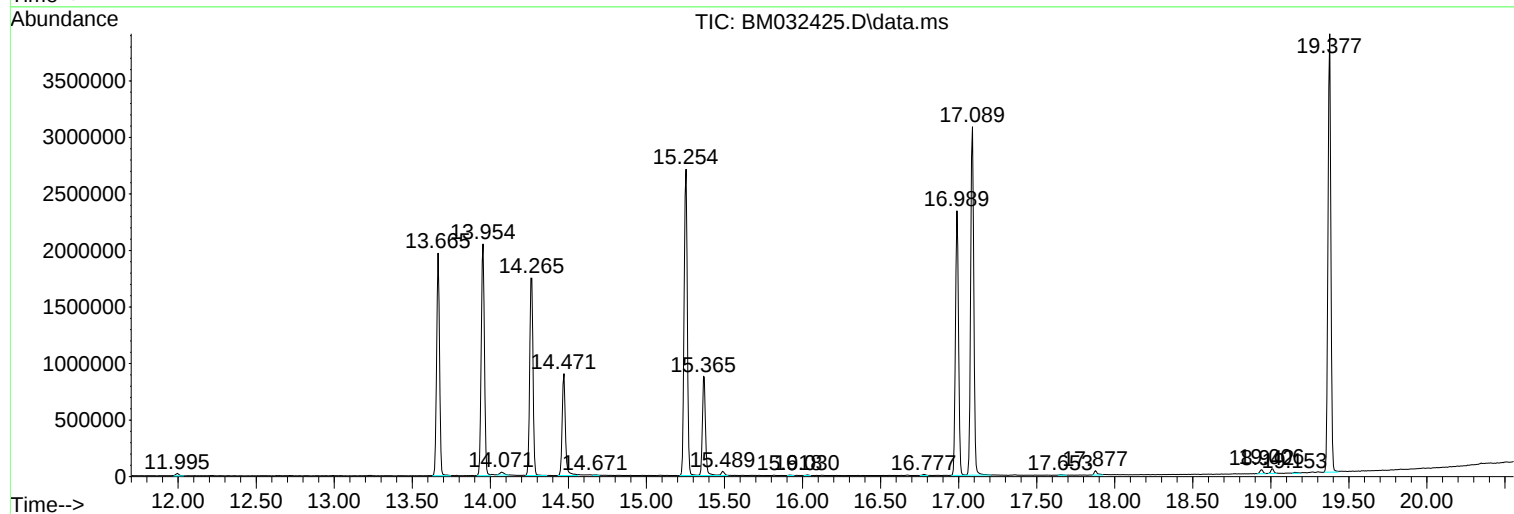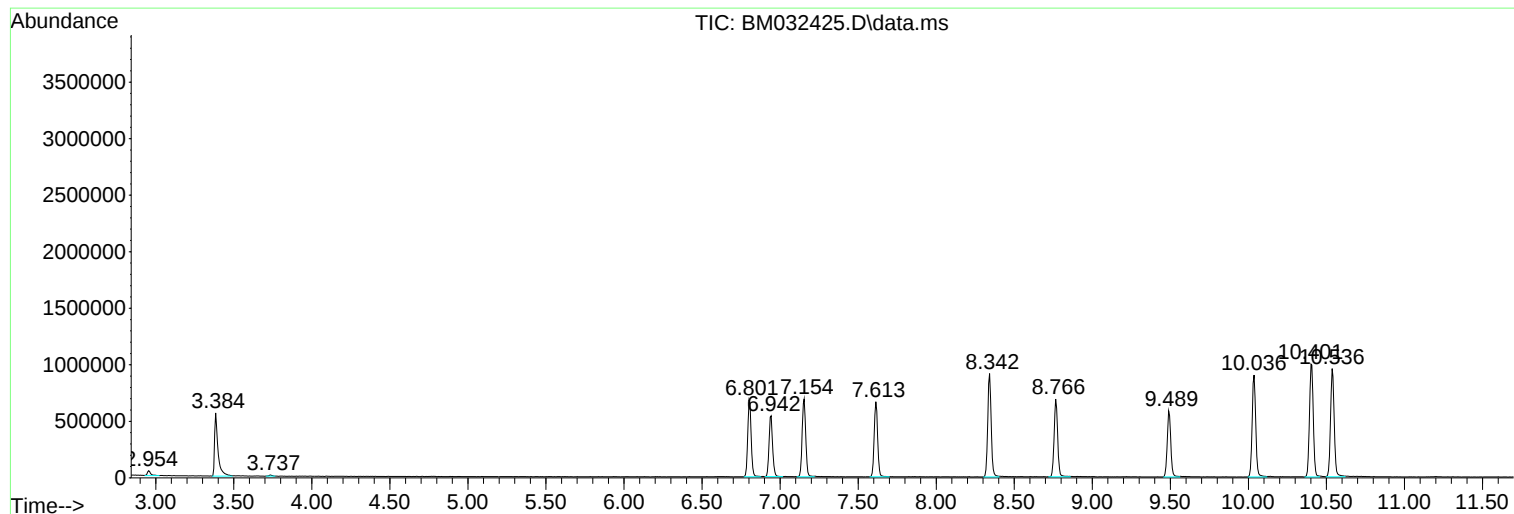

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032425.D
Acq On : 11 Oct 2021 18:12
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032425.D
Acq On : 11 Oct 2021 18:12
Operator : CG/JU
Sample : PB139762BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
