

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032429.D
 Acq On : 11 Oct 2021 20:38
 Operator : CG/JU
 Sample : M4029-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	17	20	25	rVB	19293	23303	0.57%	0.067%
2	3.396	91	95	111	rBV	106121	181907	4.45%	0.521%
3	3.502	111	113	118	rVB6	5497	6468	0.16%	0.019%
4	3.649	132	138	146	rVB	25713	45706	1.12%	0.131%
5	3.737	149	153	161	rVB2	11275	18604	0.46%	0.053%
6	3.984	191	195	200	rVB3	11254	14500	0.35%	0.042%
7	4.419	265	269	273	rVB4	5611	7125	0.17%	0.020%
8	4.690	311	315	324	rVB	8280	13544	0.33%	0.039%
9	5.190	397	400	403	rBV4	2821	4148	0.10%	0.012%
10	5.631	470	475	480	rBV7	4744	7127	0.17%	0.020%
11	6.584	631	637	639	rBV5	2380	4743	0.12%	0.014%
12	6.631	641	645	650	rVB6	3799	6313	0.15%	0.018%
13	6.743	661	664	666	rBV4	4547	5148	0.13%	0.015%
14	6.802	668	674	687	rVB	314847	485091	11.87%	1.390%
15	6.937	692	697	707	rBV	253267	395182	9.67%	1.133%
16	7.149	727	733	743	rBV	313203	503366	12.32%	1.443%
17	7.260	748	752	756	rVB2	5741	8159	0.20%	0.023%
18	7.431	779	781	788	rVB7	2461	4826	0.12%	0.014%
19	7.613	805	812	823	rBV	735744	1131339	27.69%	3.243%
20	7.690	823	825	830	rVB6	3408	5645	0.14%	0.016%
21	7.866	851	855	860	rVB6	4262	8568	0.21%	0.025%
22	8.178	904	908	911	rBV4	4316	5616	0.14%	0.016%
23	8.337	926	935	944	rBV	387915	629468	15.40%	1.804%
24	8.437	947	952	958	rVB2	15020	28590	0.70%	0.082%
25	8.766	999	1008	1017	rBV	309526	499261	12.22%	1.431%
26	9.243	1086	1089	1093	rVB4	2952	4577	0.11%	0.013%
27	9.490	1122	1131	1144	rBV	255754	415905	10.18%	1.192%
28	10.037	1217	1224	1235	rBV	390767	644210	15.77%	1.846%
29	10.178	1242	1248	1256	rBV	71564	108071	2.64%	0.310%
30	10.401	1278	1286	1299	rBV	1118336	1801624	44.09%	5.164%
31	10.537	1302	1309	1320	rVV	402887	663790	16.24%	1.903%
32	10.925	1372	1375	1380	rVB7	2912	4735	0.12%	0.014%
33	11.201	1416	1422	1428	rVB10	4074	8315	0.20%	0.024%
34	11.448	1458	1464	1468	rVB5	3464	6906	0.17%	0.020%
35	11.895	1536	1540	1542	rBV5	2950	4150	0.10%	0.012%
36	11.990	1551	1556	1563	rVB2	10231	18638	0.46%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032429.D
 Acq On : 11 Oct 2021 20:38
 Operator : CG/JU
 Sample : M4029-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	12.072	1565	1570	1574	rVV5	4090	7499	0.18%	0.021%
38	12.290	1600	1607	1611	rBV9	2495	4134	0.10%	0.012%
39	12.613	1658	1662	1669	rVB3	9276	14497	0.35%	0.042%
40	12.860	1700	1704	1712	rVB2	11286	18009	0.44%	0.052%
41	13.101	1740	1745	1748	rBV4	4854	7743	0.19%	0.022%
42	13.166	1751	1756	1759	rVV5	5511	9150	0.22%	0.026%
43	13.225	1763	1766	1769	rVB4	4195	4978	0.12%	0.014%
44	13.578	1823	1826	1831	rVB6	3817	5712	0.14%	0.016%
45	13.660	1834	1840	1847	rVV	849281	1177665	28.82%	3.375%
46	13.713	1847	1849	1854	rVB6	4862	6321	0.15%	0.018%
47	13.907	1877	1882	1883	rBV4	6500	6900	0.17%	0.020%
48	13.948	1883	1889	1900	rVV	938585	1347944	32.99%	3.864%
49	14.072	1903	1910	1920	rVV2	34137	89357	2.19%	0.256%
50	14.172	1923	1927	1933	rVB6	6520	11296	0.28%	0.032%
51	14.260	1935	1942	1955	rVV	1934321	2707584	66.26%	7.761%
52	14.466	1971	1977	1991	rBV	267949	416559	10.19%	1.194%
53	14.666	2005	2011	2018	rVB7	19969	41909	1.03%	0.120%
54	15.072	2072	2080	2084	rBV6	7275	16335	0.40%	0.047%
55	15.113	2084	2087	2096	rVB8	4470	7430	0.18%	0.021%
56	15.248	2104	2110	2125	rBV	1305712	1799264	44.03%	5.157%
57	15.366	2125	2130	2141	rBV	261531	362163	8.86%	1.038%
58	15.489	2146	2151	2155	rBV2	14257	19472	0.48%	0.056%
59	15.607	2168	2171	2175	rBV6	3597	4946	0.12%	0.014%
60	15.930	2220	2226	2230	rBV4	8903	16700	0.41%	0.048%
61	15.972	2230	2233	2236	rVB4	4860	6344	0.16%	0.018%
62	16.125	2256	2259	2261	rBV4	3838	6107	0.15%	0.018%
63	16.777	2367	2370	2374	rVB	8499	11022	0.27%	0.032%
64	16.913	2389	2393	2396	rVB6	3017	4336	0.11%	0.012%
65	16.989	2399	2406	2412	rBV	2419619	3316351	81.16%	9.505%
66	17.083	2416	2422	2434	rVV2	1400392	1936714	47.40%	5.551%
67	17.183	2434	2439	2444	rVB3	31763	43982	1.08%	0.126%
68	17.360	2463	2469	2471	rBV7	5843	10061	0.25%	0.029%
69	17.489	2486	2491	2494	rBV5	6267	8432	0.21%	0.024%
70	17.654	2516	2519	2524	rVB2	20988	23686	0.58%	0.068%
71	17.877	2548	2557	2565	rBV2	95805	165510	4.05%	0.474%
72	17.942	2566	2568	2573	rVB2	12610	15257	0.37%	0.044%
73	18.048	2582	2586	2590	rVB6	5852	9254	0.23%	0.027%
74	18.171	2604	2607	2610	rBV5	5401	6218	0.15%	0.018%
75	18.354	2636	2638	2642	rBV5	6280	6239	0.15%	0.018%
76	18.771	2705	2709	2713	rBV6	14969	24797	0.61%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032429.D
 Acq On : 11 Oct 2021 20:38
 Operator : CG/JU
 Sample : M4029-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S6

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	18.936	2735	2737	2745	rVB5	21979	27877	0.68%	0.080%
78	19.007	2745	2749	2751	rBV	23778	31802	0.78%	0.091%
79	19.036	2751	2754	2759	rVB	32343	41273	1.01%	0.118%
80	19.154	2771	2774	2778	rBV4	17860	20639	0.51%	0.059%
81	19.371	2806	2811	2824	rBV	1882734	2492723	61.00%	7.145%
82	20.860	3060	3064	3070	rBV2	155462	214234	5.24%	0.614%
83	21.154	3109	3114	3119	rBV	3111129	3790559	92.77%	10.865%
84	23.159	3449	3455	3466	rVB2	1422176	2761212	67.58%	7.914%
85	23.301	3473	3479	3496	rVB2	2377148	4086143	100.00%	11.712%




Sum of corrected areas: 34889007

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032429.D
Acq On : 11 Oct 2021 20:38
Operator : CG/JU
Sample : M4029-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

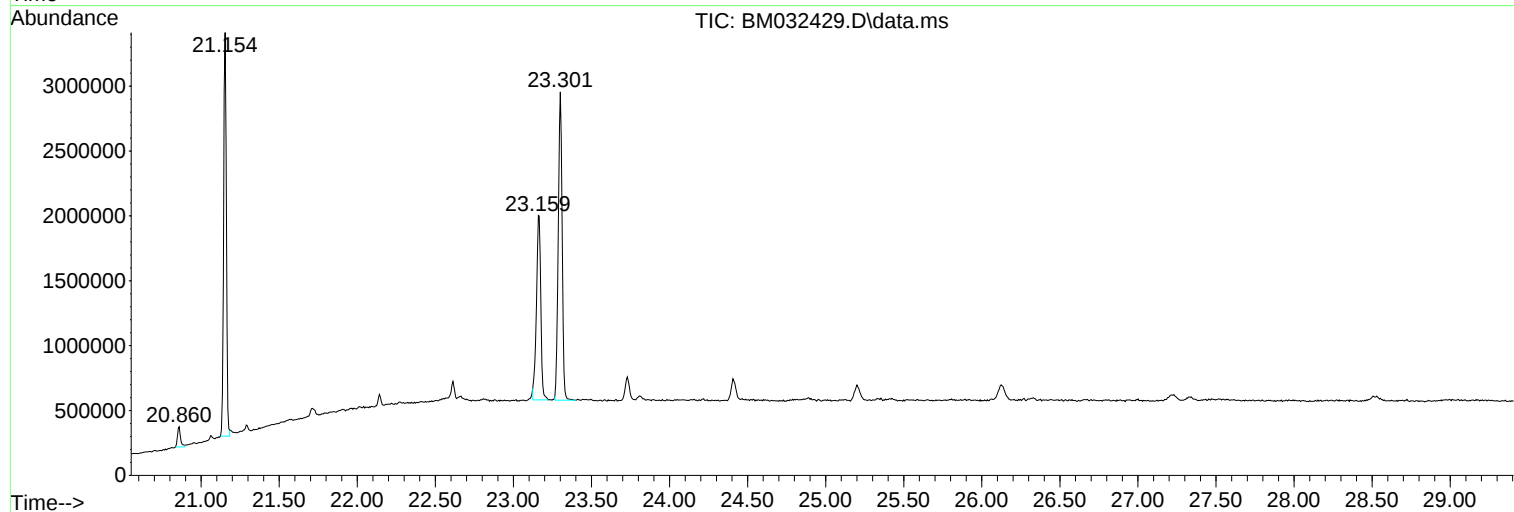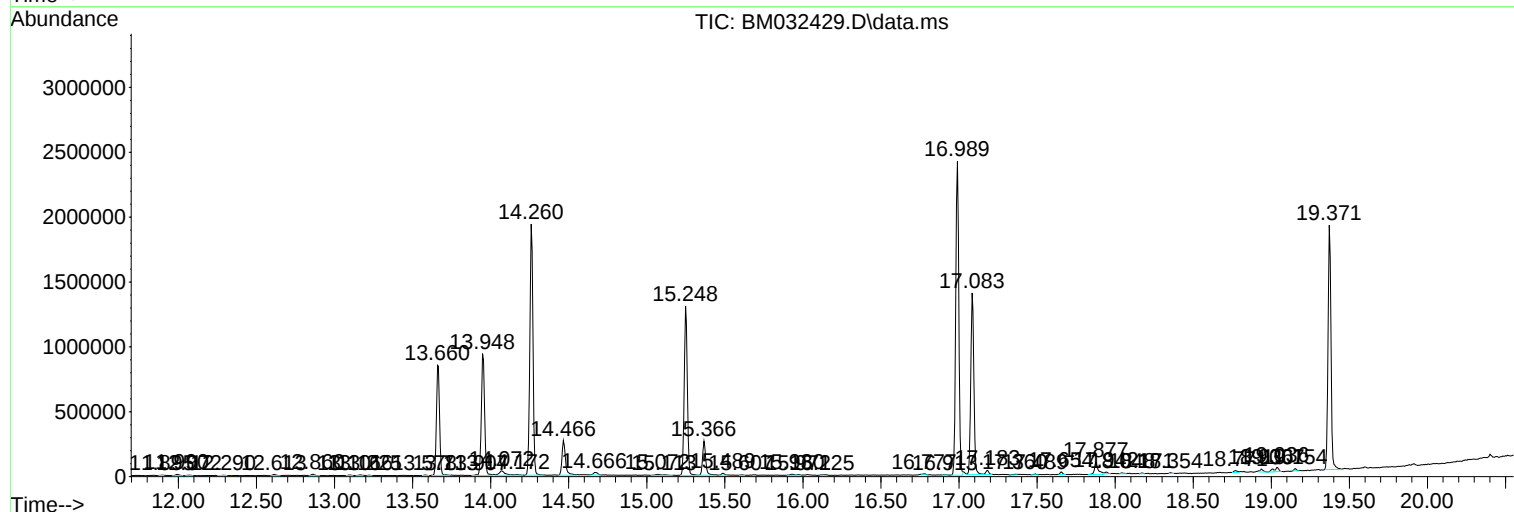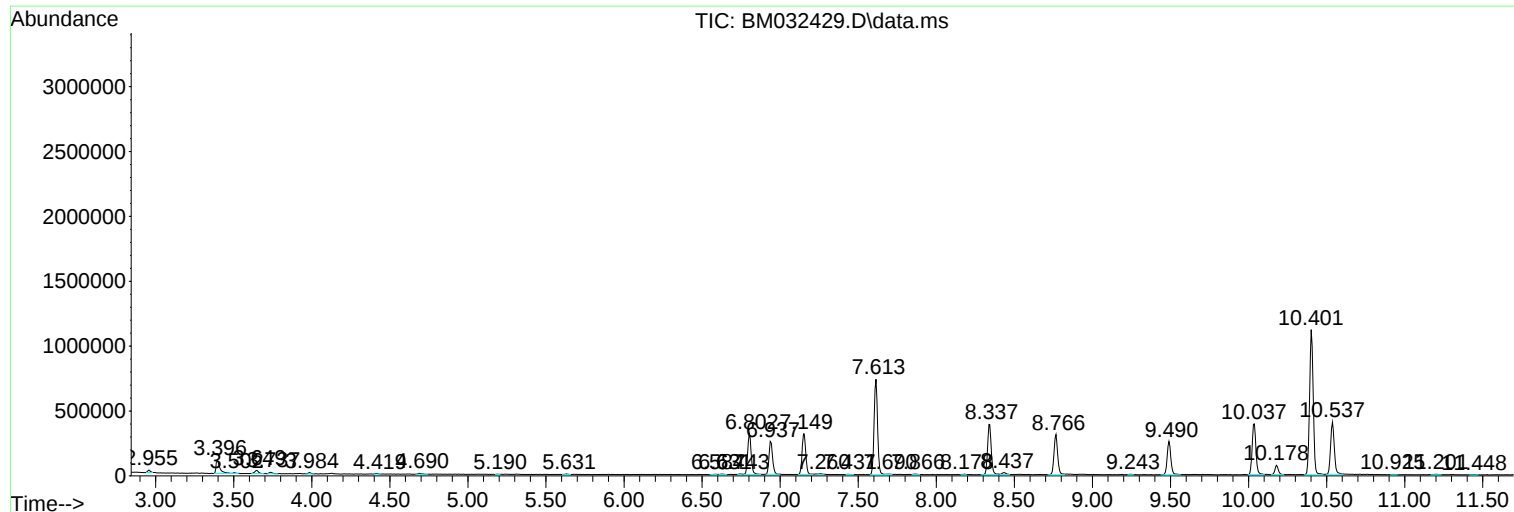

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032429.D
Acq On : 11 Oct 2021 20:38
Operator : CG/JU
Sample : M4029-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032429.D
Acq On : 11 Oct 2021 20:38
Operator : CG/JU
Sample : M4029-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
