

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032430.D
 Acq On : 11 Oct 2021 21:14
 Operator : CG/JU
 Sample : M4029-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.954	17	20	26	rVB	11629	17774	0.51%	0.060%
2	3.396	92	95	109	rVB	69105	118508	3.37%	0.401%
3	3.507	109	114	119	rVB	17427	24540	0.70%	0.083%
4	3.649	132	138	144	rBV	20110	34617	0.98%	0.117%
5	3.737	149	153	161	rVB	11344	19325	0.55%	0.065%
6	3.984	192	195	201	rVB8	6955	10963	0.31%	0.037%
7	4.690	312	315	321	rBV3	7480	11373	0.32%	0.038%
8	6.742	659	664	669	rBV	24606	40453	1.15%	0.137%
9	6.801	669	674	685	rVB	207196	328101	9.33%	1.110%
10	6.937	692	697	705	rBV	161622	255810	7.28%	0.866%
11	7.154	727	734	743	rBV	198939	321781	9.15%	1.089%
12	7.254	748	751	759	rVB5	10371	18183	0.52%	0.062%
13	7.613	805	812	821	rBV	539555	838336	23.85%	2.837%
14	8.336	926	935	943	rBV	222600	361013	10.27%	1.222%
15	8.431	943	951	958	rVV2	27355	64710	1.84%	0.219%
16	8.766	1000	1008	1021	rBV	201666	334761	9.52%	1.133%
17	9.489	1125	1131	1145	rVV	162450	272729	7.76%	0.923%
18	9.972	1207	1213	1217	rBV2	8107	11951	0.34%	0.040%
19	10.036	1217	1224	1234	rVV	272402	446486	12.70%	1.511%
20	10.178	1243	1248	1259	rVB	51572	88095	2.51%	0.298%
21	10.401	1279	1286	1292	rBV	849062	1373302	39.06%	4.648%
22	10.448	1292	1294	1302	rVB	15437	23151	0.66%	0.078%
23	10.536	1302	1309	1316	rBV	227896	377064	10.73%	1.276%
24	11.407	1451	1457	1460	rBV5	8461	16089	0.46%	0.054%
25	11.442	1460	1463	1467	rVV5	7952	13260	0.38%	0.045%
26	11.772	1515	1519	1524	rVB7	6154	10335	0.29%	0.035%
27	11.842	1527	1531	1537	rVB3	10866	17082	0.49%	0.058%
28	11.989	1549	1556	1562	rVB5	6493	12658	0.36%	0.043%
29	12.066	1564	1569	1570	rBV2	15259	18882	0.54%	0.064%
30	12.289	1602	1607	1613	rBV2	9992	17104	0.49%	0.058%
31	12.813	1690	1696	1700	rVV5	6538	13777	0.39%	0.047%
32	12.860	1700	1704	1710	rVB5	6615	12944	0.37%	0.044%
33	13.095	1738	1744	1751	rBV3	20434	33967	0.97%	0.115%
34	13.430	1791	1801	1806	rBV8	7044	20297	0.58%	0.069%
35	13.583	1822	1827	1831	rBV2	14102	21784	0.62%	0.074%
36	13.660	1831	1840	1847	rBV	559885	782548	22.26%	2.648%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032430.D
 Acq On : 11 Oct 2021 21:14
 Operator : CG/JU
 Sample : M4029-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	13.760	1853	1857	1861	rVB4	7268	10572	0.30%	0.036%
38	13.948	1884	1889	1900	rVV	632020	909226	25.86%	3.077%
39	14.071	1903	1910	1919	rVV	35093	72975	2.08%	0.247%
40	14.171	1922	1927	1932	rVB	19721	26454	0.75%	0.090%
41	14.260	1934	1942	1949	rBV	1481689	2053810	58.42%	6.951%
42	14.465	1971	1977	1995	rBV	197771	329232	9.36%	1.114%
43	14.595	1995	1999	2004	rVV7	8232	17816	0.51%	0.060%
44	14.660	2005	2010	2018	rVV5	21458	51645	1.47%	0.175%
45	14.736	2018	2023	2027	rVB3	8857	14410	0.41%	0.049%
46	15.060	2073	2078	2084	rBV6	9850	22312	0.63%	0.076%
47	15.118	2084	2088	2094	rVB2	21275	26637	0.76%	0.090%
48	15.248	2103	2110	2116	rBV	881008	1207984	34.36%	4.088%
49	15.301	2116	2119	2123	rVB4	14543	19113	0.54%	0.065%
50	15.365	2124	2130	2138	rBV	196431	271614	7.73%	0.919%
51	15.607	2165	2171	2178	rVB7	9422	22337	0.64%	0.076%
52	15.742	2187	2194	2200	rVB6	8473	21827	0.62%	0.074%
53	15.824	2203	2208	2213	rBV9	6318	12255	0.35%	0.041%
54	15.930	2221	2226	2230	rBV	61034	86186	2.45%	0.292%
55	15.971	2230	2233	2237	rVV2	29766	41258	1.17%	0.140%
56	16.301	2286	2289	2295	rVV6	5478	11347	0.32%	0.038%
57	16.536	2321	2329	2332	rBV6	13015	22803	0.65%	0.077%
58	16.654	2344	2349	2351	rBV5	10048	17375	0.49%	0.059%
59	16.730	2356	2362	2363	rVV5	7264	12883	0.37%	0.044%
60	16.754	2363	2366	2373	rVV3	25118	48837	1.39%	0.165%
61	16.806	2373	2375	2380	rVB	15567	22390	0.64%	0.076%
62	16.889	2386	2389	2396	rVB8	13466	19757	0.56%	0.067%
63	16.989	2397	2406	2410	rBV	1866935	2513931	71.51%	8.508%
64	17.030	2410	2413	2417	rVV	191911	256598	7.30%	0.868%
65	17.083	2417	2422	2434	rVV2	899087	1307224	37.18%	4.424%
66	17.177	2435	2438	2444	rVB5	21663	34185	0.97%	0.116%
67	17.301	2456	2459	2463	rVB2	10174	12653	0.36%	0.043%
68	17.383	2470	2473	2478	rVB	12422	16989	0.48%	0.057%
69	17.483	2487	2490	2496	rBV3	23211	33625	0.96%	0.114%
70	17.565	2501	2504	2507	rBV5	9681	11616	0.33%	0.039%
71	17.653	2515	2519	2524	rVB6	20689	27095	0.77%	0.092%
72	17.759	2534	2537	2540	rVB4	10773	11663	0.33%	0.039%
73	17.877	2549	2557	2560	rBV2	140502	241479	6.87%	0.817%
74	17.983	2572	2575	2580	rVB2	8988	10419	0.30%	0.035%
75	18.048	2581	2586	2590	rBV2	45412	79483	2.26%	0.269%
76	18.083	2590	2592	2599	rVB	28519	39575	1.13%	0.134%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032430.D
 Acq On : 11 Oct 2021 21:14
 Operator : CG/JU
 Sample : M4029-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	18.171	2603	2607	2610	rBV2	30605	38285	1.09%	0.130%
78	18.248	2618	2620	2624	rVB4	9569	11259	0.32%	0.038%
79	18.353	2635	2638	2641	rBV	34838	40840	1.16%	0.138%
80	18.389	2641	2644	2648	rVB4	15890	21709	0.62%	0.073%
81	18.606	2678	2681	2685	rBV6	11542	14075	0.40%	0.048%
82	18.659	2687	2690	2693	rBV2	12405	17315	0.49%	0.059%
83	18.777	2705	2710	2713	rBV2	43591	74619	2.12%	0.253%
84	18.912	2730	2733	2736	rBV4	25573	40823	1.16%	0.138%
85	19.036	2750	2754	2760	rVB	599242	786234	22.36%	2.661%
86	19.153	2771	2774	2777	rVB3	27699	25229	0.72%	0.085%
87	19.283	2794	2796	2806	rVB4	19577	35948	1.02%	0.122%
88	19.371	2806	2811	2814	rBV	1350751	1825740	51.93%	6.179%
89	19.400	2814	2816	2823	rVB	542920	619649	17.63%	2.097%
90	19.577	2844	2846	2853	rVB2	25701	38178	1.09%	0.129%
91	19.718	2867	2870	2872	rBV	36027	46837	1.33%	0.159%
92	19.895	2897	2900	2906	rVB3	80494	127169	3.62%	0.430%
93	19.995	2914	2917	2921	rBV	50199	59007	1.68%	0.200%
94	20.642	3024	3027	3033	rVB2	48050	61112	1.74%	0.207%
95	20.859	3060	3064	3067	rBV2	144880	189557	5.39%	0.642%
96	21.153	3107	3114	3118	rBV	2511597	3515700	100.00%	11.898%
97	21.189	3118	3120	3128	rVB	351895	387625	11.03%	1.312%
98	22.659	3366	3370	3375	rBV	430885	795199	22.62%	2.691%
99	23.165	3451	3456	3460	rVB2	822433	1286041	36.58%	4.352%
100	23.300	3473	3479	3485	rBV2	1838538	3136824	89.22%	10.616%




Sum of corrected areas: 29548317

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032430.D
Acq On : 11 Oct 2021 21:14
Operator : CG/JU
Sample : M4029-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

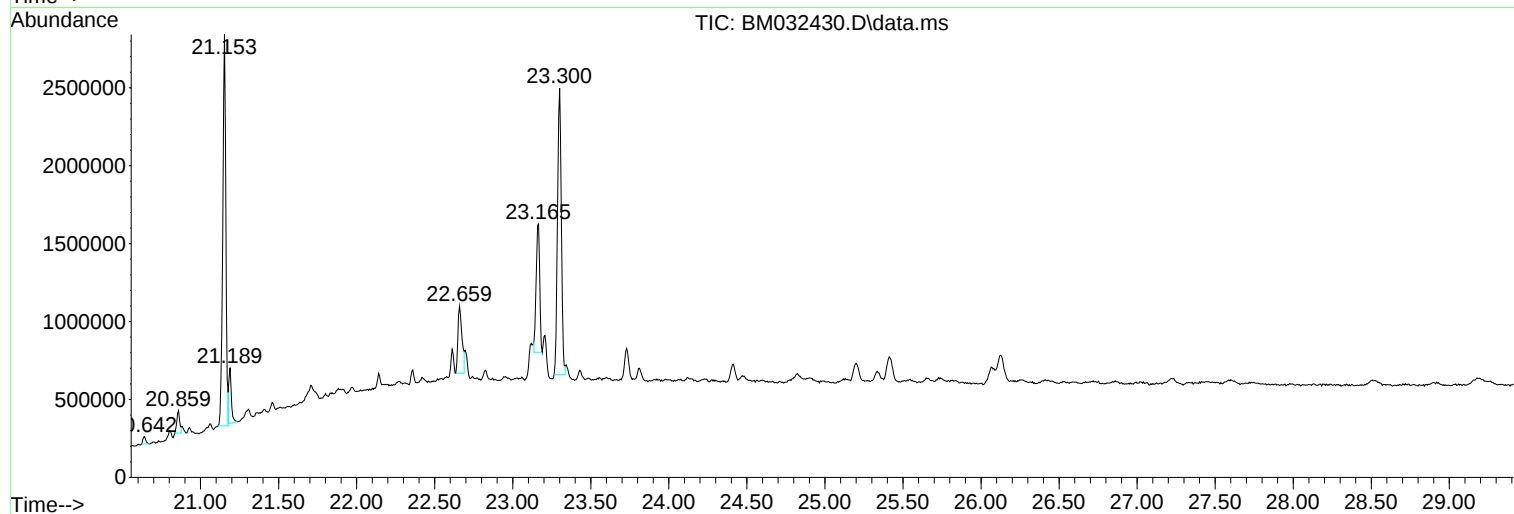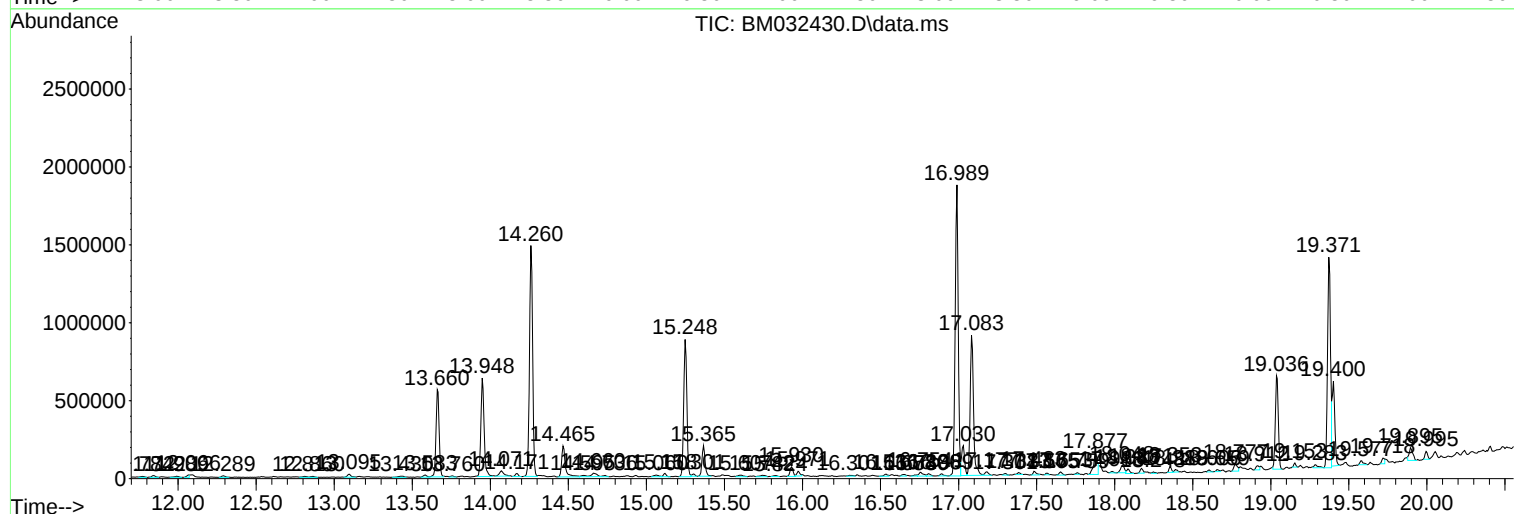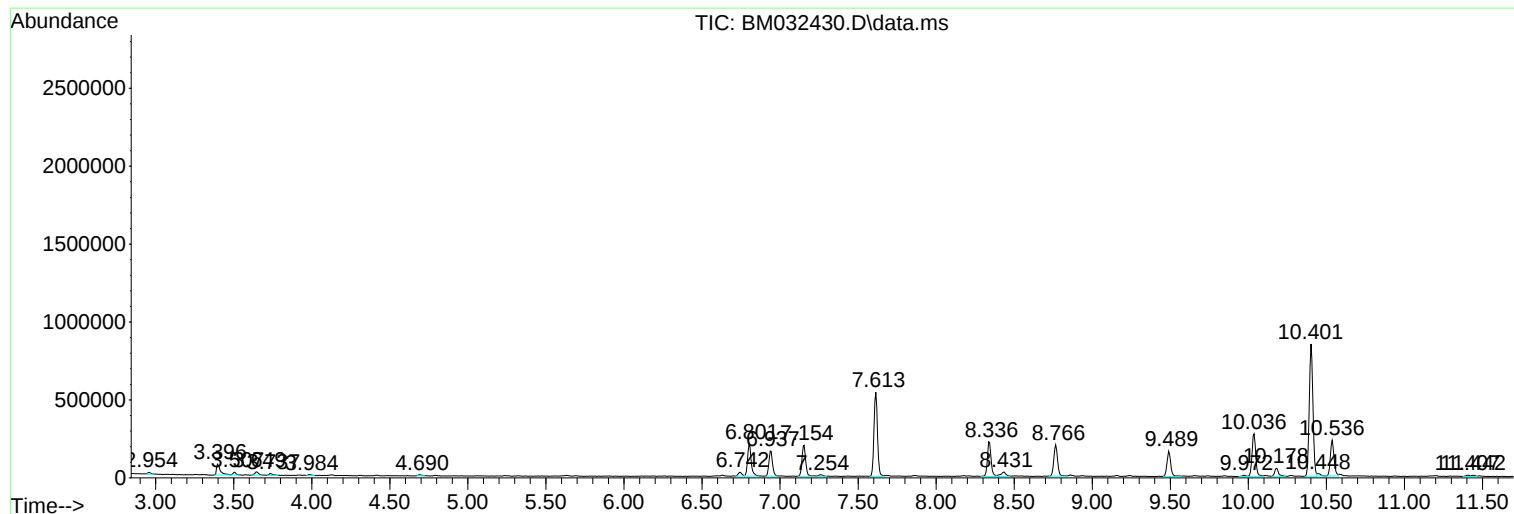

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032430.D
Acq On : 11 Oct 2021 21:14
Operator : CG/JU
Sample : M4029-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032430.D
Acq On : 11 Oct 2021 21:14
Operator : CG/JU
Sample : M4029-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
