

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032435.D
 Acq On : 12 Oct 2021 00:15
 Operator : CG/JU
 Sample : M4029-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	17	20	26	rBV	15918	21752	0.51%	0.060%
2	3.254	69	71	77	rBV5	4805	7739	0.18%	0.021%
3	3.396	91	95	106	rBV	109696	188940	4.45%	0.523%
4	3.502	111	113	119	rVB	10210	15542	0.37%	0.043%
5	3.643	132	137	147	rVB	25711	48294	1.14%	0.134%
6	3.737	149	153	158	rVV	18213	26130	0.62%	0.072%
7	3.925	182	185	189	rBV6	3246	6360	0.15%	0.018%
8	4.125	214	219	225	rVB8	4481	9892	0.23%	0.027%
9	4.690	311	315	325	rVB4	11705	22641	0.53%	0.063%
10	5.307	416	420	422	rBV5	3434	5427	0.13%	0.015%
11	5.631	473	475	480	rVB5	2653	4440	0.10%	0.012%
12	6.307	584	590	595	rVB2	13120	21000	0.49%	0.058%
13	6.584	631	637	640	rBV7	4152	8032	0.19%	0.022%
14	6.631	640	645	648	rVB7	4077	7152	0.17%	0.020%
15	6.743	660	664	668	rBV7	4148	7329	0.17%	0.020%
16	6.801	668	674	688	rVB	320206	511093	12.03%	1.414%
17	6.937	691	697	706	rBV	249207	386749	9.11%	1.070%
18	7.148	727	733	744	rBV	318840	509637	12.00%	1.410%
19	7.225	744	746	748	rVV3	5208	6162	0.15%	0.017%
20	7.260	748	752	759	rVB6	8686	15380	0.36%	0.043%
21	7.613	805	812	821	rBV	816650	1256152	29.57%	3.476%
22	7.684	822	824	832	rVB6	5492	9380	0.22%	0.026%
23	7.848	848	852	857	rBV7	9096	17584	0.41%	0.049%
24	8.178	904	908	912	rBV5	4466	5912	0.14%	0.016%
25	8.337	927	935	942	rBV	382524	612686	14.42%	1.696%
26	8.395	942	945	948	rVV3	14132	24849	0.59%	0.069%
27	8.437	948	952	960	rVB	16464	28554	0.67%	0.079%
28	8.766	999	1008	1016	rBV	287626	466950	10.99%	1.292%
29	8.948	1036	1039	1043	rVB6	4177	5312	0.13%	0.015%
30	9.236	1085	1088	1093	rVB6	4155	6773	0.16%	0.019%
31	9.489	1123	1131	1138	rBV	237553	380190	8.95%	1.052%
32	10.031	1217	1223	1235	rBV	387730	646064	15.21%	1.788%
33	10.178	1243	1248	1259	rVB	83847	132768	3.13%	0.367%
34	10.401	1279	1286	1301	rBV	1229108	1990934	46.87%	5.510%
35	10.536	1302	1309	1323	rVV	372009	609082	14.34%	1.686%
36	10.930	1372	1376	1380	rVB7	4125	6111	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032435.D
 Acq On : 12 Oct 2021 00:15
 Operator : CG/JU
 Sample : M4029-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	11.842	1527	1531	1535	rVB5	2994	4461	0.11%	0.012%
38	11.930	1535	1546	1551	rBV3	13779	30700	0.72%	0.085%
39	11.989	1553	1556	1560	rVB4	6768	10286	0.24%	0.028%
40	12.072	1565	1570	1576	rVB6	6046	10212	0.24%	0.028%
41	12.289	1603	1607	1611	rBV5	3242	5726	0.13%	0.016%
42	12.613	1657	1662	1667	rBV6	4627	8601	0.20%	0.024%
43	12.866	1701	1705	1709	rVB6	6572	8700	0.20%	0.024%
44	13.101	1738	1745	1750	rBV6	8051	15180	0.36%	0.042%
45	13.166	1752	1756	1762	rVV5	6497	11665	0.27%	0.032%
46	13.224	1762	1766	1770	rVB5	2567	4561	0.11%	0.013%
47	13.577	1823	1826	1831	rVB6	4820	6579	0.15%	0.018%
48	13.660	1831	1840	1848	rBV	816578	1133799	26.69%	3.138%
49	13.713	1848	1849	1853	rVV4	5905	8023	0.19%	0.022%
50	13.748	1853	1855	1862	rVB6	2478	4813	0.11%	0.013%
51	13.907	1878	1882	1883	rBV4	5026	5191	0.12%	0.014%
52	13.948	1883	1889	1901	rVV	890697	1250092	29.43%	3.460%
53	14.071	1905	1910	1923	rVV3	30990	78561	1.85%	0.217%
54	14.166	1924	1926	1930	rVB5	3975	4802	0.11%	0.013%
55	14.260	1935	1942	1951	rBV	2087296	2948332	69.41%	8.160%
56	14.407	1961	1967	1971	rBV8	5915	10803	0.25%	0.030%
57	14.466	1971	1977	1991	rBV	289672	446752	10.52%	1.236%
58	14.677	2008	2013	2020	rVB10	15001	27749	0.65%	0.077%
59	15.065	2073	2079	2085	rBV5	6812	15951	0.38%	0.044%
60	15.118	2085	2088	2091	rVB4	4971	5791	0.14%	0.016%
61	15.248	2104	2110	2117	rBV	1279015	1687090	39.72%	4.669%
62	15.365	2124	2130	2138	rBV	273412	367701	8.66%	1.018%
63	15.489	2146	2151	2159	rVB2	13989	22518	0.53%	0.062%
64	15.607	2169	2171	2178	rVB7	3725	5718	0.13%	0.016%
65	15.683	2178	2184	2188	rBV7	4906	8133	0.19%	0.023%
66	15.971	2230	2233	2236	rBV5	4331	5199	0.12%	0.014%
67	16.030	2241	2243	2247	rVB5	4465	5827	0.14%	0.016%
68	16.130	2255	2260	2261	rBV4	3023	4843	0.11%	0.013%
69	16.248	2276	2280	2283	rBV5	3360	4668	0.11%	0.013%
70	16.783	2364	2371	2373	rBV3	9649	16784	0.40%	0.046%
71	16.912	2389	2393	2397	rVB4	3531	4612	0.11%	0.013%
72	16.989	2399	2406	2412	rBV	2592096	3575964	84.19%	9.897%
73	17.083	2416	2422	2434	rVV	1385675	1865100	43.91%	5.162%
74	17.177	2434	2438	2442	rVB3	38872	51695	1.22%	0.143%
75	17.365	2467	2470	2472	rBV4	4161	4387	0.10%	0.012%
76	17.559	2499	2503	2505	rBV4	2792	4278	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032435.D
 Acq On : 12 Oct 2021 00:15
 Operator : CG/JU
 Sample : M4029-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	17.654	2515	2519	2522	rBV4	14852	16804	0.40%	0.047%
78	17.877	2551	2557	2560	rBV2	71663	97586	2.30%	0.270%
79	17.942	2565	2568	2572	rVB	10530	14439	0.34%	0.040%
80	18.048	2583	2586	2592	rVB7	5146	8068	0.19%	0.022%
81	18.171	2604	2607	2610	rBV5	6028	5618	0.13%	0.016%
82	18.359	2636	2639	2642	rVB4	5797	8523	0.20%	0.024%
83	18.653	2687	2689	2695	rVB7	5195	8327	0.20%	0.023%
84	18.771	2704	2709	2713	rBV8	12847	22661	0.53%	0.063%
85	18.936	2734	2737	2742	rVB3	17941	22559	0.53%	0.062%
86	19.006	2744	2749	2751	rBV2	20576	28593	0.67%	0.079%
87	19.036	2751	2754	2759	rVB	52330	66568	1.57%	0.184%
88	19.153	2771	2774	2776	rBV3	14262	14551	0.34%	0.040%
89	19.371	2805	2811	2825	rBV	1849894	2499349	58.84%	6.917%
90	19.759	2874	2877	2884	rVB3	29665	38844	0.91%	0.108%
91	20.142	2939	2942	2948	rBV2	58020	70845	1.67%	0.196%
92	20.853	3060	3063	3070	rBV3	75465	102460	2.41%	0.284%
93	21.147	3108	3113	3118	rBV	3190280	4040720	95.13%	11.183%
94	23.159	3448	3455	3467	rVB	1456714	2733498	64.35%	7.565%
95	23.294	3472	3478	3491	rVB2	2432311	4247569	100.00%	11.755%
96	23.724	3548	3551	3560	rVB	227287	364251	8.58%	1.008%




Sum of corrected areas: 36132672

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032435.D
Acq On : 12 Oct 2021 00:15
Operator : CG/JU
Sample : M4029-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

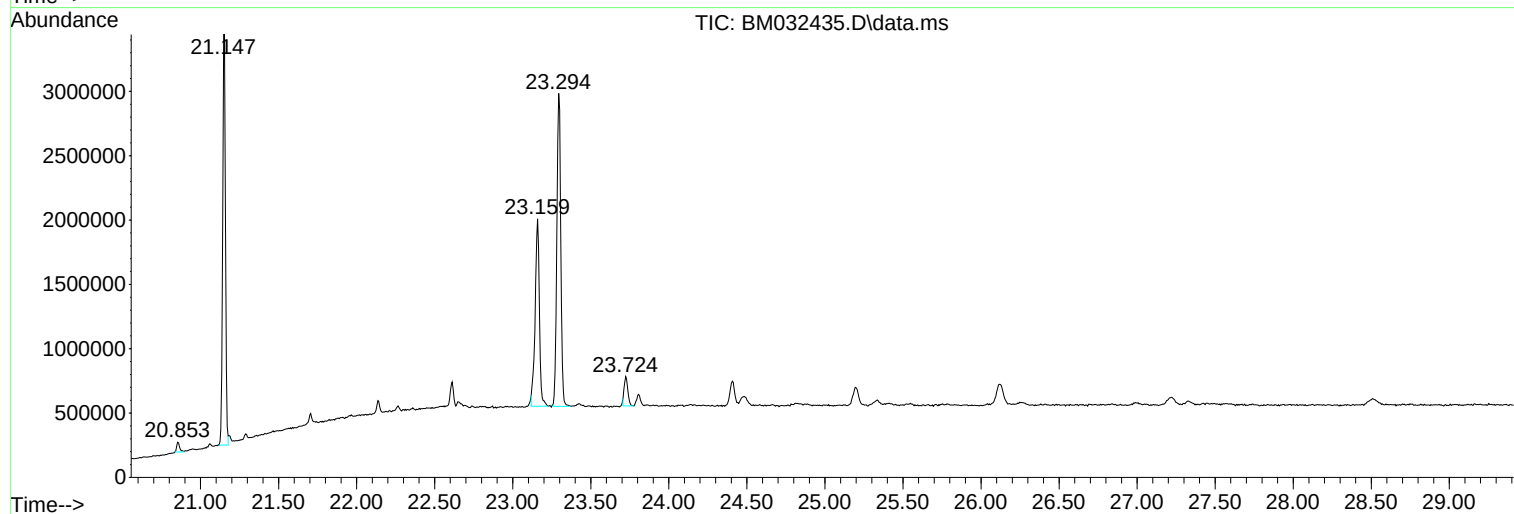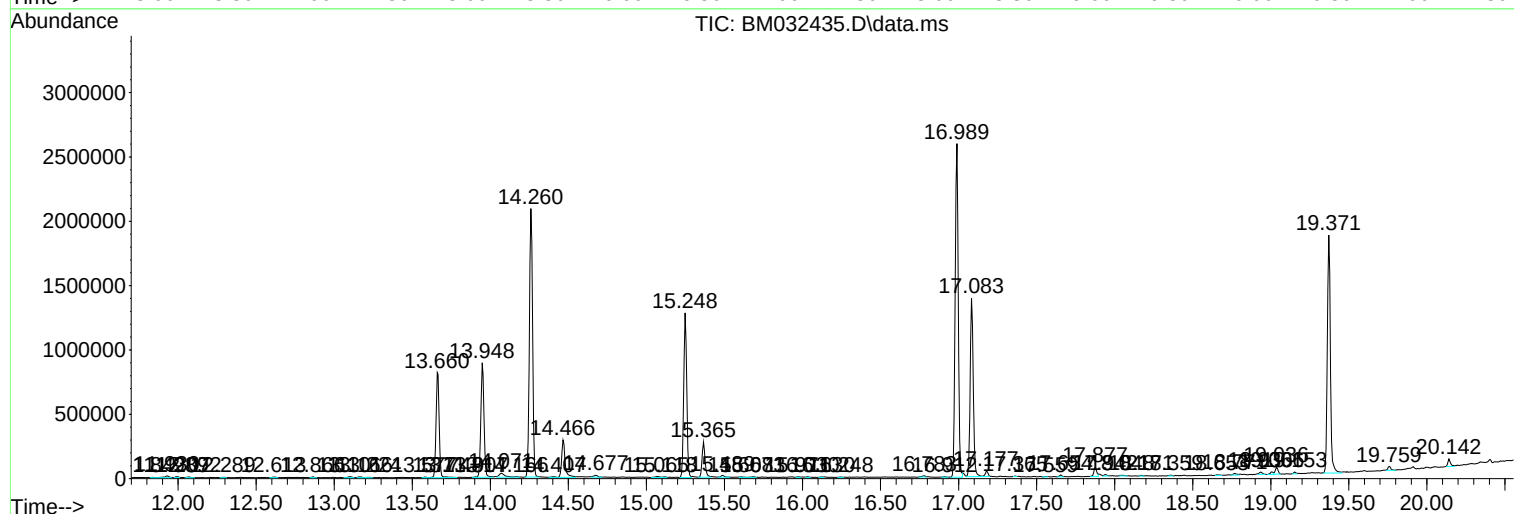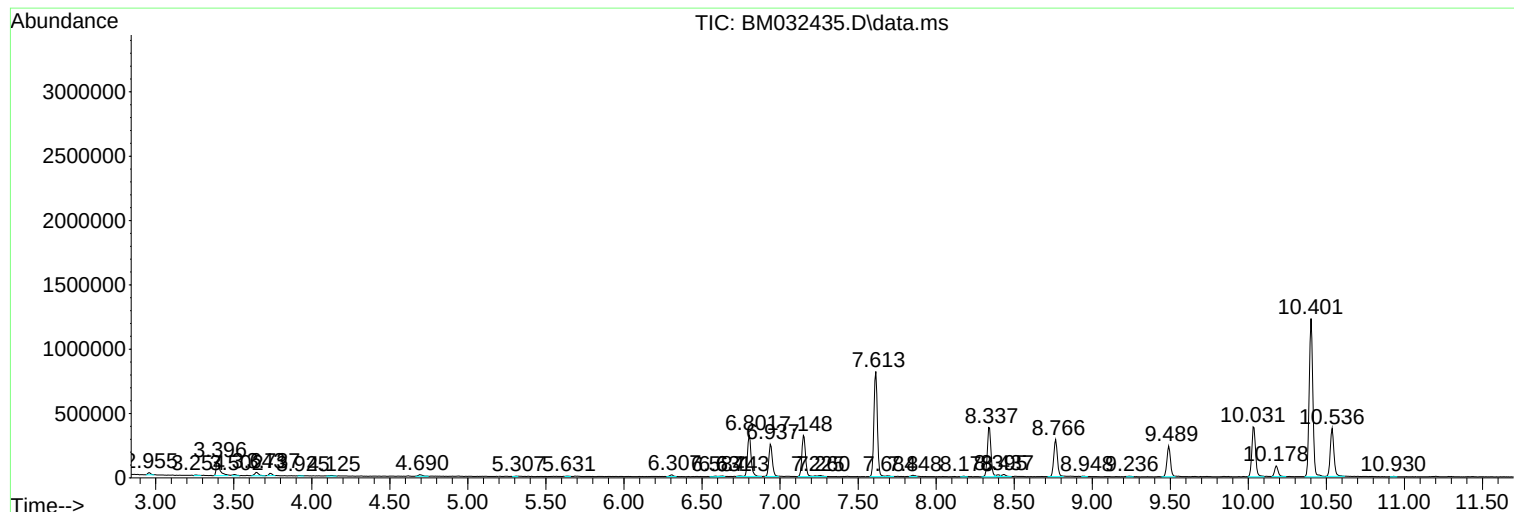

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032435.D
Acq On : 12 Oct 2021 00:15
Operator : CG/JU
Sample : M4029-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032435.D
Acq On : 12 Oct 2021 00:15
Operator : CG/JU
Sample : M4029-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
