

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032437.D
 Acq On : 12 Oct 2021 01:27
 Operator : CG/JU
 Sample : M4029-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	17	20	24	rBV	12367	15601	0.41%	0.049%
2	3.060	35	38	41	rBV5	3049	5108	0.13%	0.016%
3	3.396	92	95	110	rBV	90677	159346	4.14%	0.496%
4	3.649	133	138	144	rBV	23001	39260	1.02%	0.122%
5	3.731	149	152	157	rBV	18008	24379	0.63%	0.076%
6	3.984	190	195	200	rVB8	4784	7446	0.19%	0.023%
7	4.125	216	219	225	rVB8	3933	6047	0.16%	0.019%
8	4.413	264	268	269	rBV4	4059	4439	0.12%	0.014%
9	4.690	311	315	319	rVB	7424	10801	0.28%	0.034%
10	5.425	436	440	442	rBV5	2569	4103	0.11%	0.013%
11	5.631	470	475	480	rBV7	3236	5606	0.15%	0.017%
12	5.701	482	487	491	rVB7	2302	3906	0.10%	0.012%
13	6.584	635	637	642	rBV6	2634	5359	0.14%	0.017%
14	6.625	642	644	650	rVB7	4819	6428	0.17%	0.020%
15	6.737	660	663	668	rBV6	2741	4708	0.12%	0.015%
16	6.801	668	674	686	rVV	259470	412349	10.72%	1.282%
17	6.937	689	697	708	rBV	208702	333433	8.67%	1.037%
18	7.148	727	733	743	rBV	257257	412455	10.72%	1.283%
19	7.260	747	752	755	rVB6	5208	7868	0.20%	0.024%
20	7.431	777	781	786	rBV7	3222	5709	0.15%	0.018%
21	7.613	805	812	821	rBV	652044	1014902	26.38%	3.156%
22	7.866	849	855	859	rBV7	7104	14209	0.37%	0.044%
23	8.337	926	935	946	rBV	334501	533617	13.87%	1.659%
24	8.431	946	951	958	rVB	14232	25900	0.67%	0.081%
25	8.766	1001	1008	1019	rVV	255127	410244	10.66%	1.276%
26	8.937	1035	1037	1043	rVB6	3620	4937	0.13%	0.015%
27	9.237	1084	1088	1091	rBV5	2932	4287	0.11%	0.013%
28	9.489	1124	1131	1143	rBV	212284	340863	8.86%	1.060%
29	10.031	1217	1223	1235	rVV	336245	552209	14.35%	1.717%
30	10.178	1243	1248	1258	rVB2	50090	80276	2.09%	0.250%
31	10.401	1278	1286	1301	rBV	1016445	1656890	43.07%	5.152%
32	10.536	1301	1309	1321	rBV	340514	564565	14.68%	1.756%
33	11.295	1433	1438	1442	rBV5	2923	5778	0.15%	0.018%
34	11.995	1551	1557	1561	rBV3	6930	11214	0.29%	0.035%
35	12.066	1565	1569	1574	rVB7	2428	4642	0.12%	0.014%
36	12.401	1624	1626	1631	rVB4	3813	4794	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032437.D
 Acq On : 12 Oct 2021 01:27
 Operator : CG/JU
 Sample : M4029-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	12.613	1658	1662	1667	rVB4	5213	7543	0.20%	0.023%
38	12.866	1701	1705	1707	rBV2	6255	7770	0.20%	0.024%
39	13.107	1740	1746	1751	rBV7	4368	9500	0.25%	0.030%
40	13.160	1751	1755	1762	rVV7	7305	13423	0.35%	0.042%
41	13.224	1762	1766	1771	rVV5	3462	6138	0.16%	0.019%
42	13.295	1774	1778	1786	rVB10	2868	6044	0.16%	0.019%
43	13.660	1834	1840	1855	rBV	771025	1049408	27.28%	3.263%
44	13.907	1874	1882	1883	rBV5	5515	6506	0.17%	0.020%
45	13.948	1883	1889	1899	rVV	810245	1143627	29.73%	3.556%
46	14.071	1903	1910	1921	rVV	29749	66585	1.73%	0.207%
47	14.260	1935	1942	1949	rBV	1743293	2459335	63.93%	7.648%
48	14.407	1964	1967	1970	rVB5	3131	4510	0.12%	0.014%
49	14.466	1971	1977	1988	rBV	255210	380599	9.89%	1.184%
50	14.595	1997	1999	2003	rVB5	3865	4308	0.11%	0.013%
51	14.671	2008	2012	2018	rVB5	17507	31608	0.82%	0.098%
52	15.001	2059	2068	2070	rBV9	2208	4329	0.11%	0.013%
53	15.066	2075	2079	2084	rBV2	9101	13374	0.35%	0.042%
54	15.248	2104	2110	2124	rBV	1139776	1574903	40.94%	4.897%
55	15.366	2124	2130	2137	rBV	245971	340831	8.86%	1.060%
56	15.489	2147	2151	2155	rVB2	12908	18382	0.48%	0.057%
57	15.607	2168	2171	2177	rVB7	3846	5252	0.14%	0.016%
58	15.683	2182	2184	2189	rVB4	4585	4645	0.12%	0.014%
59	15.748	2189	2195	2202	rBV8	3858	7093	0.18%	0.022%
60	16.142	2260	2262	2266	rVB5	3984	4362	0.11%	0.014%
61	16.242	2276	2279	2283	rBV6	3926	4800	0.12%	0.015%
62	16.348	2295	2297	2302	rBV6	2556	3973	0.10%	0.012%
63	16.777	2364	2370	2380	rVB2	9721	18622	0.48%	0.058%
64	16.989	2400	2406	2412	rVV	2226169	3041269	79.06%	9.457%
65	17.083	2416	2422	2434	rVV	1230865	1709330	44.43%	5.315%
66	17.177	2434	2438	2446	rVV2	25403	40132	1.04%	0.125%
67	17.271	2450	2454	2459	rBV6	3160	5499	0.14%	0.017%
68	17.365	2466	2470	2473	rBV5	2831	5044	0.13%	0.016%
69	17.477	2486	2489	2492	rBV5	3519	4966	0.13%	0.015%
70	17.654	2515	2519	2522	rBV5	13998	15848	0.41%	0.049%
71	17.877	2551	2557	2564	rBV2	72947	109728	2.85%	0.341%
72	17.942	2565	2568	2574	rVB	10945	17424	0.45%	0.054%
73	18.042	2582	2585	2589	rBV6	2734	4412	0.11%	0.014%
74	18.342	2632	2636	2637	rBV3	4365	4908	0.13%	0.015%
75	18.765	2706	2708	2712	rBV5	6214	8005	0.21%	0.025%
76	18.936	2734	2737	2742	rVB6	15212	22035	0.57%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032437.D
 Acq On : 12 Oct 2021 01:27
 Operator : CG/JU
 Sample : M4029-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	19.006	2745	2749	2751	rBV	16808	23110	0.60%	0.072%
78	19.036	2751	2754	2760	rVB	38710	48778	1.27%	0.152%
79	19.154	2771	2774	2777	rBV3	16095	17788	0.46%	0.055%
80	19.371	2805	2811	2822	rBV	1717498	2251278	58.52%	7.001%
81	19.601	2846	2850	2854	rVB	36194	41396	1.08%	0.129%
82	20.853	3060	3063	3071	rBV6	65341	104357	2.71%	0.325%
83	21.148	3108	3113	3119	rBV	2877134	3582945	93.14%	11.142%
84	22.606	3359	3361	3365	rVB	154390	179881	4.68%	0.559%
85	22.653	3366	3369	3376	rVB3	166736	228616	5.94%	0.711%
86	23.159	3448	3455	3467	rVB	1373652	2589500	67.31%	8.052%
87	23.294	3472	3478	3491	rVB2	2205483	3846982	100.00%	11.963%
88	23.724	3548	3551	3557	rVB	227310	354043	9.20%	1.101%




Sum of corrected areas: 32158422

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032437.D
Acq On : 12 Oct 2021 01:27
Operator : CG/JU
Sample : M4029-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

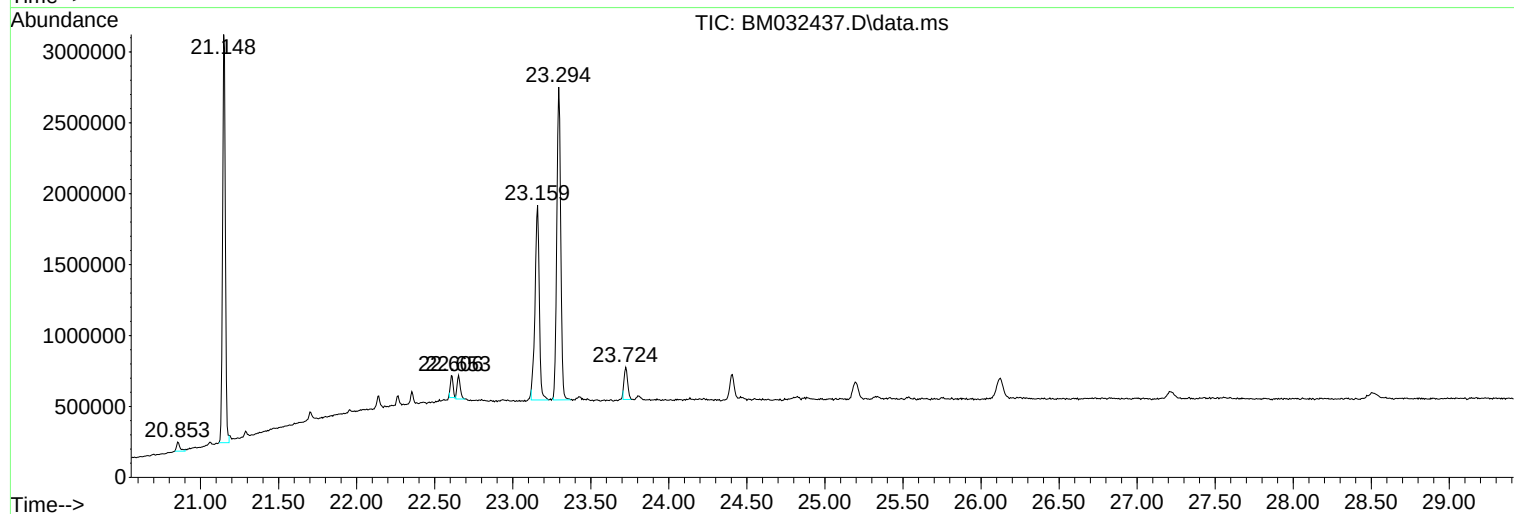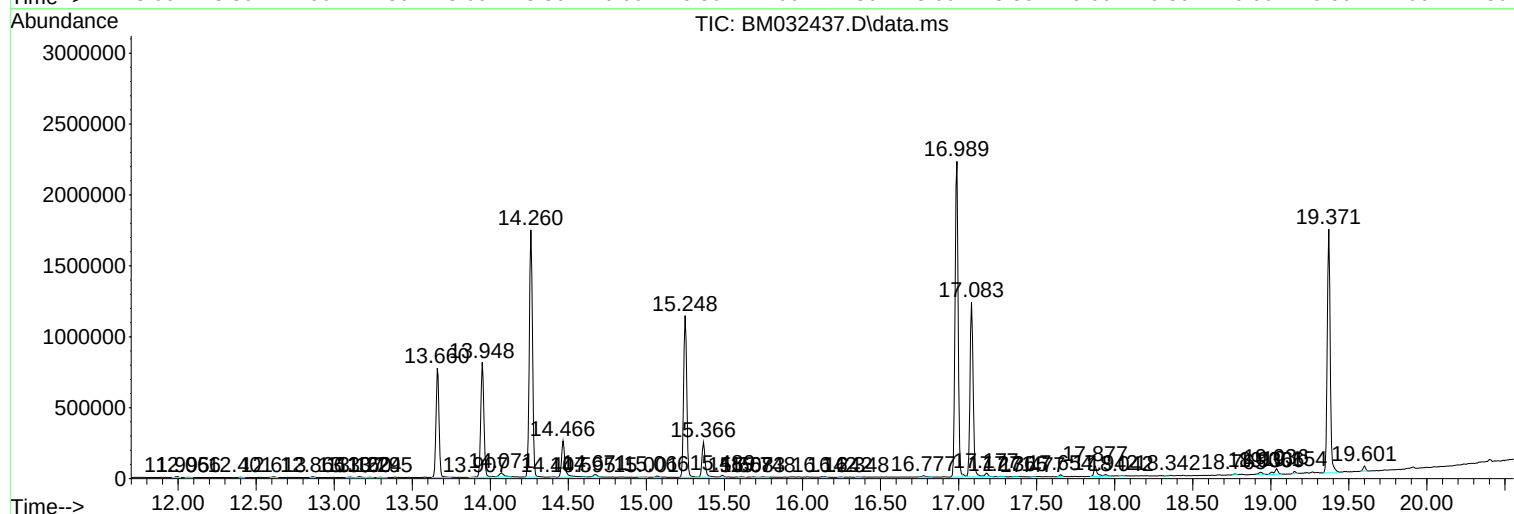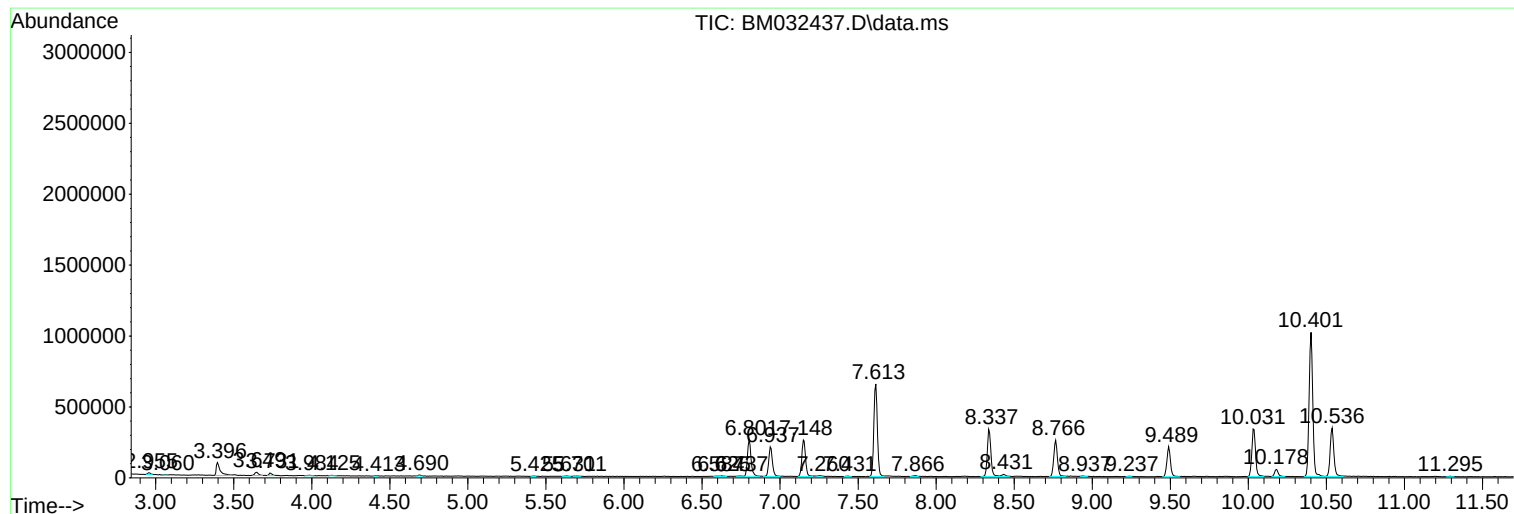

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032437.D
Acq On : 12 Oct 2021 01:27
Operator : CG/JU
Sample : M4029-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032437.D
Acq On : 12 Oct 2021 01:27
Operator : CG/JU
Sample : M4029-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------