

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032438.D
 Acq On : 12 Oct 2021 02:03
 Operator : CG/JU
 Sample : M4029-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	17	20	25	rVB	10450	13941	0.35%	0.051%
2	3.402	92	96	106	rBV	52466	86349	2.15%	0.315%
3	3.502	109	113	117	rBV2	24225	29805	0.74%	0.109%
4	3.649	132	138	143	rVB	24043	41240	1.03%	0.150%
5	3.737	149	153	164	rVB	11165	20710	0.52%	0.075%
6	3.984	192	195	200	rVB4	5230	7147	0.18%	0.026%
7	4.125	215	219	224	rBV7	3558	5710	0.14%	0.021%
8	4.413	263	268	271	rBV6	5882	8809	0.22%	0.032%
9	4.696	310	316	323	rBV3	11141	22337	0.56%	0.081%
10	4.796	328	333	338	rVB6	4774	7672	0.19%	0.028%
11	5.325	417	423	428	rBV8	3943	8555	0.21%	0.031%
12	5.590	464	468	472	rBV4	5554	7435	0.19%	0.027%
13	5.631	472	475	482	rVB9	3849	6480	0.16%	0.024%
14	6.743	658	664	669	rBV2	33663	53070	1.32%	0.193%
15	6.801	669	674	689	rVB2	171876	307152	7.66%	1.119%
16	6.937	689	697	707	rBV	138832	217014	5.41%	0.791%
17	7.149	727	733	742	rBV	165922	267560	6.67%	0.975%
18	7.254	748	751	757	rVB3	7075	12267	0.31%	0.045%
19	7.613	805	812	822	rBV	713672	1119237	27.91%	4.078%
20	7.860	848	854	859	rBV8	4370	7748	0.19%	0.028%
21	8.066	880	889	891	rBV7	3517	7150	0.18%	0.026%
22	8.178	904	908	912	rVB6	2523	4017	0.10%	0.015%
23	8.337	924	935	943	rBV	114956	194674	4.85%	0.709%
24	8.431	945	951	958	rBV	120538	186964	4.66%	0.681%
25	8.548	967	971	980	rVB	15294	28291	0.71%	0.103%
26	8.766	1000	1008	1019	rBV	162287	269066	6.71%	0.980%
27	8.872	1021	1026	1030	rVB4	5094	8605	0.21%	0.031%
28	9.490	1125	1131	1139	rBV	126949	200644	5.00%	0.731%
29	9.660	1155	1160	1170	rBV	31393	61545	1.53%	0.224%
30	9.842	1185	1191	1198	rBV	21445	37023	0.92%	0.135%
31	9.972	1207	1213	1214	rBV5	2978	4428	0.11%	0.016%
32	10.031	1217	1223	1235	rBV	200362	334943	8.35%	1.220%
33	10.178	1241	1248	1259	rBV	59380	90890	2.27%	0.331%
34	10.401	1278	1286	1300	rBV	1088128	1781855	44.43%	6.493%
35	10.537	1302	1309	1322	rVV	179642	308007	7.68%	1.122%
36	10.931	1371	1376	1385	rVB6	13575	22579	0.56%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032438.D
 Acq On : 12 Oct 2021 02:03
 Operator : CG/JU
 Sample : M4029-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	11.172	1413	1417	1423	rBV	18595	32384	0.81%	0.118%
38	11.436	1456	1462	1464	rBV6	3787	4872	0.12%	0.018%
39	11.748	1512	1515	1521	rVB	4963	7283	0.18%	0.027%
40	11.842	1526	1531	1536	rBV5	3336	7546	0.19%	0.027%
41	11.895	1536	1540	1543	rBV5	3149	6245	0.16%	0.023%
42	11.931	1543	1546	1551	rVV5	4964	9095	0.23%	0.033%
43	11.989	1551	1556	1564	rVB5	9461	17582	0.44%	0.064%
44	12.613	1658	1662	1668	rBV7	3275	5586	0.14%	0.020%
45	12.672	1668	1672	1676	rBV4	3396	5997	0.15%	0.022%
46	12.860	1699	1704	1708	rBV7	6312	10598	0.26%	0.039%
47	13.089	1740	1743	1751	rVB9	5390	7613	0.19%	0.028%
48	13.660	1833	1840	1849	rBV	485057	644695	16.08%	2.349%
49	13.948	1883	1889	1898	rBV	483279	680345	16.97%	2.479%
50	14.072	1903	1910	1919	rVV2	26264	53956	1.35%	0.197%
51	14.160	1921	1925	1932	rVB9	5771	11387	0.28%	0.041%
52	14.260	1935	1942	1956	rBV	1898243	2699501	67.32%	9.837%
53	14.466	1971	1977	1990	rBV	112533	186208	4.64%	0.679%
54	14.589	1995	1998	2004	rVV7	7595	13645	0.34%	0.050%
55	14.683	2004	2014	2027	rVB	48073	81821	2.04%	0.298%
56	15.060	2074	2078	2084	rBV7	4354	7684	0.19%	0.028%
57	15.119	2084	2088	2092	rVB5	4456	5587	0.14%	0.020%
58	15.248	2104	2110	2119	rBV	746566	983978	24.54%	3.585%
59	15.366	2124	2130	2143	rVV	95959	142202	3.55%	0.518%
60	15.489	2146	2151	2155	rVB4	8647	11712	0.29%	0.043%
61	15.830	2205	2209	2213	rVB7	5210	8089	0.20%	0.029%
62	15.930	2221	2226	2232	rBV	88857	124196	3.10%	0.453%
63	16.119	2254	2258	2260	rBV5	3711	4508	0.11%	0.016%
64	16.242	2274	2279	2284	rBV7	2565	5595	0.14%	0.020%
65	16.530	2325	2328	2333	rVB3	14151	17870	0.45%	0.065%
66	16.777	2364	2370	2373	rBV2	8955	12212	0.30%	0.044%
67	16.989	2399	2406	2416	rBV	2353474	3312399	82.60%	12.070%
68	17.083	2416	2422	2434	rVV	780227	1051231	26.21%	3.831%
69	17.177	2434	2438	2442	rVB3	25876	34554	0.86%	0.126%
70	17.360	2466	2469	2470	rBV3	4904	5190	0.13%	0.019%
71	17.389	2470	2474	2480	rVB2	16641	25581	0.64%	0.093%
72	17.483	2485	2490	2494	rVV7	5710	10117	0.25%	0.037%
73	17.654	2515	2519	2525	rVB5	15609	19671	0.49%	0.072%
74	17.742	2532	2534	2541	rVB	5906	7709	0.19%	0.028%
75	17.871	2551	2556	2560	rBV	36104	51283	1.28%	0.187%
76	17.936	2563	2567	2572	rVB	36011	50035	1.25%	0.182%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032438.D
 Acq On : 12 Oct 2021 02:03
 Operator : CG/JU
 Sample : M4029-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00S5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

77	17.989	2572	2576	2579	rBV5	3534	4701	0.12%	0.017%
78	18.442	2649	2653	2658	rVB2	27999	35221	0.88%	0.128%
79	18.665	2687	2691	2696	rBV	31852	40661	1.01%	0.148%
80	18.718	2698	2700	2704	rVB3	8549	9776	0.24%	0.036%
81	18.777	2706	2710	2712	rBV4	5834	8703	0.22%	0.032%
82	18.930	2722	2736	2744	rBV4	62557	229176	5.71%	0.835%
83	19.007	2746	2749	2751	rVV	9737	15031	0.37%	0.055%
84	19.036	2752	2754	2759	rVB	18399	18219	0.45%	0.066%
85	19.301	2797	2799	2802	rBV4	6046	5886	0.15%	0.021%
86	19.371	2805	2811	2821	rVV	1118346	1427254	35.59%	5.201%
87	21.148	3108	3113	3119	rBV	3072280	3826739	95.43%	13.944%
88	23.153	3448	3454	3465	rVB2	844435	1643396	40.98%	5.988%
89	23.295	3472	3478	3487	rVB2	2320801	4010081	100.00%	14.612%




Sum of corrected areas: 27443525

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032438.D
Acq On : 12 Oct 2021 02:03
Operator : CG/JU
Sample : M4029-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

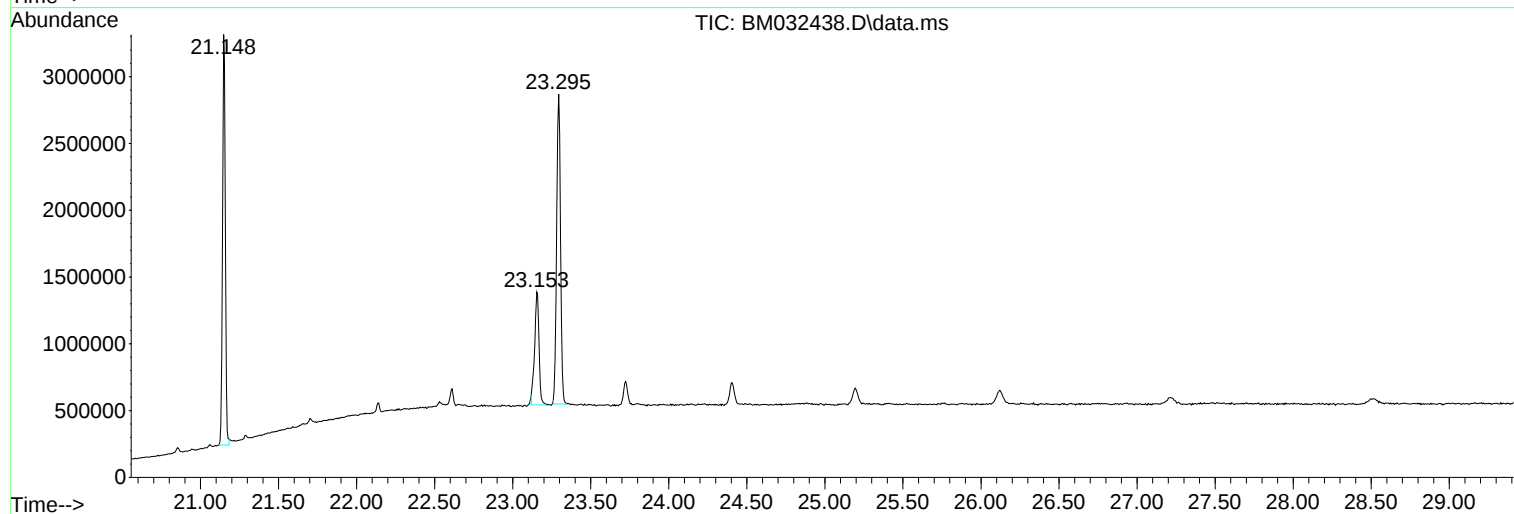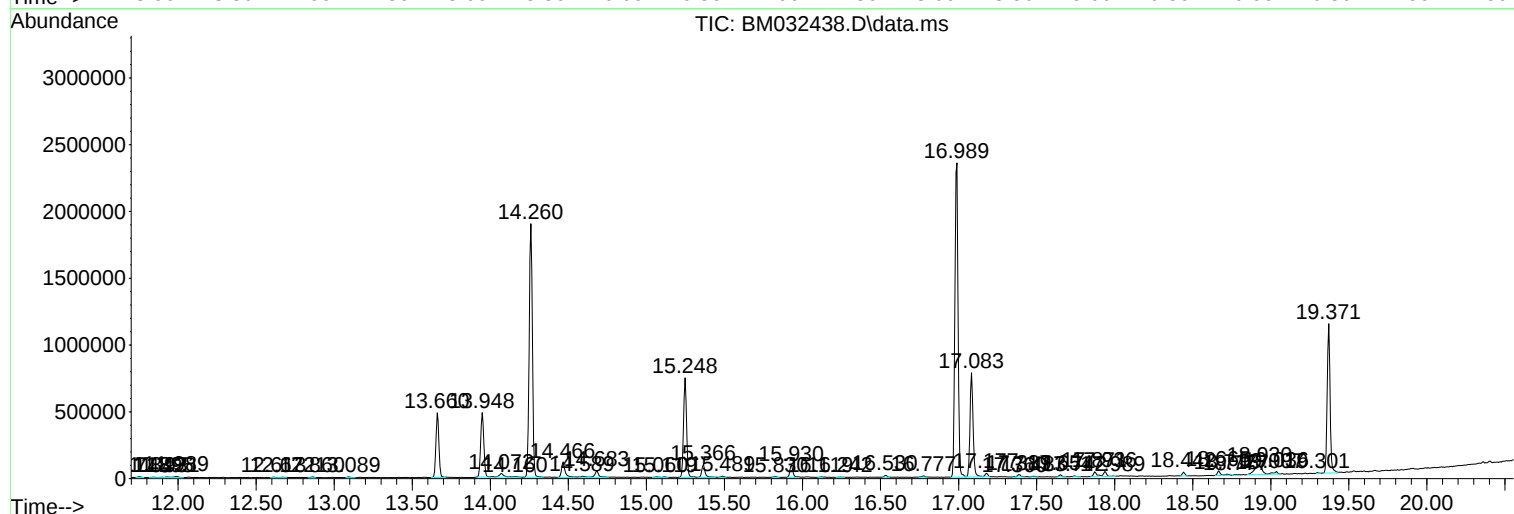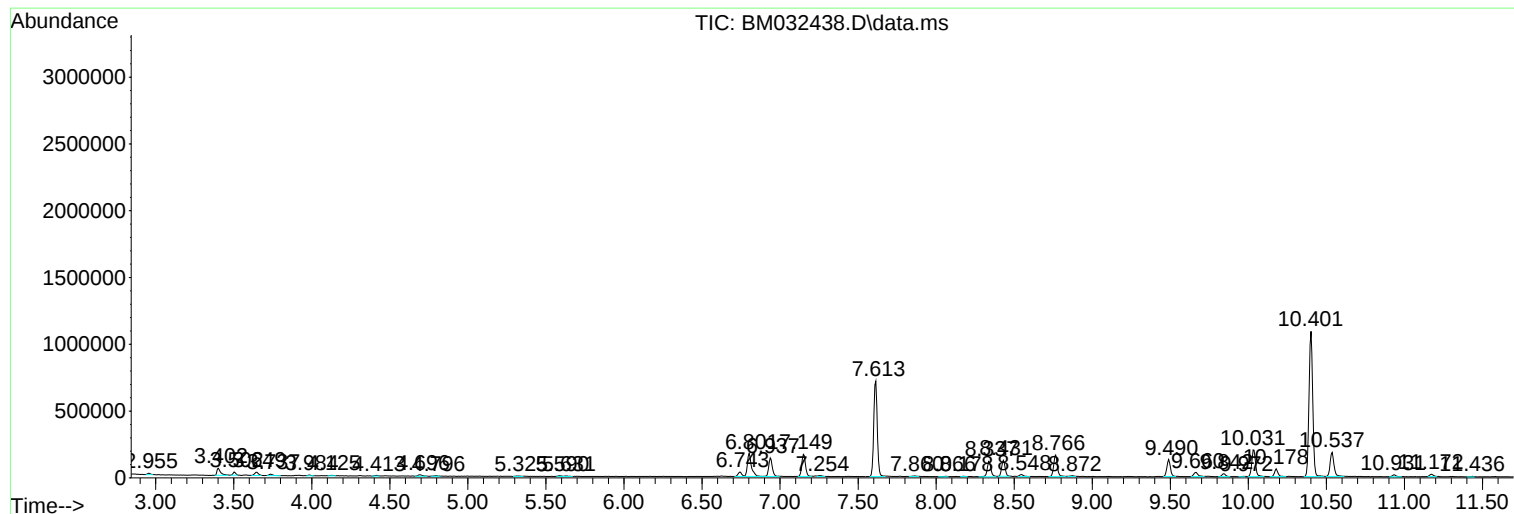

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032438.D
Acq On : 12 Oct 2021 02:03
Operator : CG/JU
Sample : M4029-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032438.D
Acq On : 12 Oct 2021 02:03
Operator : CG/JU
Sample : M4029-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
