

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032439.D
 Acq On : 12 Oct 2021 02:39
 Operator : CG/JU
 Sample : M4029-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.954	17	20	32	rVB	18009	27766	0.67%	0.082%
2	3.396	92	95	110	rBV	84576	145976	3.52%	0.432%
3	3.501	110	113	121	rVB3	14053	22335	0.54%	0.066%
4	3.648	132	138	145	rBV	26644	50229	1.21%	0.149%
5	3.731	148	152	161	rVB	13850	21522	0.52%	0.064%
6	3.984	192	195	200	rVB3	11473	15143	0.36%	0.045%
7	4.131	217	220	223	rVB4	3464	4327	0.10%	0.013%
8	4.413	265	268	274	rVB5	6319	9249	0.22%	0.027%
9	4.695	311	316	321	rVB2	6365	10285	0.25%	0.030%
10	6.595	635	639	642	rBV5	2903	4842	0.12%	0.014%
11	6.801	668	674	686	rVB	288904	440025	10.60%	1.304%
12	6.936	692	697	705	rBV	245009	376076	9.06%	1.114%
13	7.148	727	733	741	rBV	302607	469391	11.31%	1.391%
14	7.260	745	752	760	rVB9	7343	16676	0.40%	0.049%
15	7.436	778	782	784	rBV3	3539	4300	0.10%	0.013%
16	7.613	805	812	822	rBV	742028	1159784	27.95%	3.436%
17	7.860	852	854	860	rVB6	4201	6549	0.16%	0.019%
18	7.925	862	865	870	rVB7	2632	4543	0.11%	0.013%
19	8.178	904	908	911	rBV4	4004	6055	0.15%	0.018%
20	8.336	924	935	943	rBV	309647	485946	11.71%	1.440%
21	8.431	948	951	958	rVB	11892	20590	0.50%	0.061%
22	8.766	1001	1008	1020	rBV	284053	465165	11.21%	1.378%
23	8.942	1035	1038	1043	rVB7	3481	5166	0.12%	0.015%
24	9.489	1124	1131	1140	rVV	231109	370976	8.94%	1.099%
25	10.030	1217	1223	1237	rBV	382395	619564	14.93%	1.836%
26	10.177	1243	1248	1259	rVB	137954	207563	5.00%	0.615%
27	10.401	1277	1286	1294	rBV	1152054	1838342	44.30%	5.446%
28	10.536	1302	1309	1319	rBV	384718	634226	15.28%	1.879%
29	11.989	1550	1556	1562	rVB2	7572	14921	0.36%	0.044%
30	12.613	1656	1662	1666	rVB4	8196	11116	0.27%	0.033%
31	12.860	1698	1704	1710	rBV3	10280	15185	0.37%	0.045%
32	13.101	1740	1745	1746	rBV5	3377	4294	0.10%	0.013%
33	13.160	1750	1755	1761	rVV2	18169	29668	0.71%	0.088%
34	13.218	1761	1765	1769	rVB6	3216	5495	0.13%	0.016%
35	13.583	1823	1827	1831	rBV7	3283	4787	0.12%	0.014%
36	13.660	1834	1840	1849	rBV	822746	1136146	27.38%	3.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032439.D
 Acq On : 12 Oct 2021 02:39
 Operator : CG/JU
 Sample : M4029-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	13.907	1879	1882	1883	rBV3	4253	4297	0.10%	0.013%
38	13.948	1883	1889	1899	rVV	895270	1245421	30.01%	3.690%
39	14.071	1904	1910	1919	rVB	21812	49665	1.20%	0.147%
40	14.260	1935	1942	1951	rBV	1963230	2760949	66.54%	8.180%
41	14.407	1962	1967	1971	rBV7	4987	8188	0.20%	0.024%
42	14.465	1971	1977	1991	rBV	187309	309628	7.46%	0.917%
43	14.671	2006	2012	2019	rVB5	16339	30020	0.72%	0.089%
44	15.065	2075	2079	2085	rBV3	8708	15293	0.37%	0.045%
45	15.248	2104	2110	2124	rBV	1275610	1707712	41.16%	5.059%
46	15.365	2124	2130	2143	rVV	206066	291612	7.03%	0.864%
47	15.489	2147	2151	2157	rVB	15125	21906	0.53%	0.065%
48	15.607	2169	2171	2176	rVB5	3709	4896	0.12%	0.015%
49	15.683	2176	2184	2188	rBV7	7123	15106	0.36%	0.045%
50	15.924	2221	2225	2229	rBV5	4328	7717	0.19%	0.023%
51	16.036	2239	2244	2249	rVB7	4116	8661	0.21%	0.026%
52	16.136	2259	2261	2264	rVB3	3889	4349	0.10%	0.013%
53	16.248	2275	2280	2286	rBV9	2872	5944	0.14%	0.018%
54	16.530	2322	2328	2332	rBV3	13249	20336	0.49%	0.060%
55	16.777	2361	2370	2375	rBV	11264	21200	0.51%	0.063%
56	16.912	2389	2393	2396	rVB5	5399	7374	0.18%	0.022%
57	16.989	2399	2406	2412	rBV	2425341	3374118	81.32%	9.996%
58	17.083	2416	2422	2435	rVV2	1322007	1846807	44.51%	5.471%
59	17.177	2435	2438	2443	rVB3	28667	35949	0.87%	0.107%
60	17.265	2450	2453	2457	rBV	5380	7866	0.19%	0.023%
61	17.371	2466	2471	2477	rBV8	5449	9800	0.24%	0.029%
62	17.653	2512	2519	2523	rBV2	21698	27191	0.66%	0.081%
63	17.871	2552	2556	2564	rBV3	30182	46130	1.11%	0.137%
64	17.942	2564	2568	2573	rVB	11053	15842	0.38%	0.047%
65	18.665	2687	2691	2694	rBV6	4451	6847	0.17%	0.020%
66	18.771	2705	2709	2713	rBV6	7274	13983	0.34%	0.041%
67	18.824	2714	2718	2721	rVB6	16664	22597	0.54%	0.067%
68	18.936	2733	2737	2745	rVB9	16263	29343	0.71%	0.087%
69	19.006	2745	2749	2751	rBV	17791	22154	0.53%	0.066%
70	19.036	2751	2754	2762	rVB	48568	61305	1.48%	0.182%
71	19.371	2805	2811	2825	rBV	1836104	2408499	58.04%	7.135%
72	21.147	3108	3113	3118	rBV	3208957	3854499	92.89%	11.419%
73	23.159	3448	3455	3470	rVB	1353928	2617107	63.07%	7.753%
74	23.294	3472	3478	3492	rVB	2407868	4149407	100.00%	12.293%

Sum of corrected areas: 33753941

Instrument :

BNA_M

ClientSampleId :




C00Q9

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032439.D
Acq On : 12 Oct 2021 02:39
Operator : CG/JU
Sample : M4029-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00Q9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

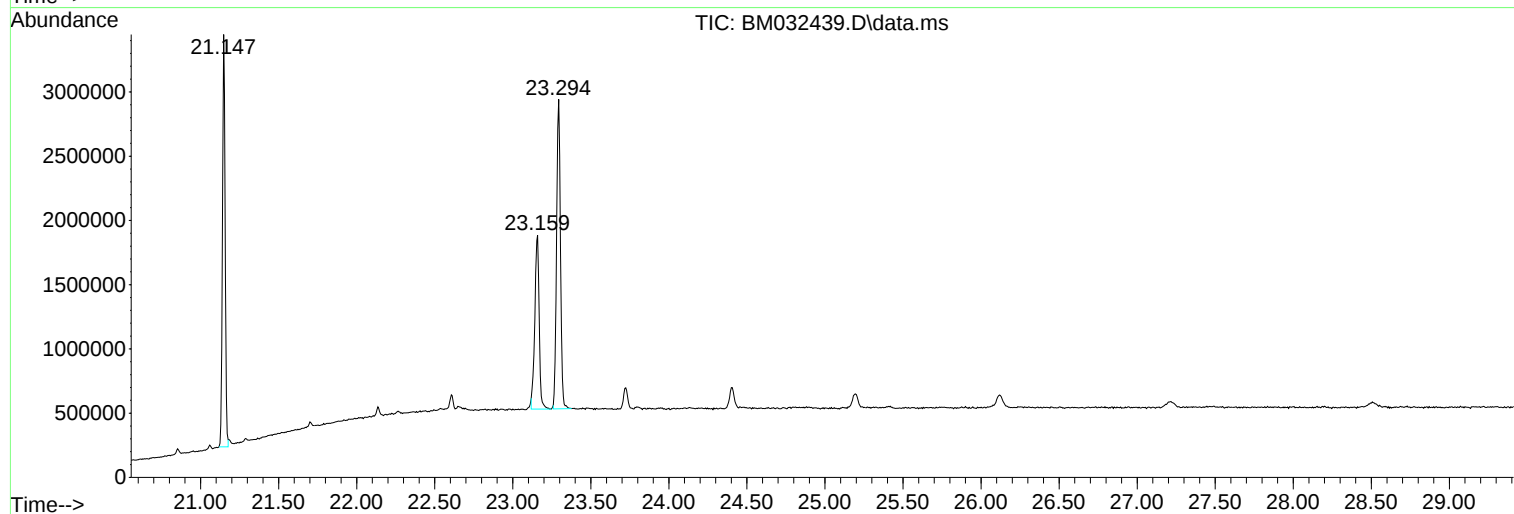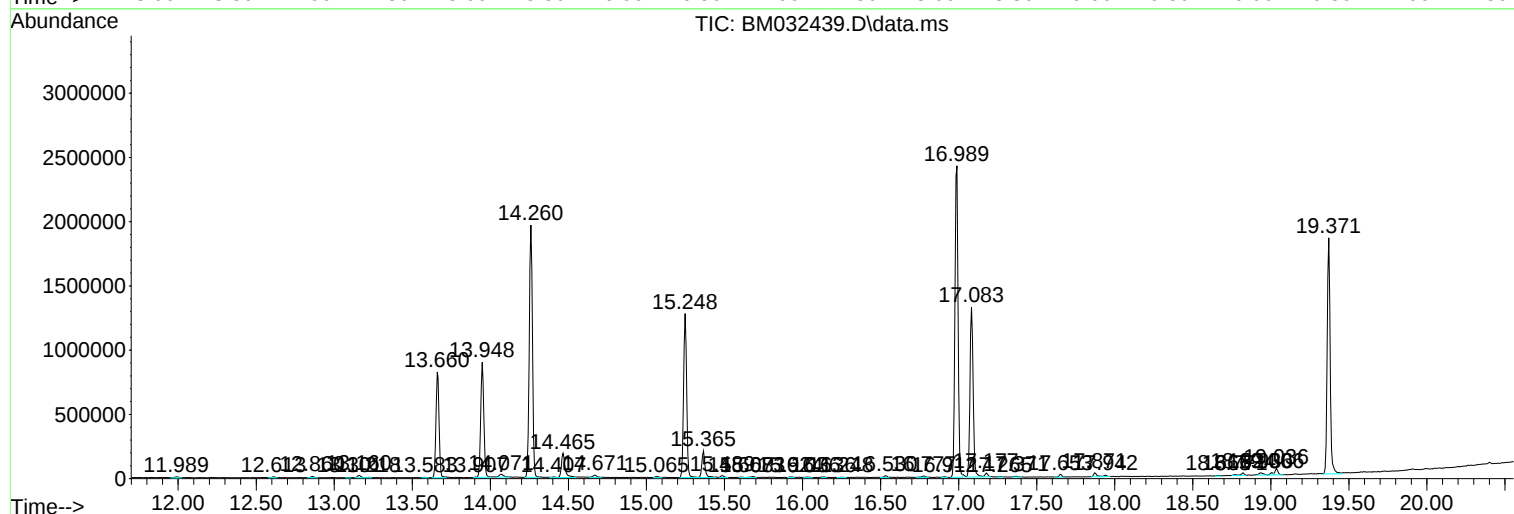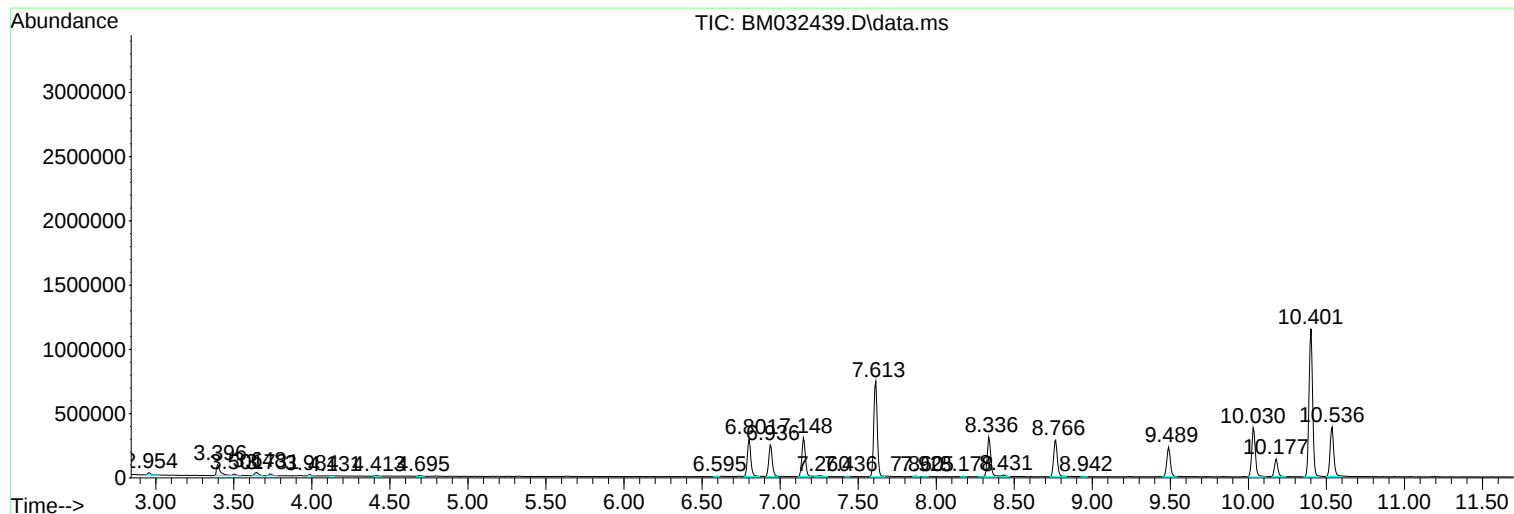

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032439.D
Acq On : 12 Oct 2021 02:39
Operator : CG/JU
Sample : M4029-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00Q9










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.177	2.26 ng/ul	207563	Naphthalene-d8	10.401

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

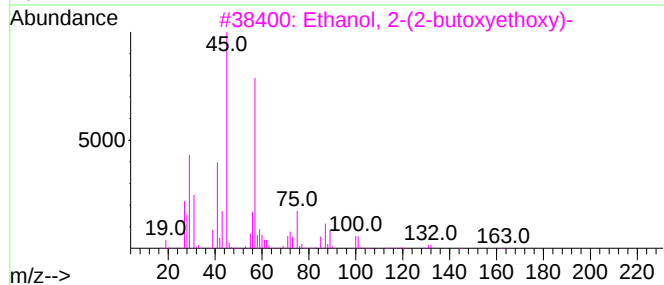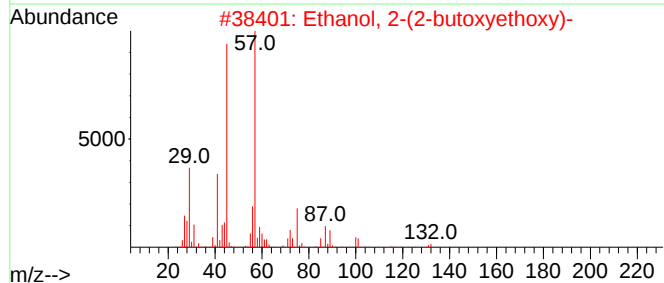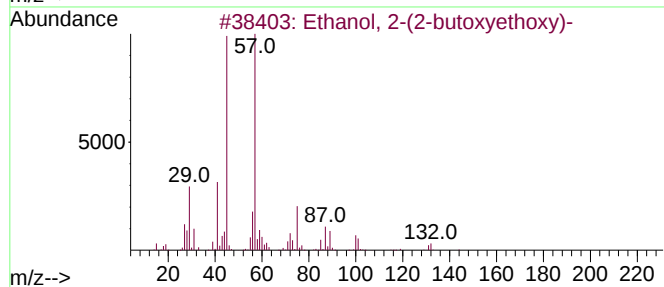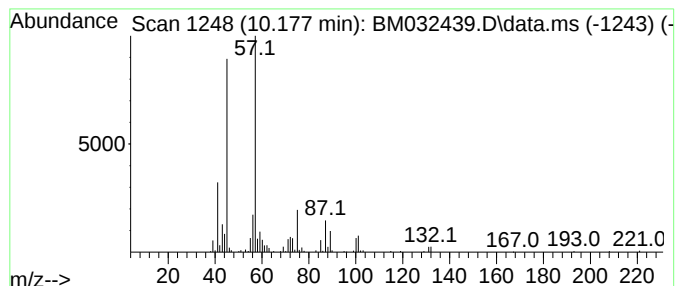

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032439.D
Acq On : 12 Oct 2021 02:39
Operator : CG/JU
Sample : M4029-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00Q9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.177	2.3	ng/u1	207563	2	10.401	1838340	20.0