

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032441.D
 Acq On : 12 Oct 2021 04:27
 Operator : CG/JU
 Sample : PB139668BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	30	rVB	58882	81495	1.37%	0.126%
2	3.384	89	93	112	rBV	740016	1126583	18.94%	1.746%
3	3.737	149	153	158	rVB	12799	16829	0.28%	0.026%
4	6.801	667	674	685	rBV	906412	1360141	22.87%	2.107%
5	6.937	691	697	708	rVB	740925	1107836	18.62%	1.717%
6	7.148	726	733	742	rBV	935309	1417248	23.83%	2.196%
7	7.607	805	811	823	rBV	844126	1336662	22.47%	2.071%
8	8.337	927	935	950	rBV	1189192	1833700	30.83%	2.841%
9	8.766	1000	1008	1018	rBV	864431	1411414	23.73%	2.187%
10	9.489	1122	1131	1146	rBV	753896	1208617	20.32%	1.873%
11	10.031	1216	1223	1237	rBV	1184542	1869196	31.42%	2.896%
12	10.401	1278	1286	1300	rBV	1335795	2178664	36.63%	3.376%
13	10.536	1301	1309	1321	rBV	1192925	1995029	33.54%	3.091%
14	11.989	1550	1556	1562	rBV	22120	35680	0.60%	0.055%
15	13.660	1834	1840	1855	rBV	2259768	3139436	52.78%	4.864%
16	13.948	1882	1889	1902	rBV	2682746	3710200	62.37%	5.749%
17	14.071	1905	1910	1918	rVB4	15592	35726	0.60%	0.055%
18	14.260	1935	1942	1957	rVB	2305227	3240069	54.47%	5.020%
19	14.466	1969	1977	1996	rBV	1098578	1564531	26.30%	2.424%
20	15.071	2072	2080	2084	rVB10	2457	6220	0.10%	0.010%
21	15.248	2103	2110	2124	rBV	3490165	4685008	78.76%	7.259%
22	15.365	2124	2130	2144	rVV	1093027	1422266	23.91%	2.204%
23	15.489	2146	2151	2156	rVB	41200	61976	1.04%	0.096%
24	15.913	2219	2223	2231	rVB9	5467	11610	0.20%	0.018%
25	16.030	2239	2243	2246	rVB4	5322	6721	0.11%	0.010%
26	16.665	2348	2351	2357	rBV7	5405	8050	0.14%	0.012%
27	16.777	2363	2370	2374	rBV2	11596	18237	0.31%	0.028%
28	16.989	2399	2406	2416	rBV	2816466	3885102	65.31%	6.020%
29	17.083	2416	2422	2443	rVB	3816618	5079242	85.39%	7.870%
30	17.359	2465	2469	2473	rVB3	5021	6230	0.10%	0.010%
31	17.654	2516	2519	2523	rBV4	8258	9183	0.15%	0.014%
32	17.871	2549	2556	2559	rBV7	9459	14189	0.24%	0.022%
33	18.936	2733	2737	2744	rBV	36569	48888	0.82%	0.076%
34	19.006	2744	2749	2754	rBV	48900	64952	1.09%	0.101%
35	19.259	2789	2792	2795	rBV2	6917	10065	0.17%	0.016%
36	19.371	2805	2811	2823	rBV	4495730	5896884	99.13%	9.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032441.D
Acq On : 12 Oct 2021 04:27
Operator : CG/JU
Sample : PB139668BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Title : SVOA CALIBRATION

37	21.147	3108	3113	3122	rBV	3494945	4282192	71.99%	6.635%
38	23.159	3448	3455	3465	rVB2	3430824	5948351	100.00%	9.217%
39	23.294	3472	3478	3492	rVB2	2530765	4405796	74.07%	6.826%




Sum of corrected areas: 64540218

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032441.D
Acq On : 12 Oct 2021 04:27
Operator : CG/JU
Sample : PB139668BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

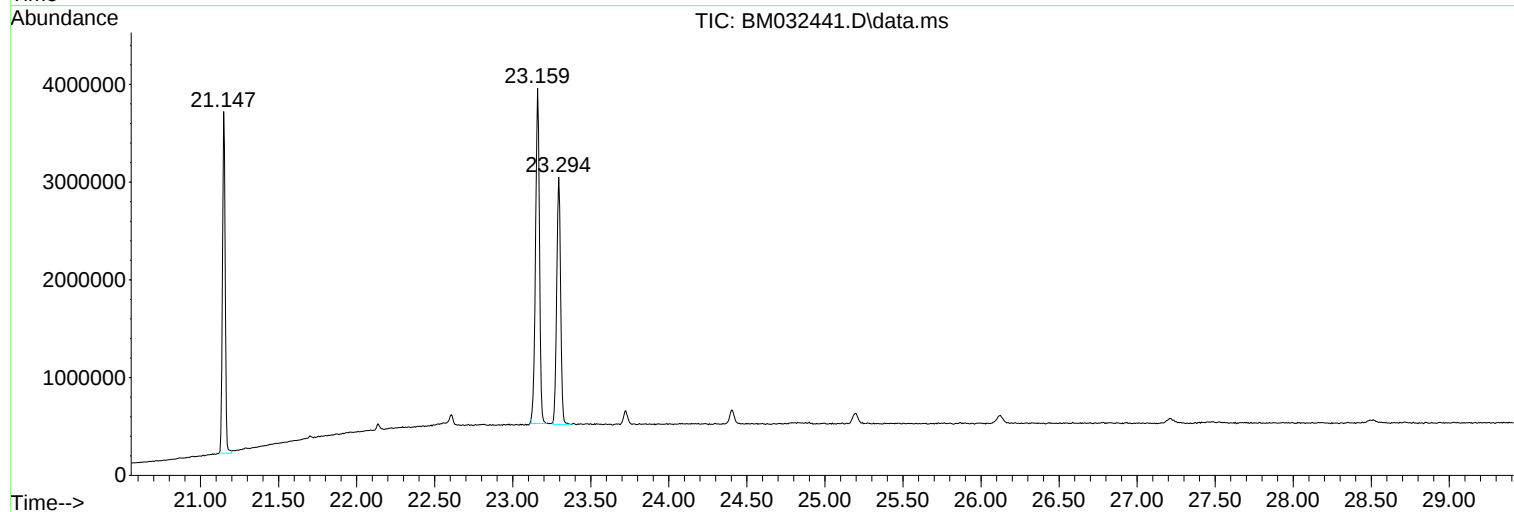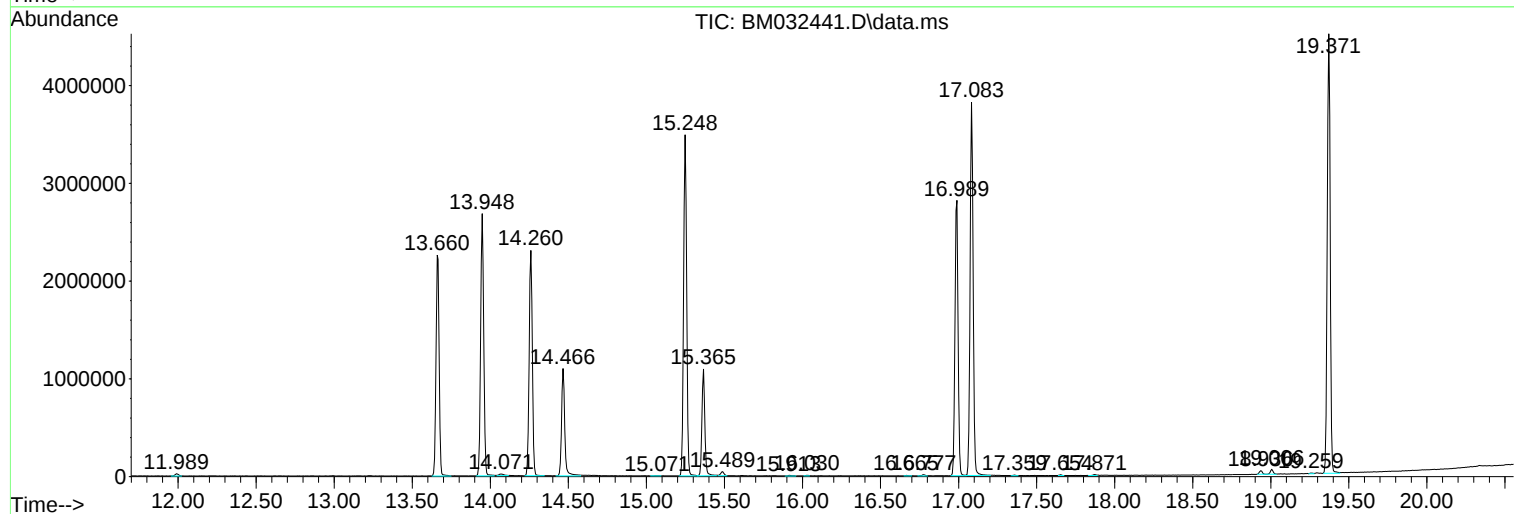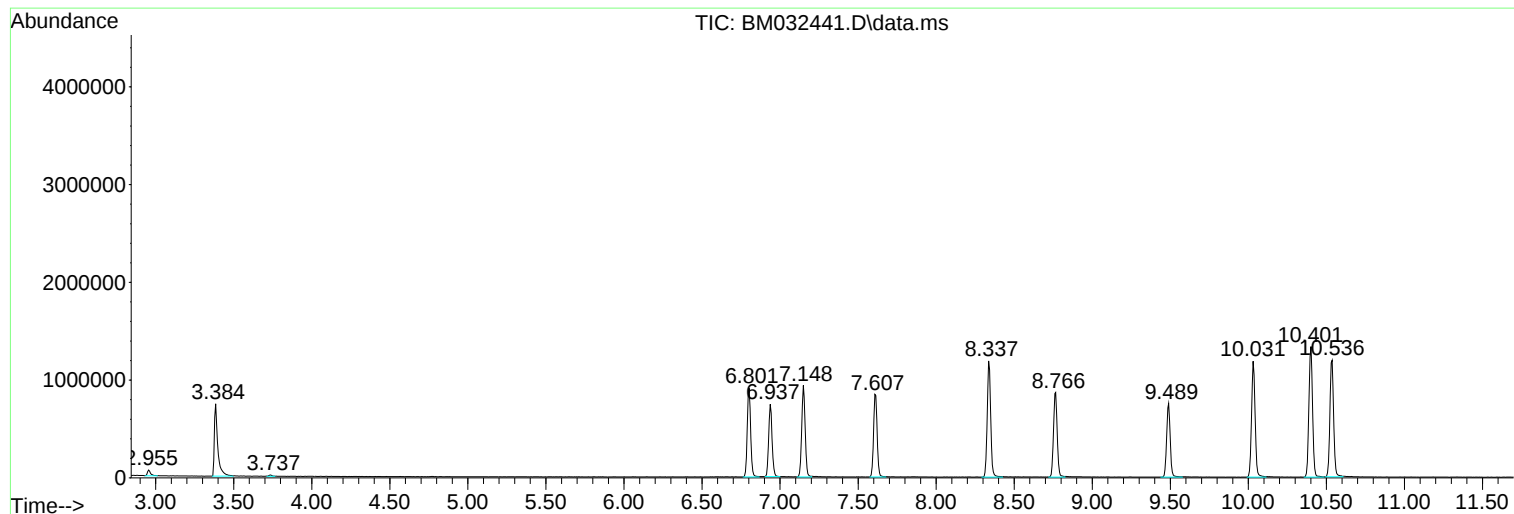

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032441.D
Acq On : 12 Oct 2021 04:27
Operator : CG/JU
Sample : PB139668BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032441.D
Acq On : 12 Oct 2021 04:27
Operator : CG/JU
Sample : PB139668BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
