

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032442.D
 Acq On : 12 Oct 2021 05:03
 Operator : CG/JU
 Sample : PB139788BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK788

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	27	rBV	70076	92334	1.28%	0.124%
2	3.384	89	93	114	rBV	911779	1413748	19.62%	1.901%
3	3.737	149	153	160	rVB	12546	17714	0.25%	0.024%
4	6.801	667	674	687	rBV	1161538	1713222	23.78%	2.304%
5	6.937	690	697	710	rVB	924957	1405824	19.51%	1.890%
6	7.148	726	733	746	rBV	1161328	1780517	24.71%	2.394%
7	7.613	804	812	825	rBV	815759	1299117	18.03%	1.747%
8	8.337	928	935	949	rBV	1477273	2287156	31.74%	3.075%
9	8.766	1001	1008	1024	rBV	1106567	1779305	24.69%	2.392%
10	9.489	1123	1131	1141	rBV	949351	1521870	21.12%	2.046%
11	10.031	1216	1223	1237	rBV	1492703	2359764	32.75%	3.173%
12	10.131	1239	1240	1246	rVB3	4804	7398	0.10%	0.010%
13	10.401	1278	1286	1301	rBV	1271573	2106598	29.24%	2.832%
14	10.536	1301	1309	1325	rBV	1532004	2523500	35.02%	3.393%
15	11.201	1417	1422	1428	rVB4	4725	8721	0.12%	0.012%
16	11.989	1549	1556	1562	rBV	27263	43337	0.60%	0.058%
17	13.225	1763	1766	1774	rVB4	5293	7511	0.10%	0.010%
18	13.666	1833	1841	1854	rBV	2797384	3887911	53.96%	5.228%
19	13.948	1882	1889	1898	rBV	3270879	4627027	64.21%	6.221%
20	14.072	1904	1910	1917	rVB3	14087	26669	0.37%	0.036%
21	14.260	1935	1942	1954	rBV	2187075	3100426	43.03%	4.169%
22	14.466	1970	1977	1995	rBV	1319276	1957235	27.16%	2.632%
23	15.248	2103	2110	2124	rBV	4324777	5791459	80.37%	7.787%
24	15.366	2124	2130	2142	rVV	1476617	1819745	25.25%	2.447%
25	15.483	2146	2150	2156	rVB	49931	73224	1.02%	0.098%
26	16.024	2239	2242	2249	rVB5	6933	9106	0.13%	0.012%
27	16.777	2364	2370	2374	rBV2	10784	18233	0.25%	0.025%
28	16.989	2399	2406	2415	rBV	2646043	3724052	51.68%	5.007%
29	17.083	2415	2422	2442	rVV	4507865	6266536	86.97%	8.426%
30	17.871	2553	2556	2560	rBV3	7971	10029	0.14%	0.013%
31	18.936	2733	2737	2742	rVB	49873	59274	0.82%	0.080%
32	19.006	2744	2749	2754	rBV	54436	73252	1.02%	0.098%
33	19.371	2805	2811	2822	rBV	5505090	7205583	100.00%	9.688%
34	21.148	3108	3113	3119	rBV	3379629	4061577	56.37%	5.461%
35	23.159	3448	3455	3464	rVB2	4104103	7195378	99.86%	9.675%
36	23.294	3472	3478	3486	rVB2	2376268	4099259	56.89%	5.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032442.D
Acq On : 12 Oct 2021 05:03
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Title : SVOA CALIBRATION




Sum of corrected areas: 74373611

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032442.D
Acq On : 12 Oct 2021 05:03
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

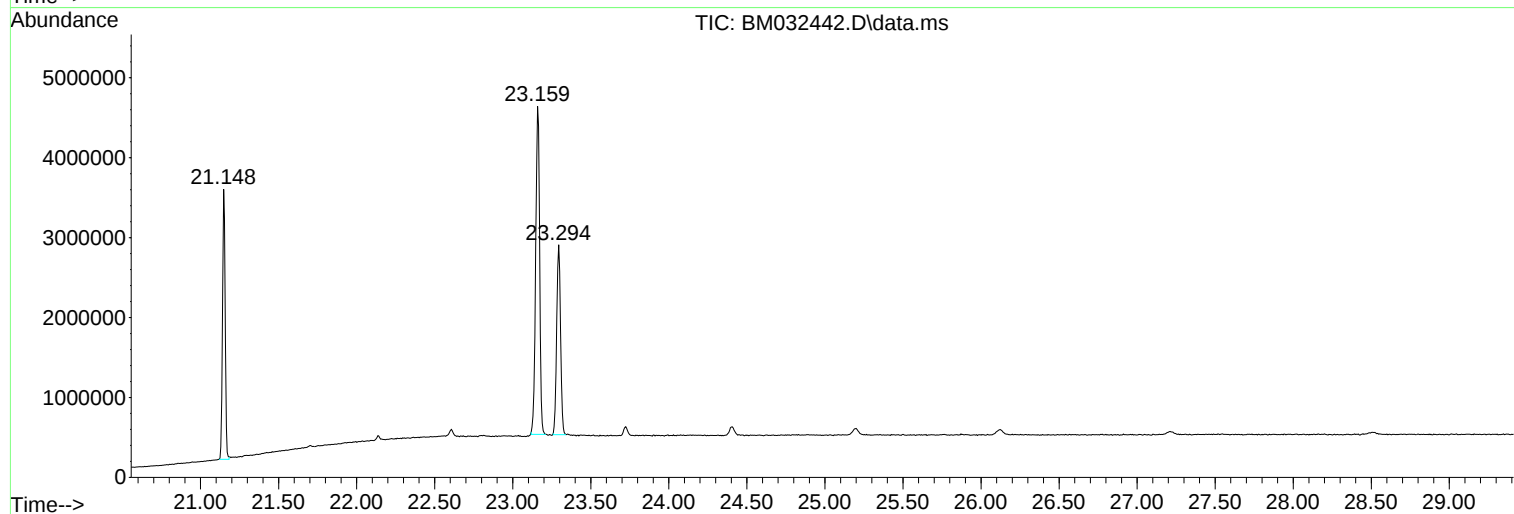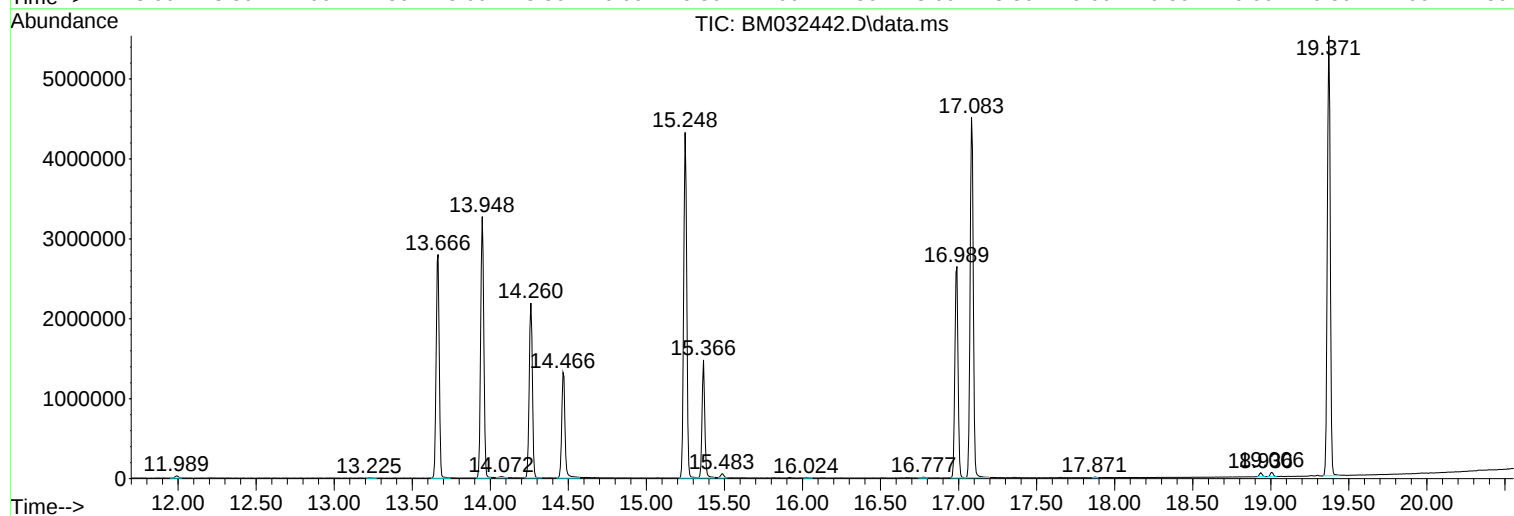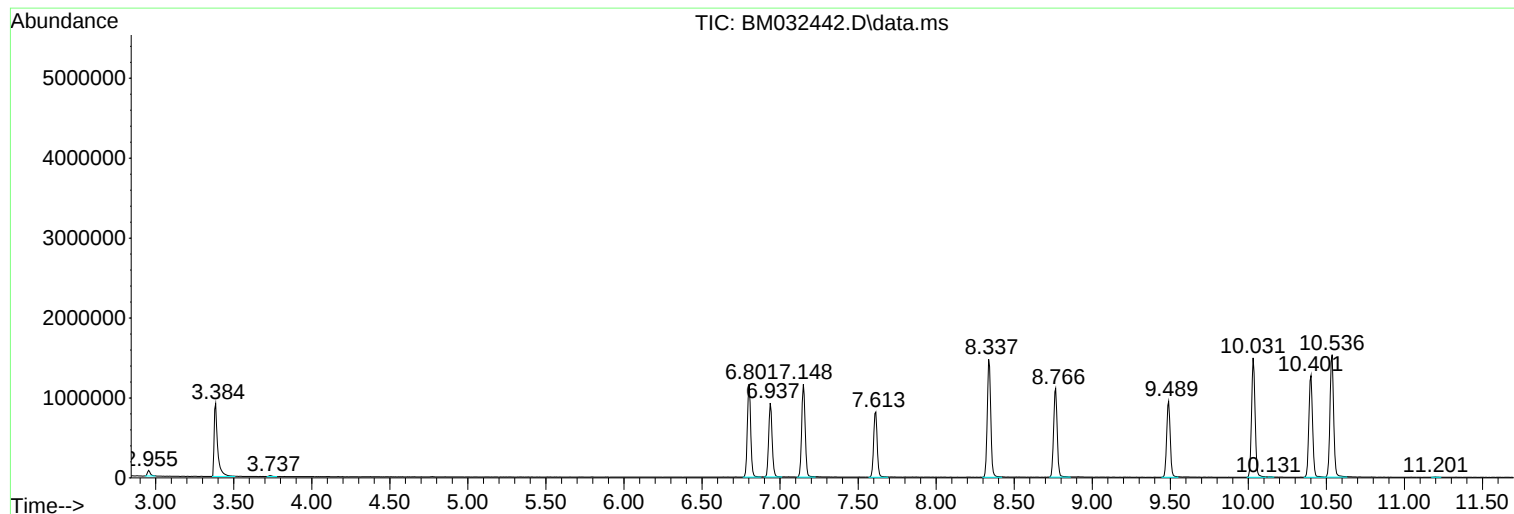

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032442.D
Acq On : 12 Oct 2021 05:03
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032442.D
Acq On : 12 Oct 2021 05:03
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
