

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032443.D
 Acq On : 12 Oct 2021 05:39
 Operator : CG/JU
 Sample : PB139789BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK789

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	29	rVB	65766	88806	1.37%	0.126%
2	3.384	89	93	114	rBV	840941	1278069	19.65%	1.815%
3	3.737	149	153	160	rVB2	15050	24194	0.37%	0.034%
4	6.802	667	674	687	rBV	1022346	1531890	23.55%	2.175%
5	6.937	690	697	707	rVV	833388	1254341	19.29%	1.781%
6	7.149	726	733	744	rBV	1050474	1587774	24.41%	2.254%
7	7.607	805	811	823	rBV	938651	1454905	22.37%	2.066%
8	8.337	927	935	950	rBV	1300803	2046113	31.46%	2.905%
9	8.766	999	1008	1025	rBV	994207	1581225	24.31%	2.245%
10	9.490	1122	1131	1143	rBV	839920	1343641	20.66%	1.908%
11	10.031	1216	1223	1238	rBV	1330586	2087845	32.10%	2.964%
12	10.401	1278	1286	1299	rBV	1452023	2355985	36.22%	3.345%
13	10.537	1301	1309	1322	rBV	1332093	2227198	34.24%	3.162%
14	11.201	1417	1422	1429	rBV9	4829	9287	0.14%	0.013%
15	11.990	1549	1556	1563	rBV	23856	39132	0.60%	0.056%
16	13.660	1834	1840	1856	rBV	2510992	3473357	53.40%	4.932%
17	13.948	1882	1889	1900	rBV	2964024	4092161	62.92%	5.810%
18	14.066	1905	1909	1917	rVB3	10965	25202	0.39%	0.036%
19	14.260	1934	1942	1954	rBV	2492158	3483852	53.56%	4.946%
20	14.466	1971	1977	1992	rBV	1237795	1705635	26.22%	2.422%
21	14.625	2000	2004	2009	rVB8	3392	6884	0.11%	0.010%
22	15.248	2103	2110	2124	rBV	3793534	5192679	79.84%	7.373%
23	15.366	2124	2130	2142	rVV	1217159	1575231	24.22%	2.237%
24	15.483	2146	2150	2157	rVB2	43363	66751	1.03%	0.095%
25	15.919	2219	2224	2230	rBV7	5329	9847	0.15%	0.014%
26	16.025	2239	2242	2247	rBV6	6202	8786	0.14%	0.012%
27	16.777	2363	2370	2375	rBV	11601	21142	0.33%	0.030%
28	16.983	2399	2405	2416	rBV	2924242	4148039	63.77%	5.889%
29	17.083	2416	2422	2432	rBV	4154249	5590714	85.96%	7.938%
30	17.354	2464	2468	2472	rVB4	4668	7148	0.11%	0.010%
31	17.871	2553	2556	2559	rBV4	10262	11749	0.18%	0.017%
32	18.936	2733	2737	2741	rBV2	42250	53746	0.83%	0.076%
33	19.007	2744	2749	2754	rBV	51220	66542	1.02%	0.094%
34	19.295	2795	2798	2802	rBV3	16630	19600	0.30%	0.028%
35	19.371	2805	2811	2817	rBV	4992984	6431036	98.87%	9.131%
36	21.148	3108	3113	3124	rBV	3640097	4521278	69.51%	6.419%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032443.D
Acq On : 12 Oct 2021 05:39
Operator : CG/JU
Sample : PB139789BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Title : SVOA CALIBRATION

37	23.159	3447	3455	3468	rVB2	3653433	6504231	100.00%	9.235%
38	23.295	3472	3478	3487	rVB2	2589551	4505596	69.27%	6.397%




Sum of corrected areas: 70431611

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032443.D
Acq On : 12 Oct 2021 05:39
Operator : CG/JU
Sample : PB139789BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

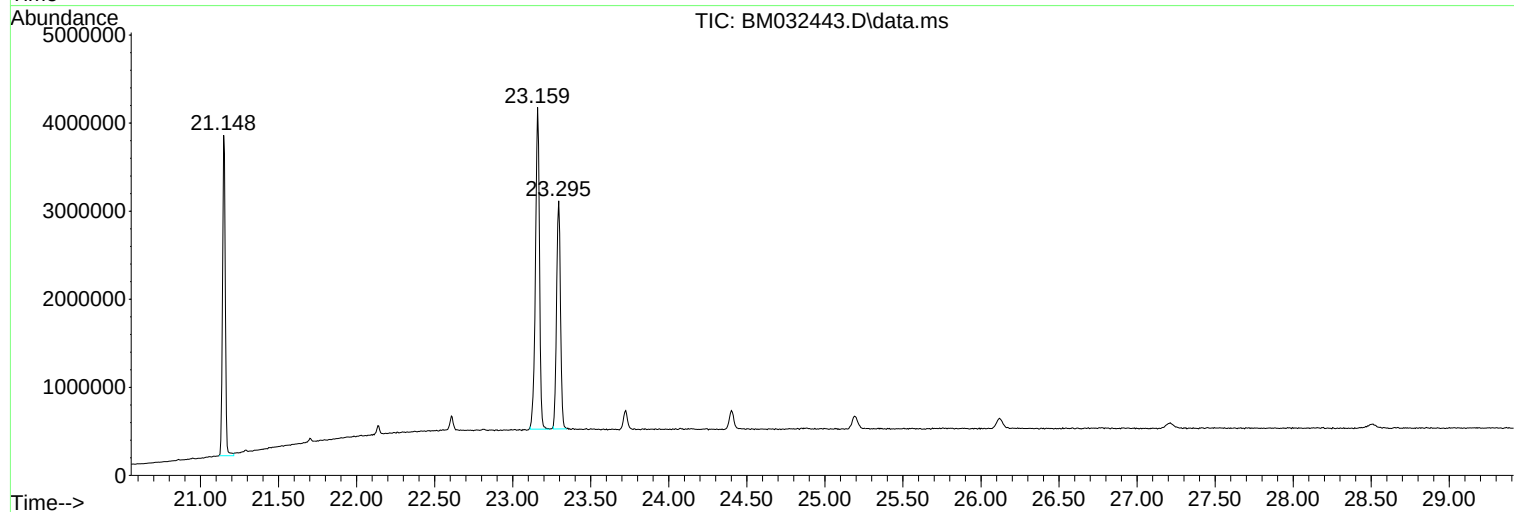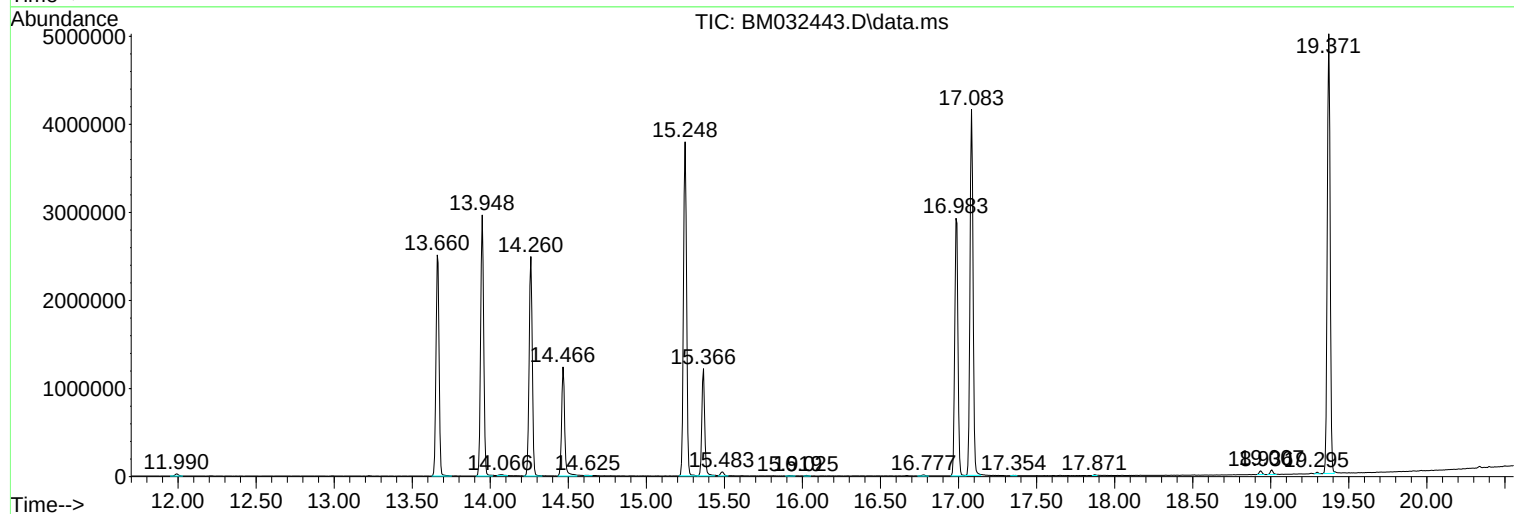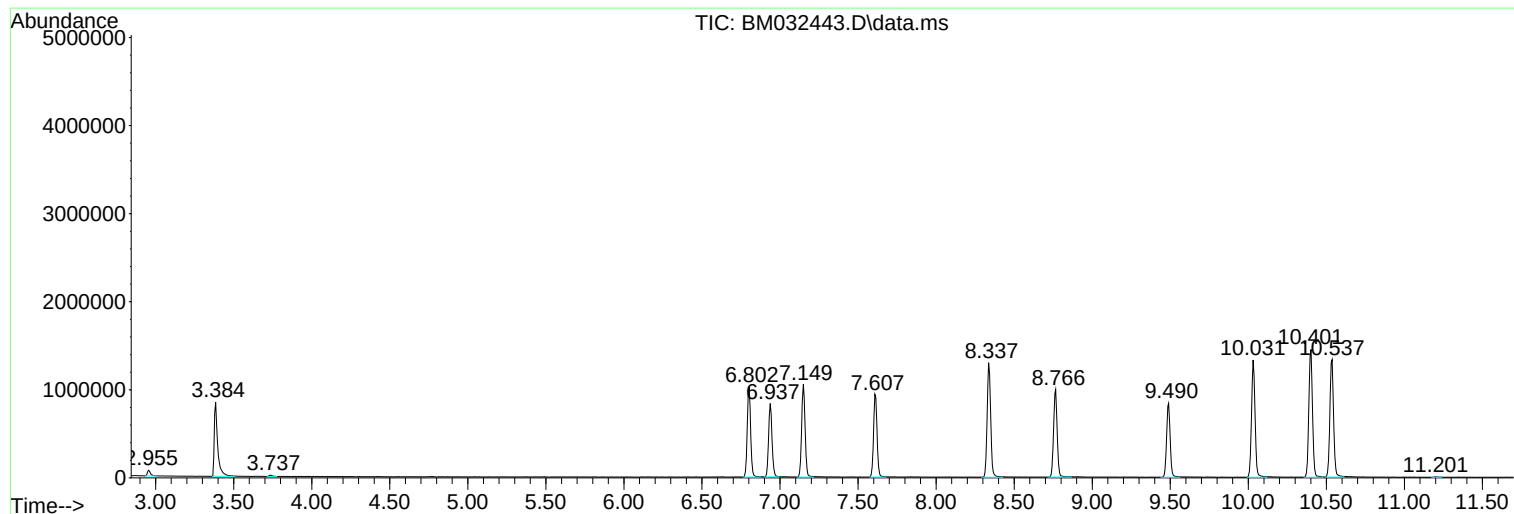

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032443.D
Acq On : 12 Oct 2021 05:39
Operator : CG/JU
Sample : PB139789BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032443.D
Acq On : 12 Oct 2021 05:39
Operator : CG/JU
Sample : PB139789BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc