

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032451.D
 Acq On : 12 Oct 2021 10:28
 Operator : CG/JU
 Sample : M4098-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAT57

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	29	rVB	68273	87264	0.98%	0.108%
2	3.390	90	94	107	rBV	257918	404656	4.56%	0.501%
3	3.649	132	138	146	rVB	24192	44047	0.50%	0.054%
4	3.731	149	152	161	rVB	13777	22485	0.25%	0.028%
5	4.701	312	317	323	rVB4	6061	10193	0.11%	0.013%
6	6.801	667	674	689	rBV	332569	516182	5.82%	0.639%
7	6.937	689	697	709	rBV	947781	1449911	16.35%	1.794%
8	7.148	726	733	743	rBV	1025541	1539745	17.36%	1.905%
9	7.254	749	751	756	rVB6	8212	9174	0.10%	0.011%
10	7.607	805	811	822	rBV	986801	1544349	17.41%	1.911%
11	7.690	822	825	829	rVB2	10822	16252	0.18%	0.020%
12	8.337	928	935	946	rBV	935041	1415467	15.96%	1.751%
13	8.760	998	1007	1018	rBV	1153226	1861511	20.99%	2.303%
14	8.919	1029	1034	1041	rBV7	6535	16134	0.18%	0.020%
15	9.242	1080	1089	1093	rVB2	11950	20232	0.23%	0.025%
16	9.489	1123	1131	1145	rBV	944812	1536895	17.33%	1.901%
17	10.031	1216	1223	1238	rBV	1436581	2291279	25.83%	2.835%
18	10.178	1242	1248	1261	rVB	463518	677070	7.63%	0.838%
19	10.401	1277	1286	1293	rBV	1475508	2454887	27.68%	3.037%
20	10.536	1301	1309	1325	rBV	1318986	2196936	24.77%	2.718%
21	11.719	1503	1510	1516	rBV2	13234	24254	0.27%	0.030%
22	11.989	1550	1556	1565	rBV2	28427	44015	0.50%	0.054%
23	12.613	1657	1662	1668	rBV5	5673	10461	0.12%	0.013%
24	12.860	1699	1704	1710	rVB2	9964	15255	0.17%	0.019%
25	13.095	1739	1744	1750	rVB4	5940	10931	0.12%	0.014%
26	13.160	1750	1755	1760	rVV2	66348	101470	1.14%	0.126%
27	13.224	1763	1766	1771	rVB3	7435	10733	0.12%	0.013%
28	13.660	1834	1840	1848	rBV	2896359	4044669	45.60%	5.004%
29	13.724	1848	1851	1858	rVB2	15579	23956	0.27%	0.030%
30	13.948	1878	1889	1902	rBV	3472261	4860408	54.80%	6.013%
31	14.260	1935	1942	1950	rVV	2501500	3562328	40.16%	4.407%
32	14.318	1950	1952	1964	rVB5	9911	15802	0.18%	0.020%
33	14.466	1970	1977	1991	rBV	364505	576924	6.50%	0.714%
34	14.666	2006	2011	2018	rVB5	12287	26443	0.30%	0.033%
35	15.066	2074	2079	2082	rBV3	7065	11722	0.13%	0.015%
36	15.118	2084	2088	2091	rVB3	8605	9698	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032451.D
 Acq On : 12 Oct 2021 10:28
 Operator : CG/JU
 Sample : M4098-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAT57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	15.248	2103	2110	2117	rBV	4546804	6321200	71.27%	7.820%
38	15.365	2124	2130	2145	rBV	1710502	2173233	24.50%	2.688%
39	15.483	2145	2150	2155	rVV	54220	77546	0.87%	0.096%
40	15.607	2166	2171	2176	rBV7	7855	12485	0.14%	0.015%
41	15.683	2176	2184	2189	rBV5	12529	22672	0.26%	0.028%
42	15.795	2199	2203	2212	rVB9	7481	15375	0.17%	0.019%
43	15.918	2220	2224	2230	rBV8	9706	19761	0.22%	0.024%
44	16.030	2239	2243	2249	rVB4	13072	19542	0.22%	0.024%
45	16.136	2255	2261	2267	rBV5	11171	20909	0.24%	0.026%
46	16.242	2275	2279	2284	rVB2	8923	11591	0.13%	0.014%
47	16.395	2302	2305	2311	rVB3	13027	17285	0.19%	0.021%
48	16.601	2334	2340	2346	rBV6	5483	11560	0.13%	0.014%
49	16.671	2346	2352	2354	rBV5	5915	8916	0.10%	0.011%
50	16.771	2364	2369	2372	rBV2	11891	20373	0.23%	0.025%
51	16.801	2372	2374	2380	rVB5	9282	12093	0.14%	0.015%
52	16.983	2399	2405	2411	rBV	3046353	4324210	48.75%	5.349%
53	17.083	2416	2422	2434	rVV2	5501334	7531945	84.92%	9.318%
54	17.177	2434	2438	2444	rVB6	16882	30817	0.35%	0.038%
55	17.289	2455	2457	2463	rVB6	7173	9219	0.10%	0.011%
56	17.365	2463	2470	2477	rBV4	12640	34890	0.39%	0.043%
57	17.518	2493	2496	2501	rVB3	7713	10188	0.11%	0.013%
58	17.654	2515	2519	2525	rBV	163836	190827	2.15%	0.236%
59	17.877	2552	2557	2564	rBV	148024	223525	2.52%	0.277%
60	18.789	2708	2712	2714	rBV3	32481	37840	0.43%	0.047%
61	18.824	2714	2718	2722	rVB	280353	317809	3.58%	0.393%
62	18.936	2732	2737	2744	rBV2	64242	136409	1.54%	0.169%
63	19.006	2744	2749	2753	rBV	77198	110273	1.24%	0.136%
64	19.153	2770	2774	2782	rBV	65395	90660	1.02%	0.112%
65	19.259	2789	2792	2795	rBV	13866	16096	0.18%	0.020%
66	19.301	2796	2799	2804	rVB4	15704	18820	0.21%	0.023%
67	19.371	2805	2811	2825	rBV	6630324	8780398	98.99%	10.862%
68	20.359	2977	2979	2982	rVB2	39567	36623	0.41%	0.045%
69	20.853	3059	3063	3068	rBV	205175	254847	2.87%	0.315%
70	21.147	3108	3113	3122	rBV	3773418	4784241	53.94%	5.919%
71	23.165	3447	3456	3467	rVB2	4784418	8869830	100.00%	10.973%
72	23.294	3472	3478	3489	rVB2	2693789	4796829	54.08%	5.934%




Sum of corrected areas: 80834575

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032451.D
Acq On : 12 Oct 2021 10:28
Operator : CG/JU
Sample : M4098-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAT57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

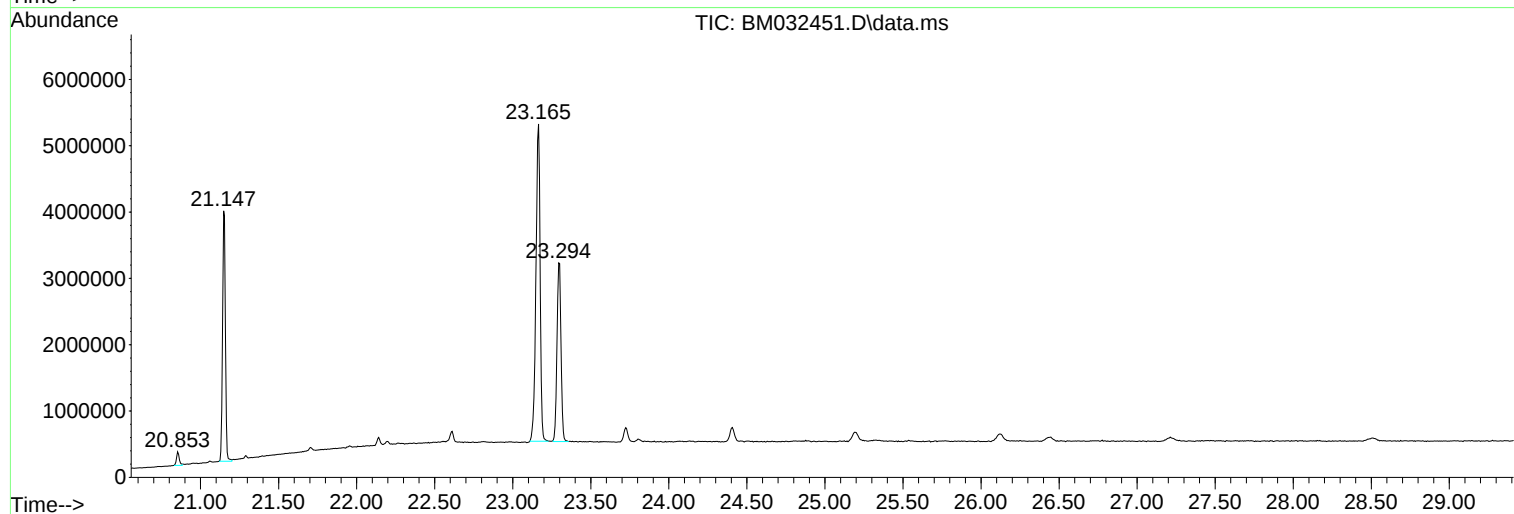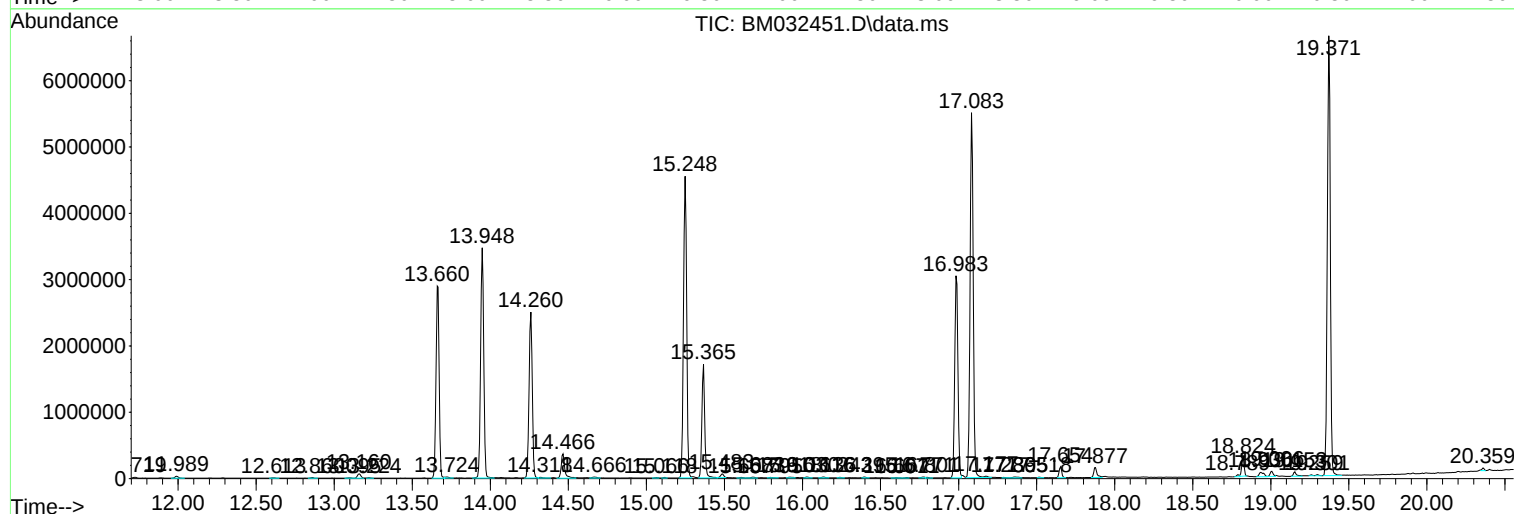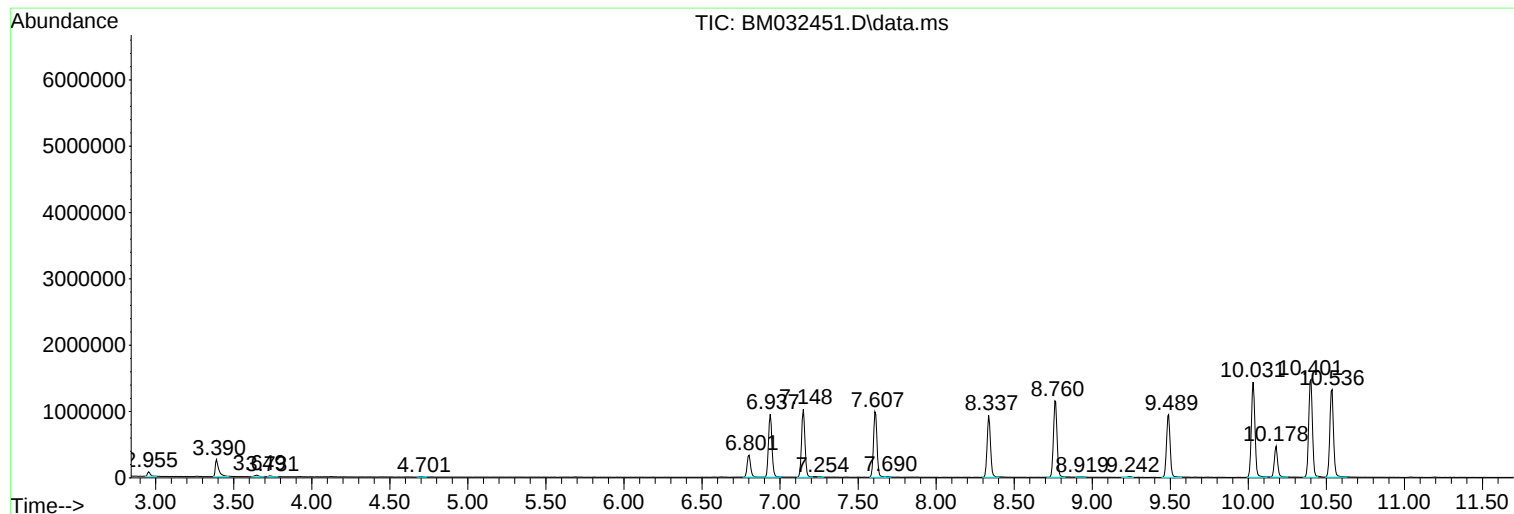

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032451.D
Acq On : 12 Oct 2021 10:28
Operator : CG/JU
Sample : M4098-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAT57










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.178	5.52 ng/ul	677070	Naphthalene-d8	10.401

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

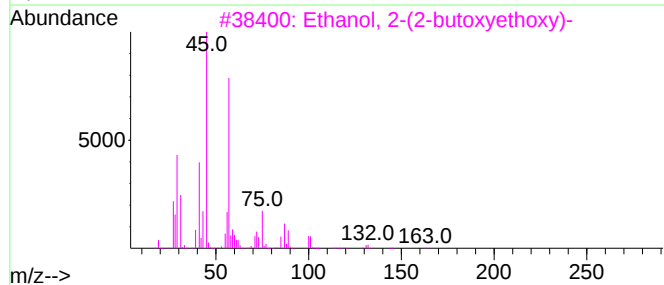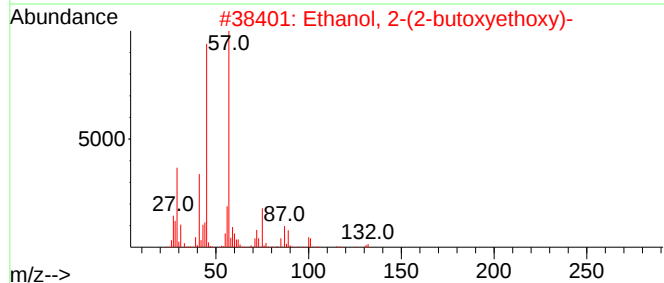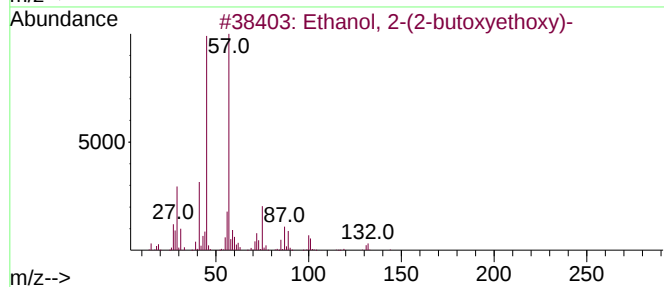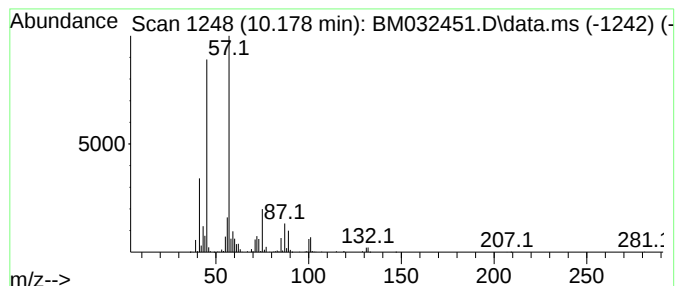

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032451.D
Acq On : 12 Oct 2021 10:28
Operator : CG/JU
Sample : M4098-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAT57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.178	5.5	ng/u1	677070	2	10.401	2454890	20.0