

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032459.D
 Acq On : 12 Oct 2021 15:55
 Operator : CG/JU
 Sample : PB139788BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK788

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	30	rVB	71789	96782	1.36%	0.133%
2	3.384	89	93	113	rBV	919995	1393491	19.65%	1.917%
3	3.737	147	153	160	rBV	13188	22089	0.31%	0.030%
4	6.801	667	674	685	rBV	1130317	1711801	24.13%	2.355%
5	6.937	691	697	710	rVB	919284	1401764	19.76%	1.929%
6	7.148	726	733	746	rBV	1169618	1760733	24.82%	2.423%
7	7.607	804	811	825	rBV	831374	1291016	18.20%	1.776%
8	8.337	928	935	946	rBV	1484612	2278793	32.13%	3.135%
9	8.760	1000	1007	1017	rBV	1101588	1768380	24.93%	2.433%
10	9.484	1124	1130	1145	rBV	906554	1502247	21.18%	2.067%
11	10.031	1212	1223	1236	rBV	1456564	2332419	32.88%	3.209%
12	10.125	1237	1239	1245	rVB6	5382	10263	0.14%	0.014%
13	10.395	1278	1285	1300	rBV	1222368	2008330	28.31%	2.763%
14	10.531	1301	1308	1322	rBV	1510058	2502366	35.28%	3.443%
15	11.989	1550	1556	1562	rBV	26516	42334	0.60%	0.058%
16	13.660	1833	1840	1856	rBV	2833420	3887818	54.81%	5.349%
17	13.948	1882	1889	1906	rBV	3339651	4593524	64.76%	6.320%
18	14.260	1935	1942	1954	rBV	2029175	2989737	42.15%	4.114%
19	14.466	1970	1977	1996	rBV	1346882	1878948	26.49%	2.585%
20	14.666	2008	2011	2018	rVB5	5604	10227	0.14%	0.014%
21	15.248	2103	2110	2124	rBV	4163185	5799102	81.76%	7.979%
22	15.366	2124	2130	2143	rVV	1275857	1705101	24.04%	2.346%
23	15.483	2145	2150	2155	rVB	52991	76251	1.08%	0.105%
24	15.913	2218	2223	2228	rBV7	5846	8739	0.12%	0.012%
25	16.030	2238	2243	2247	rVB5	5458	8198	0.12%	0.011%
26	16.771	2364	2369	2374	rBV	9904	13773	0.19%	0.019%
27	16.983	2399	2405	2415	rBV	2707848	3617244	51.00%	4.977%
28	17.083	2415	2422	2437	rVV2	4499495	6225566	87.77%	8.566%
29	17.871	2551	2556	2560	rBV8	7532	11805	0.17%	0.016%
30	18.936	2732	2737	2742	rBV	45270	64132	0.90%	0.088%
31	19.007	2744	2749	2755	rVV	53526	74750	1.05%	0.103%
32	19.371	2805	2811	2825	rBV	5543691	7092831	100.00%	9.759%
33	21.148	3108	3113	3122	rBV	3046996	3954956	55.76%	5.442%
34	23.165	3449	3456	3468	rVB2	3833610	6692536	94.36%	9.209%
35	23.294	3472	3478	3488	rVB2	2214867	3849654	54.28%	5.297%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032459.D
Acq On : 12 Oct 2021 15:55
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Title : SVOA CALIBRATION




Sum of corrected areas: 72677700

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032459.D
Acq On : 12 Oct 2021 15:55
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

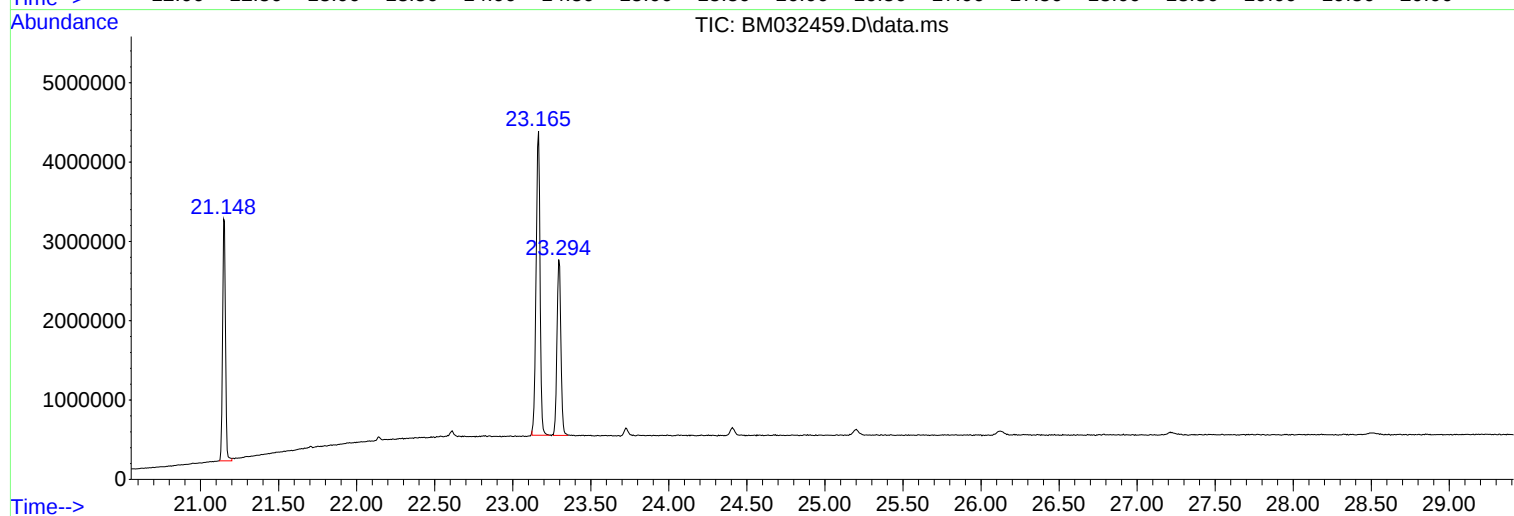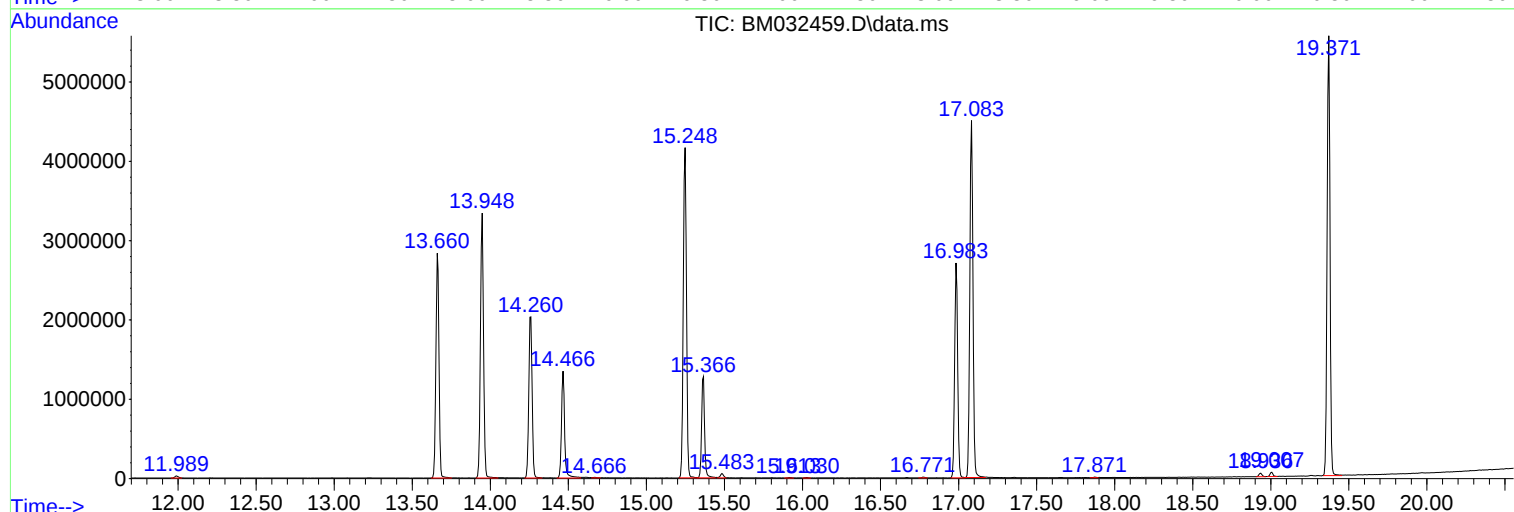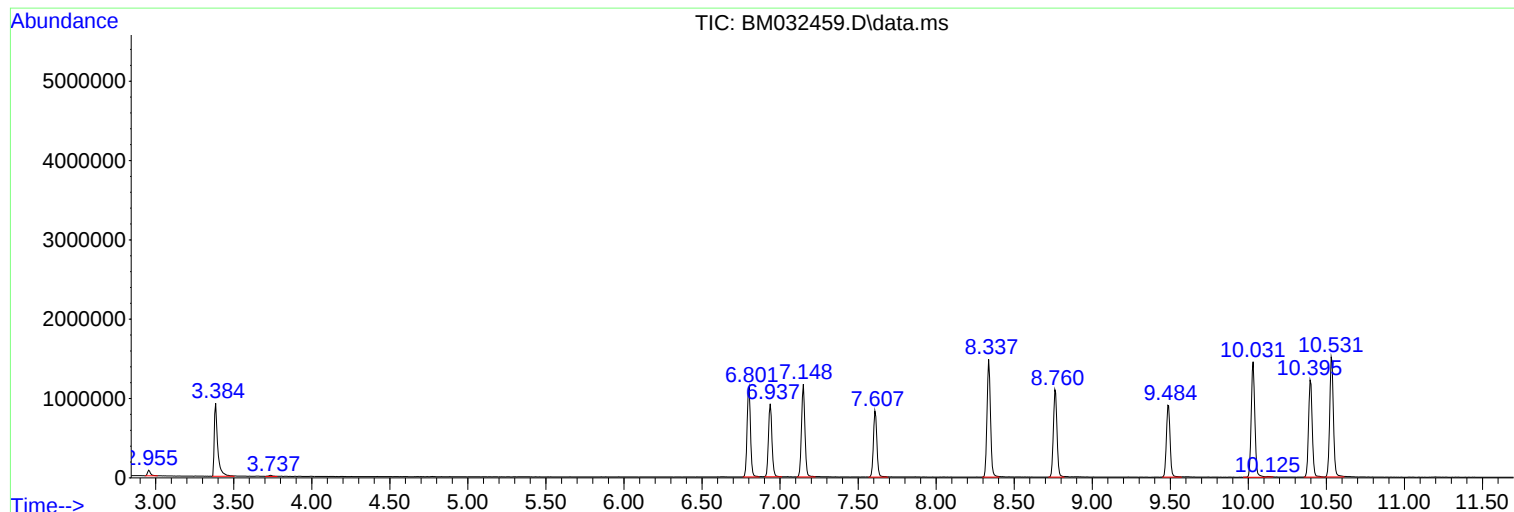

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032459.D
Acq On : 12 Oct 2021 15:55
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032459.D
Acq On : 12 Oct 2021 15:55
Operator : CG/JU
Sample : PB139788BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK788

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
