

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032472.D
 Acq On : 13 Oct 2021 00:23
 Operator : CG/JU
 Sample : PB139806BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK806

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	31	rVB	63874	91990	1.53%	0.147%
2	3.384	89	93	116	rBV	782750	1182475	19.72%	1.891%
3	3.737	148	153	159	rBV	12580	19326	0.32%	0.031%
4	6.795	666	673	688	rBV	925500	1401196	23.37%	2.240%
5	6.937	688	697	709	rVB	728375	1135496	18.94%	1.816%
6	7.148	726	733	744	rBV	933474	1453205	24.24%	2.323%
7	7.607	805	811	824	rBV	833457	1279026	21.33%	2.045%
8	8.337	928	935	947	rBV	1187606	1863266	31.07%	2.979%
9	8.760	1000	1007	1021	rBV	904070	1435921	23.95%	2.296%
10	9.484	1123	1130	1138	rBV	776971	1211674	20.21%	1.937%
11	10.025	1215	1222	1235	rBV	1184880	1898597	31.66%	3.036%
12	10.395	1276	1285	1294	rBV	1231194	2006694	33.47%	3.208%
13	10.531	1301	1308	1322	rBV	1269976	2041932	34.05%	3.265%
14	11.983	1551	1555	1564	rBV	21243	34956	0.58%	0.056%
15	13.660	1834	1840	1855	rBV	2449379	3206485	53.48%	5.127%
16	13.942	1881	1888	1906	rBV	2643229	3814887	63.62%	6.100%
17	14.254	1934	1941	1956	rBV	2083883	2937678	48.99%	4.697%
18	14.460	1970	1976	1996	rBV	992177	1470853	24.53%	2.352%
19	14.660	2008	2010	2017	rVB8	4365	7346	0.12%	0.012%
20	15.242	2102	2109	2123	rBV	3414103	4814294	80.29%	7.697%
21	15.360	2123	2129	2145	rVV	1092497	1387963	23.15%	2.219%
22	15.483	2145	2150	2155	rVB	42524	58789	0.98%	0.094%
23	15.918	2219	2224	2229	rVB8	4701	7321	0.12%	0.012%
24	16.024	2239	2242	2247	rBV5	5371	7142	0.12%	0.011%
25	16.771	2364	2369	2373	rBV2	10183	15102	0.25%	0.024%
26	16.983	2398	2405	2415	rBV	2640666	3529730	58.87%	5.644%
27	17.077	2415	2421	2436	rVV	3663190	5189823	86.55%	8.298%
28	18.930	2731	2736	2741	rBV	37290	52391	0.87%	0.084%
29	19.001	2744	2748	2753	rBV	45005	59859	1.00%	0.096%
30	19.365	2804	2810	2824	rBV	4547512	5996149	100.00%	9.587%
31	21.147	3108	3113	3119	rBV	3073984	3717186	61.99%	5.943%
32	23.153	3447	3454	3469	rVB2	3137259	5623329	93.78%	8.991%
33	23.289	3471	3477	3488	rVB2	2113276	3591869	59.90%	5.743%




Sum of corrected areas: 62543950

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032472.D
Acq On : 13 Oct 2021 00:23
Operator : CG/JU
Sample : PB139806BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK806

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

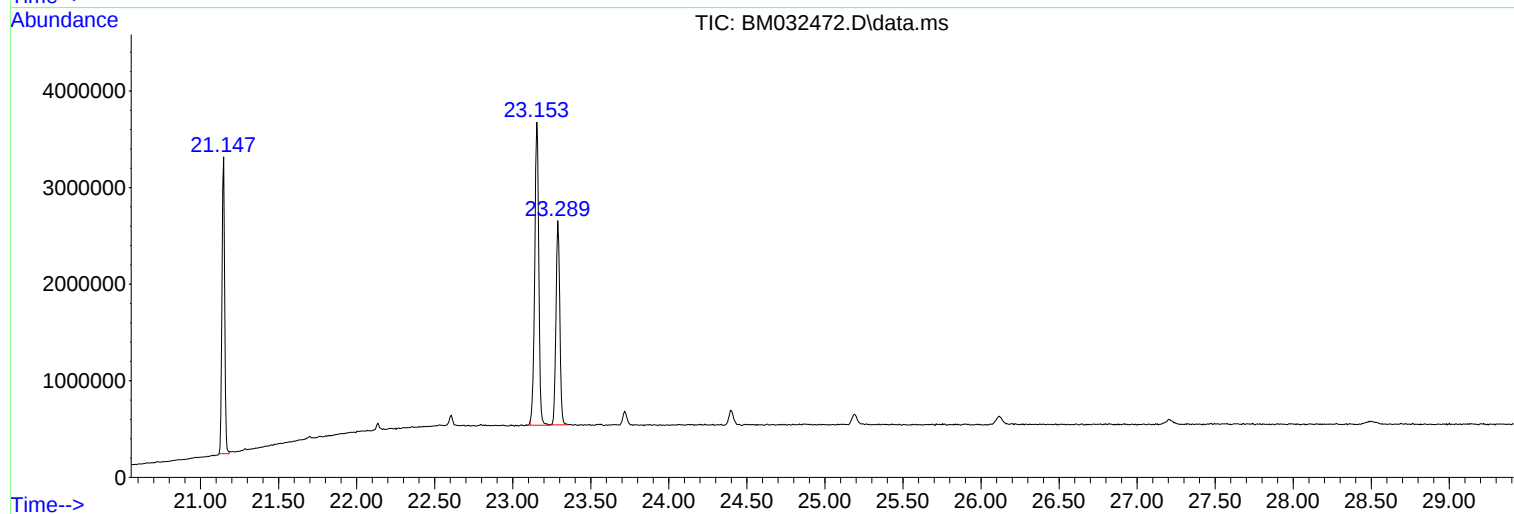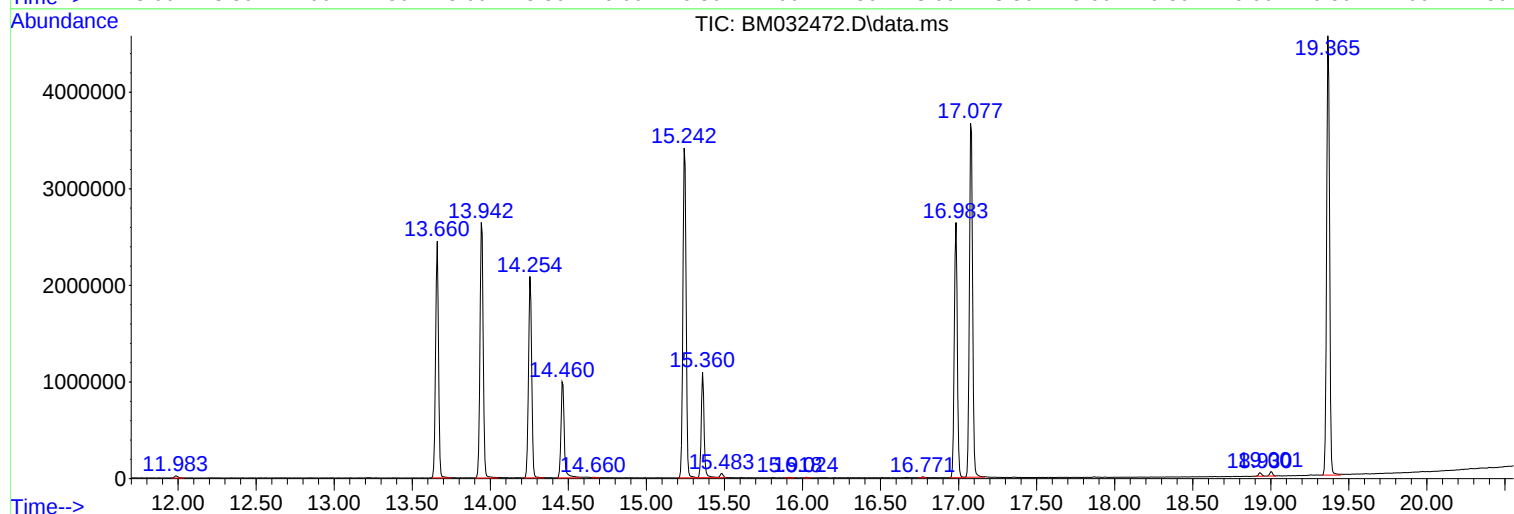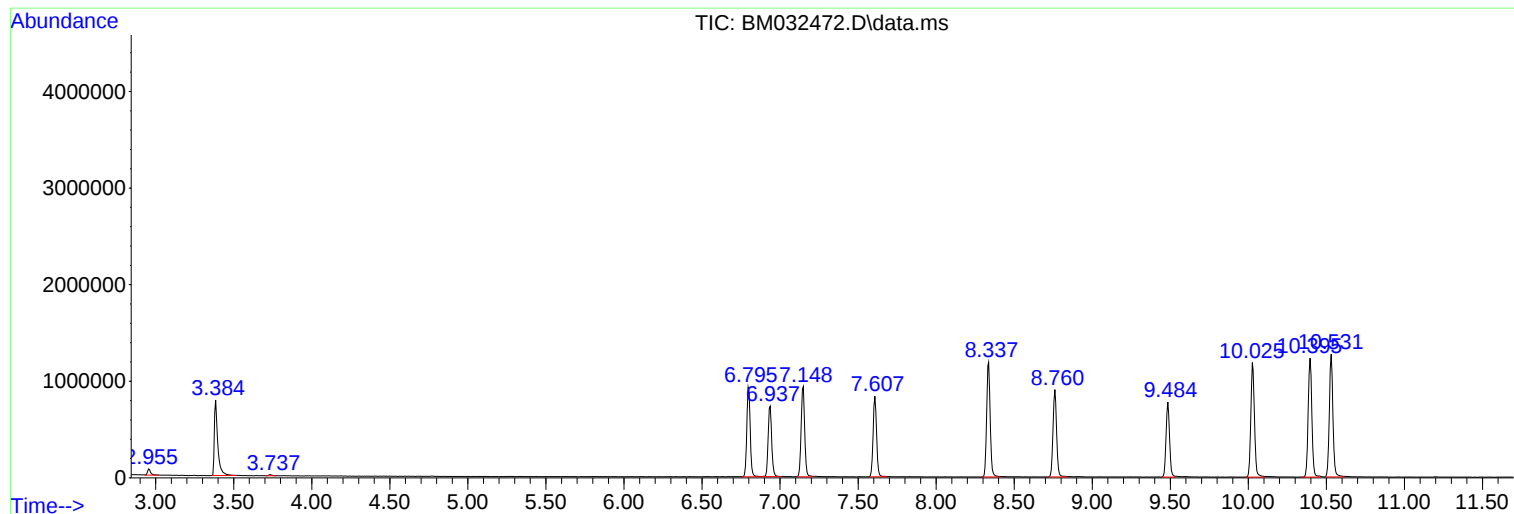

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032472.D
Acq On : 13 Oct 2021 00:23
Operator : CG/JU
Sample : PB139806BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK806

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032472.D
Acq On : 13 Oct 2021 00:23
Operator : CG/JU
Sample : PB139806BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK806

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------