

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032473.D
 Acq On : 13 Oct 2021 00:59
 Operator : CG/JU
 Sample : PB139820BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	16	20	26	rBV	62411	80383	1.30%	0.123%
2	3.384	89	93	111	rBV	817735	1251597	20.27%	1.916%
3	3.737	148	153	159	rVB	12931	20529	0.33%	0.031%
4	6.796	667	673	685	rBV	985646	1482330	24.00%	2.269%
5	6.937	690	697	710	rVB	767998	1204482	19.50%	1.844%
6	7.148	725	733	744	rBV	968518	1544187	25.00%	2.364%
7	7.607	804	811	821	rBV	860731	1326315	21.48%	2.030%
8	8.337	928	935	949	rBV	1250615	1985998	32.16%	3.040%
9	8.760	999	1007	1027	rBV	985199	1537571	24.90%	2.354%
10	9.484	1122	1130	1145	rBV	834739	1297890	21.02%	1.987%
11	10.025	1213	1222	1236	rBV	1268496	2031305	32.89%	3.110%
12	10.125	1236	1239	1245	rVB6	5625	10519	0.17%	0.016%
13	10.395	1278	1285	1300	rBV	1288077	2072257	33.55%	3.172%
14	10.531	1300	1308	1333	rBV	1324281	2184073	35.36%	3.344%
15	11.983	1550	1555	1561	rBV2	20206	34143	0.55%	0.052%
16	13.660	1833	1840	1853	rBV	2492127	3292994	53.32%	5.041%
17	13.942	1881	1888	1897	rBV	2866857	3967563	64.24%	6.074%
18	14.254	1934	1941	1952	rBV	2164265	3037627	49.19%	4.650%
19	14.460	1969	1976	1995	rBV	1031662	1533694	24.83%	2.348%
20	15.242	2103	2109	2123	rBV	3471370	4998781	80.94%	7.653%
21	15.360	2123	2129	2146	rVV	1059460	1396165	22.61%	2.137%
22	15.483	2146	2150	2156	rVB	43975	63395	1.03%	0.097%
23	16.024	2237	2242	2246	rVB6	5232	8031	0.13%	0.012%
24	16.771	2364	2369	2373	rBV2	8435	11972	0.19%	0.018%
25	16.983	2398	2405	2415	rBV	2631103	3653890	59.16%	5.594%
26	17.077	2415	2421	2441	rVB2	3897867	5416773	87.71%	8.292%
27	17.648	2515	2518	2522	rBV6	5417	6993	0.11%	0.011%
28	18.930	2732	2736	2741	rBV2	39215	51636	0.84%	0.079%
29	19.001	2744	2748	2753	rVV	47238	62252	1.01%	0.095%
30	19.254	2789	2791	2795	rBV3	6581	10111	0.16%	0.015%
31	19.365	2804	2810	2821	rBV	4687835	6175918	100.00%	9.455%
32	21.148	3108	3113	3122	rBV	3124808	3933319	63.69%	6.021%
33	23.153	3447	3454	3465	rVB2	3330923	5803038	93.96%	8.884%
34	23.289	3471	3477	3488	rVB2	2269974	3833888	62.08%	5.869%

Sum of corrected areas: 65321619

Instrument :

BNA_M

ClientSampleId :




SBLK820

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032473.D
Acq On : 13 Oct 2021 00:59
Operator : CG/JU
Sample : PB139820BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

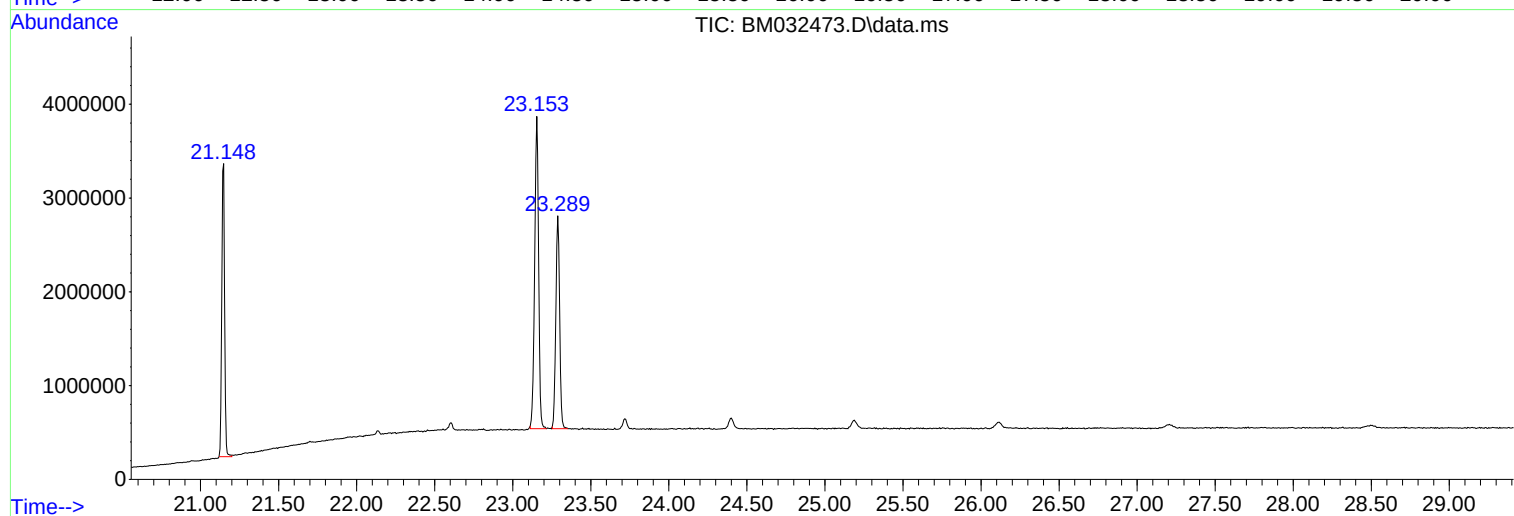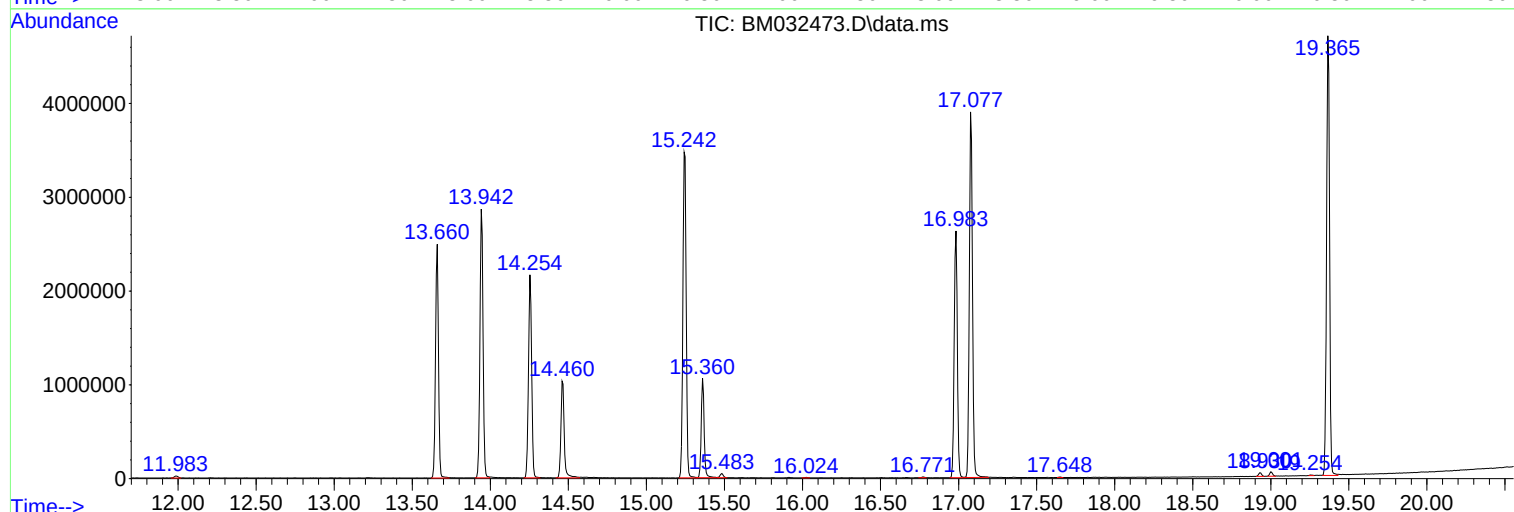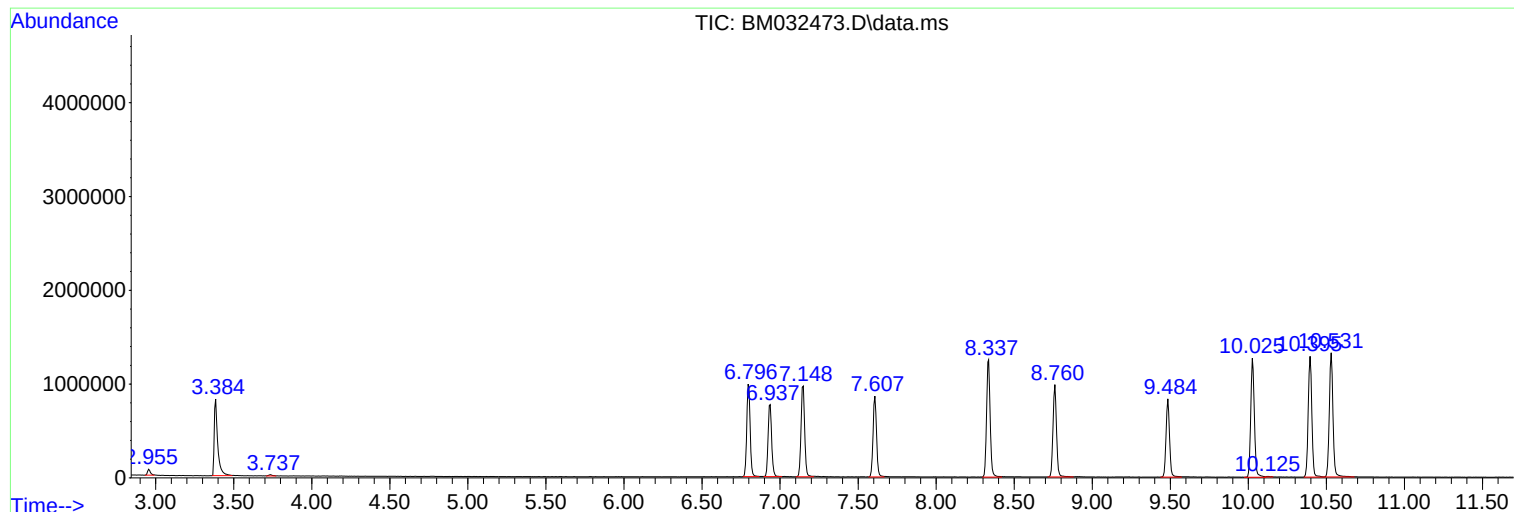

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032473.D
Acq On : 13 Oct 2021 00:59
Operator : CG/JU
Sample : PB139820BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032473.D
Acq On : 13 Oct 2021 00:59
Operator : CG/JU
Sample : PB139820BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
