

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032480.D
 Acq On : 13 Oct 2021 05:11
 Operator : CG/JU
 Sample : M4128-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.954	16	20	29	rVB	79539	108930	1.35%	0.133%
2	3.254	68	71	78	rBV	17418	21949	0.27%	0.027%
3	3.384	89	93	112	rBV	1009689	1554313	19.31%	1.905%
4	3.643	135	137	145	rVB3	11861	19310	0.24%	0.024%
5	3.737	148	153	158	rVB2	15349	22645	0.28%	0.028%
6	6.795	667	673	688	rBV	1366970	2073530	25.77%	2.541%
7	6.937	690	697	710	rVB	1021012	1581569	19.65%	1.938%
8	7.148	726	733	740	rBV	1312726	2044685	25.41%	2.506%
9	7.213	740	744	749	rVB	18395	29414	0.37%	0.036%
10	7.607	804	811	821	rBV	801258	1241213	15.42%	1.521%
11	7.684	821	824	830	rVB3	7138	12900	0.16%	0.016%
12	8.336	925	935	950	rBV	1781519	2783713	34.59%	3.411%
13	8.760	999	1007	1018	rBV	1318054	2060035	25.60%	2.525%
14	8.936	1033	1037	1041	rVB7	7633	12853	0.16%	0.016%
15	9.483	1122	1130	1143	rBV	1126789	1770655	22.00%	2.170%
16	9.589	1146	1148	1155	rVB6	5021	10681	0.13%	0.013%
17	9.736	1168	1173	1179	rBV6	8991	15345	0.19%	0.019%
18	10.025	1215	1222	1240	rBV	1739426	2821420	35.06%	3.458%
19	10.172	1241	1247	1262	rVB	1042663	1608023	19.98%	1.971%
20	10.395	1277	1285	1299	rBV	1156775	1923157	23.90%	2.357%
21	10.530	1299	1308	1322	rBV	1741496	2823317	35.08%	3.460%
22	11.201	1415	1422	1427	rBV6	8787	16099	0.20%	0.020%
23	11.924	1540	1545	1551	rVV	29287	43582	0.54%	0.053%
24	11.983	1551	1555	1563	rVB2	30782	52651	0.65%	0.065%
25	12.060	1563	1568	1575	rVB	8607	14713	0.18%	0.018%
26	12.283	1602	1606	1612	rVB3	5123	8781	0.11%	0.011%
27	12.607	1656	1661	1667	rBV2	10543	16171	0.20%	0.020%
28	12.860	1697	1704	1708	rBV	13569	21192	0.26%	0.026%
29	13.089	1739	1743	1748	rVB5	5809	9599	0.12%	0.012%
30	13.154	1750	1754	1761	rVV3	12769	19889	0.25%	0.024%
31	13.219	1761	1765	1772	rVB2	6120	8529	0.11%	0.010%
32	13.577	1820	1826	1830	rBV7	6280	11115	0.14%	0.014%
33	13.660	1832	1840	1854	rBV	3283962	4337655	53.90%	5.316%
34	13.942	1877	1888	1907	rBV	3631484	5321693	66.13%	6.522%
35	14.254	1933	1941	1953	rVV	1919482	2705574	33.62%	3.316%
36	14.401	1961	1966	1970	rBV2	12158	14483	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032480.D
 Acq On : 13 Oct 2021 05:11
 Operator : CG/JU
 Sample : M4128-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	14.460	1970	1976	1997	rBV	1385282	2071768	25.74%	2.539%
38	14.665	2006	2011	2018	rVB6	17171	36082	0.45%	0.044%
39	15.065	2074	2079	2082	rBV3	9998	16384	0.20%	0.020%
40	15.107	2084	2086	2091	rVB4	6645	9010	0.11%	0.011%
41	15.242	2102	2109	2123	rBV	4606115	6583943	81.81%	8.068%
42	15.360	2123	2129	2144	rVV	1487354	1908040	23.71%	2.338%
43	15.477	2145	2149	2156	rVB	55490	82498	1.03%	0.101%
44	15.607	2166	2171	2174	rVB6	6594	11501	0.14%	0.014%
45	15.683	2176	2184	2188	rBV5	18745	28024	0.35%	0.034%
46	15.795	2199	2203	2210	rVB8	4372	10098	0.13%	0.012%
47	15.924	2220	2225	2229	rBV6	6706	13937	0.17%	0.017%
48	16.030	2239	2243	2247	rVB4	16846	24822	0.31%	0.030%
49	16.130	2255	2260	2265	rVB8	5829	11490	0.14%	0.014%
50	16.730	2356	2362	2364	rBV5	6352	10218	0.13%	0.013%
51	16.765	2364	2368	2371	rVV4	5816	8190	0.10%	0.010%
52	16.983	2398	2405	2415	rBV	2302102	3258983	40.50%	3.994%
53	17.077	2415	2421	2433	rVV2	4956297	7005673	87.05%	8.585%
54	17.171	2433	2437	2442	rVB7	34080	51520	0.64%	0.063%
55	17.354	2464	2468	2472	rBV3	6775	10669	0.13%	0.013%
56	17.648	2513	2518	2524	rBV	63940	77052	0.96%	0.094%
57	17.871	2550	2556	2564	rBV	98850	148368	1.84%	0.182%
58	17.936	2564	2567	2572	rVB	13866	18506	0.23%	0.023%
59	18.348	2631	2637	2642	rBV8	4468	10091	0.13%	0.012%
60	18.930	2732	2736	2742	rVB2	61641	81662	1.01%	0.100%
61	19.000	2744	2748	2751	rVV	66950	88984	1.11%	0.109%
62	19.030	2751	2753	2758	rVB	19062	20712	0.26%	0.025%
63	19.148	2770	2773	2778	rBV6	7439	8936	0.11%	0.011%
64	19.365	2804	2810	2825	rBV	6047309	8047852	100.00%	9.862%
65	20.847	3059	3062	3067	rBV2	147487	178280	2.22%	0.218%
66	21.142	3107	3112	3118	rBV	2876344	3530090	43.86%	4.326%
67	23.153	3446	3454	3466	rVB2	4203826	7690771	95.56%	9.425%
68	23.283	3471	3476	3489	rVB2	1988950	3406021	42.32%	4.174%




Sum of corrected areas: 81601558

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032480.D
Acq On : 13 Oct 2021 05:11
Operator : CG/JU
Sample : M4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

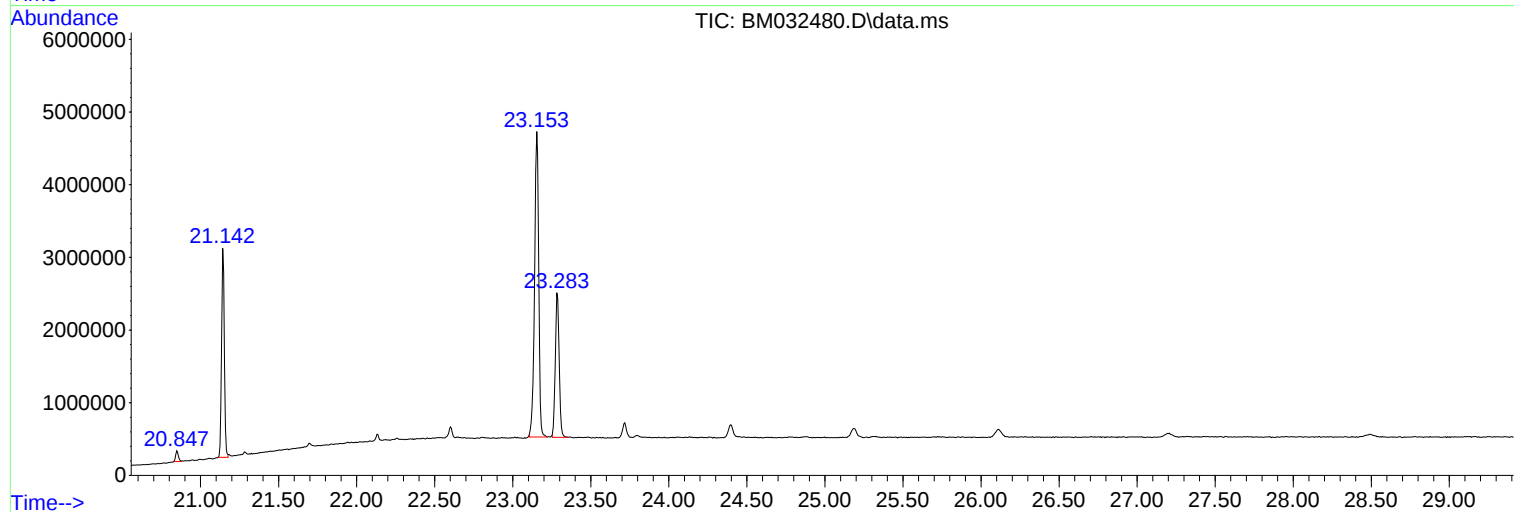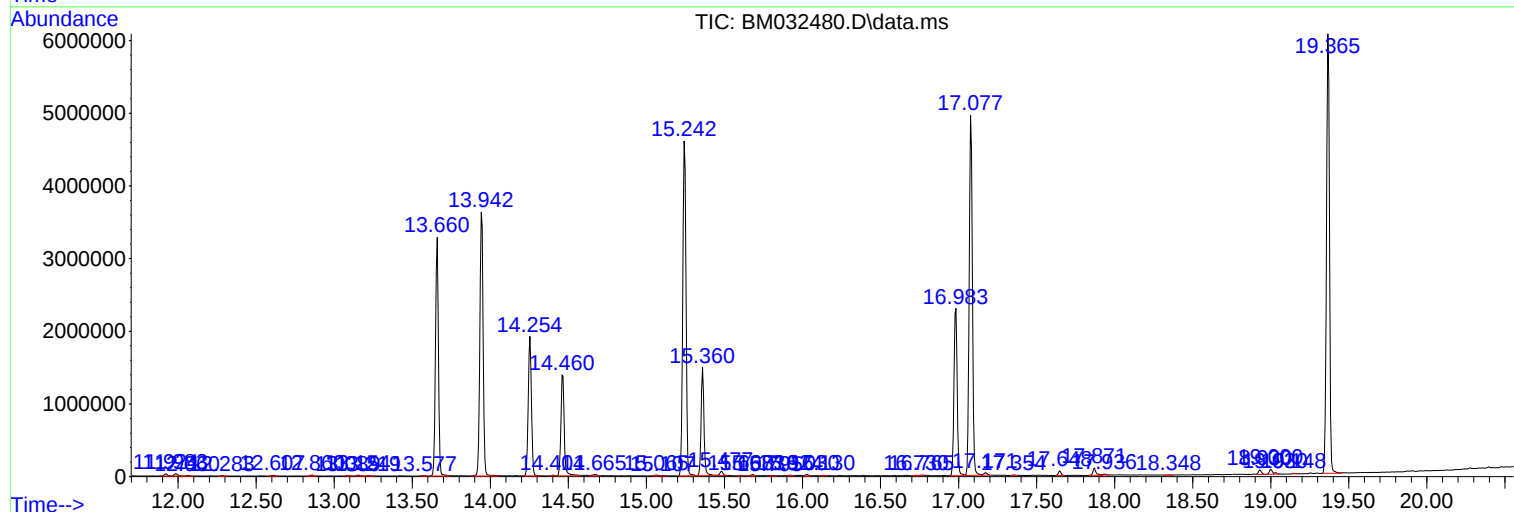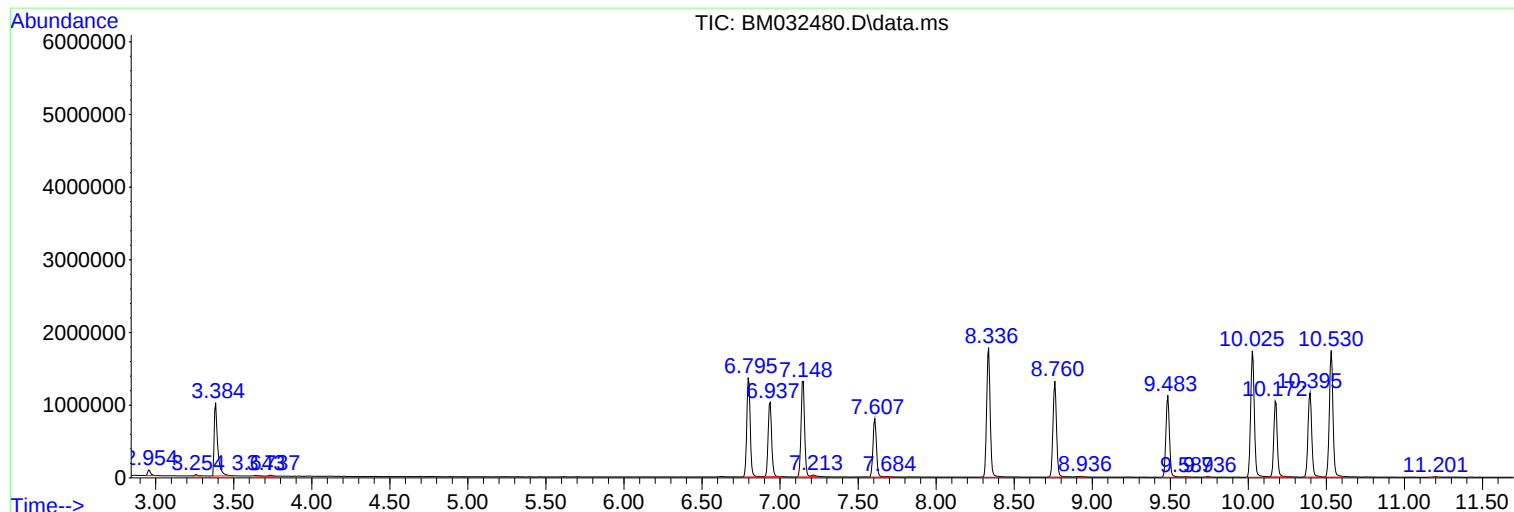

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032480.D
Acq On : 13 Oct 2021 05:11
Operator : CG/JU
Sample : M4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB7










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.172	16.72 ng/ul	1608020	Naphthalene-d8	10.395

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

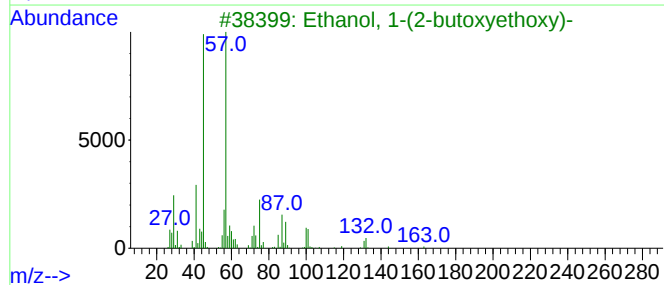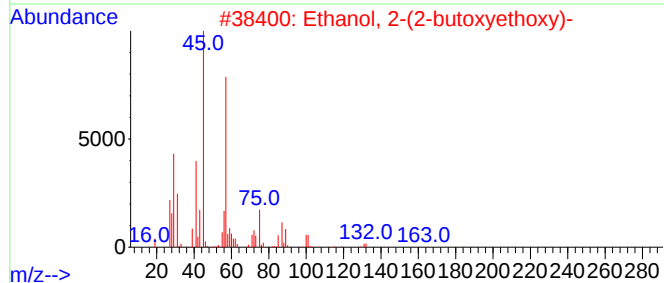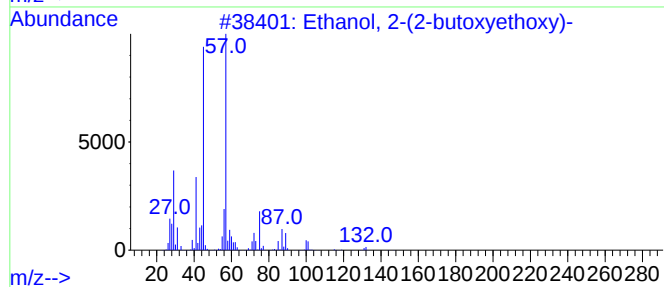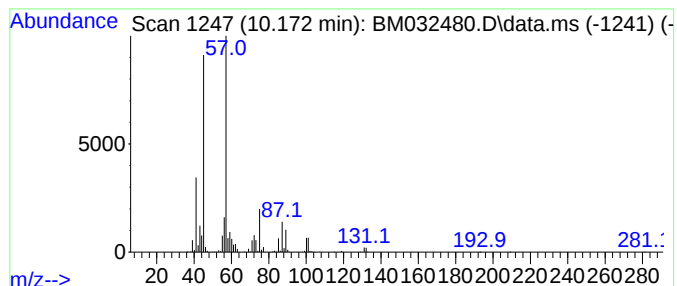

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032480.D
Acq On : 13 Oct 2021 05:11
Operator : CG/JU
Sample : M4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.172	16.7	ng/ul	1608020	2	10.395	1923160	20.0