

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032482.D
 Acq On : 13 Oct 2021 06:22
 Operator : CG/JU
 Sample : M4128-08
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.955	17	20	28	rVB	22279	32555	0.98%	0.108%
2	3.390	91	94	107	rBV	169432	273444	8.26%	0.903%
3	3.643	132	137	145	rVB	32459	55636	1.68%	0.184%
4	3.731	148	152	159	rBV	23167	36036	1.09%	0.119%
5	4.119	216	218	225	rVB6	4537	8626	0.26%	0.028%
6	4.690	311	315	320	rBV	9709	13347	0.40%	0.044%
7	5.319	420	422	426	rVB5	3053	3844	0.12%	0.013%
8	5.631	468	475	480	rBV10	3740	8476	0.26%	0.028%
9	6.796	667	673	683	rBV	317442	476149	14.38%	1.573%
10	6.931	691	696	708	rVB	244104	386621	11.68%	1.277%
11	7.143	725	732	743	rBV	321243	507268	15.32%	1.676%
12	7.248	747	750	756	rVB4	9101	14706	0.44%	0.049%
13	7.431	777	781	785	rBV6	2490	3813	0.12%	0.013%
14	7.607	803	811	823	rBV	699194	1104507	33.35%	3.649%
15	7.866	852	855	858	rVB5	3048	3702	0.11%	0.012%
16	8.331	928	934	944	rBV	398583	613254	18.52%	2.026%
17	8.431	946	951	960	rVB	17321	33241	1.00%	0.110%
18	8.760	1000	1007	1014	rBV	280404	462895	13.98%	1.529%
19	8.931	1032	1036	1041	rVB8	3628	8261	0.25%	0.027%
20	9.231	1082	1087	1092	rVB9	2790	4852	0.15%	0.016%
21	9.484	1123	1130	1143	rBV	220952	362484	10.95%	1.198%
22	10.025	1214	1222	1238	rBV	373907	612591	18.50%	2.024%
23	10.172	1242	1247	1255	rVV	91067	139681	4.22%	0.461%
24	10.395	1277	1285	1300	rBV	1014916	1684979	50.88%	5.567%
25	10.531	1300	1308	1324	rVV	362710	626584	18.92%	2.070%
26	10.931	1373	1376	1380	rVB6	3379	5338	0.16%	0.018%
27	11.195	1414	1421	1423	rBV6	4794	8058	0.24%	0.027%
28	11.889	1533	1539	1542	rVB5	2579	3777	0.11%	0.012%
29	11.983	1550	1555	1564	rVB4	6901	12772	0.39%	0.042%
30	12.054	1564	1567	1571	rBV4	2943	3435	0.10%	0.011%
31	12.607	1657	1661	1666	rBV5	6065	8664	0.26%	0.029%
32	12.860	1699	1704	1707	rBV3	7164	10477	0.32%	0.035%
33	13.160	1750	1755	1759	rBV5	4650	6728	0.20%	0.022%
34	13.572	1823	1825	1830	rVB6	3092	3848	0.12%	0.013%
35	13.654	1832	1839	1854	rVV	790373	1054458	31.84%	3.484%
36	13.942	1882	1888	1897	rBV	838898	1163024	35.12%	3.842%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
 Data File : BM032482.D
 Acq On : 13 Oct 2021 06:22
 Operator : CG/JU
 Sample : M4128-08
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

37	14.254	1934	1941	1954	rBV	1721087	2422876	73.17%	8.004%
38	14.395	1962	1965	1970	rVB5	2357	3358	0.10%	0.011%
39	14.460	1970	1976	1992	rBV	211765	341300	10.31%	1.128%
40	14.666	2005	2011	2018	rVB8	12685	24104	0.73%	0.080%
41	15.066	2072	2079	2082	rBV3	6170	10346	0.31%	0.034%
42	15.107	2083	2086	2091	rVB5	2192	3534	0.11%	0.012%
43	15.242	2103	2109	2123	rBV	1162316	1608270	48.57%	5.313%
44	15.360	2123	2129	2142	rVV	194075	288249	8.70%	0.952%
45	15.477	2146	2149	2154	rVV	12684	16597	0.50%	0.055%
46	15.601	2166	2170	2174	rVB7	2077	3739	0.11%	0.012%
47	15.683	2182	2184	2187	rVB4	3995	3566	0.11%	0.012%
48	15.918	2220	2224	2229	rBV	12957	21371	0.65%	0.071%
49	16.030	2239	2243	2247	rBV6	6542	8385	0.25%	0.028%
50	16.236	2274	2278	2281	rBV4	3453	4699	0.14%	0.016%
51	16.771	2359	2369	2373	rBV3	7794	17220	0.52%	0.057%
52	16.977	2398	2404	2415	rVV	2069605	2937436	88.70%	9.704%
53	17.077	2415	2421	2433	rVV	1249097	1752486	52.92%	5.790%
54	17.171	2433	2437	2444	rVB3	28004	42219	1.27%	0.139%
55	17.477	2485	2489	2492	rBV6	2410	3710	0.11%	0.012%
56	17.648	2514	2518	2522	rBV	12478	15400	0.47%	0.051%
57	17.865	2551	2555	2560	rBV2	30277	38725	1.17%	0.128%
58	17.936	2563	2567	2571	rVB	9873	13034	0.39%	0.043%
59	18.154	2602	2604	2611	rVB7	2459	4316	0.13%	0.014%
60	18.659	2688	2690	2698	rVB10	4581	5457	0.16%	0.018%
61	18.930	2732	2736	2742	rVB7	15287	27120	0.82%	0.090%
62	19.001	2745	2748	2750	rVV3	13169	17183	0.52%	0.057%
63	19.030	2750	2753	2758	rVB2	12108	19596	0.59%	0.065%
64	19.365	2804	2810	2821	rBV	1665683	2168222	65.48%	7.163%
65	20.848	3060	3062	3069	rVB5	50173	53389	1.61%	0.176%
66	21.142	3107	3112	3121	rBV	2621337	3311496	100.00%	10.940%
67	23.147	3447	3453	3465	rVB2	1194836	2127183	64.24%	7.027%
68	23.283	3470	3476	3492	rVB2	1830400	3196876	96.54%	10.561%




Sum of corrected areas: 30269593

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032482.D
Acq On : 13 Oct 2021 06:22
Operator : CG/JU
Sample : M4128-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

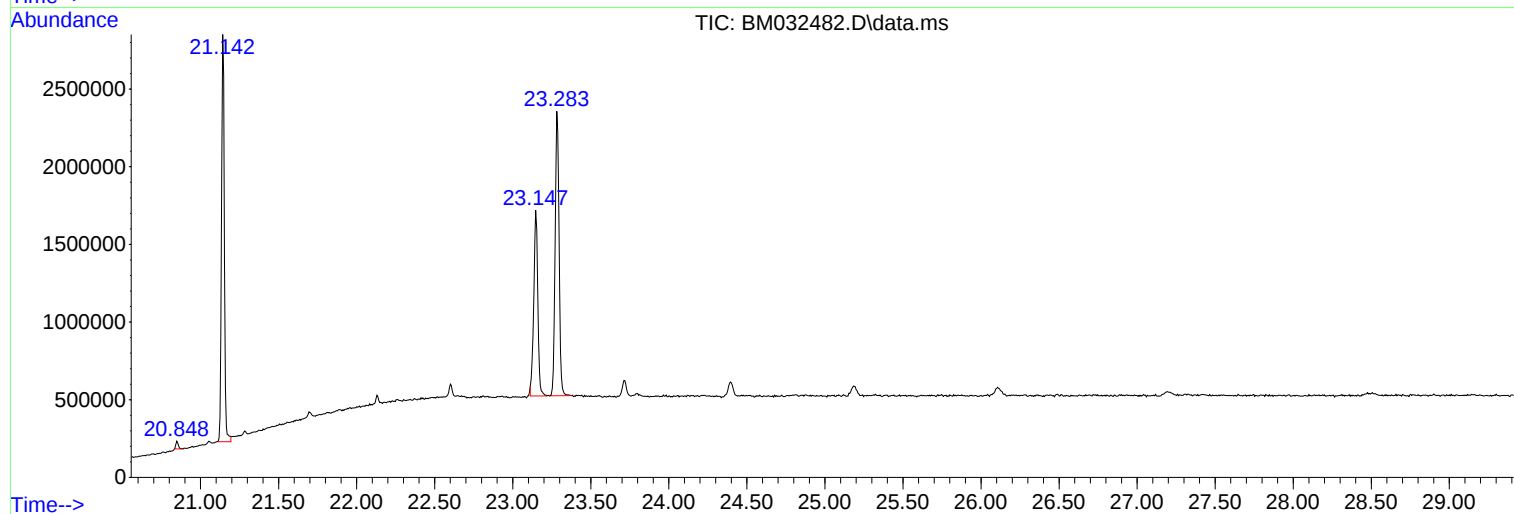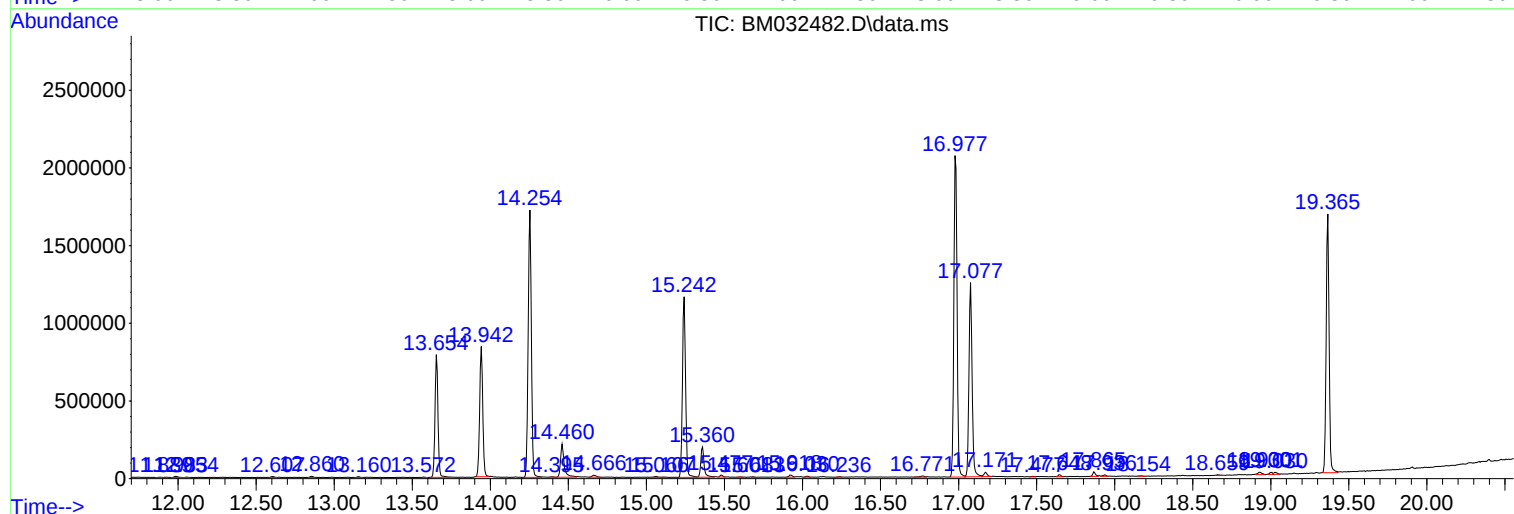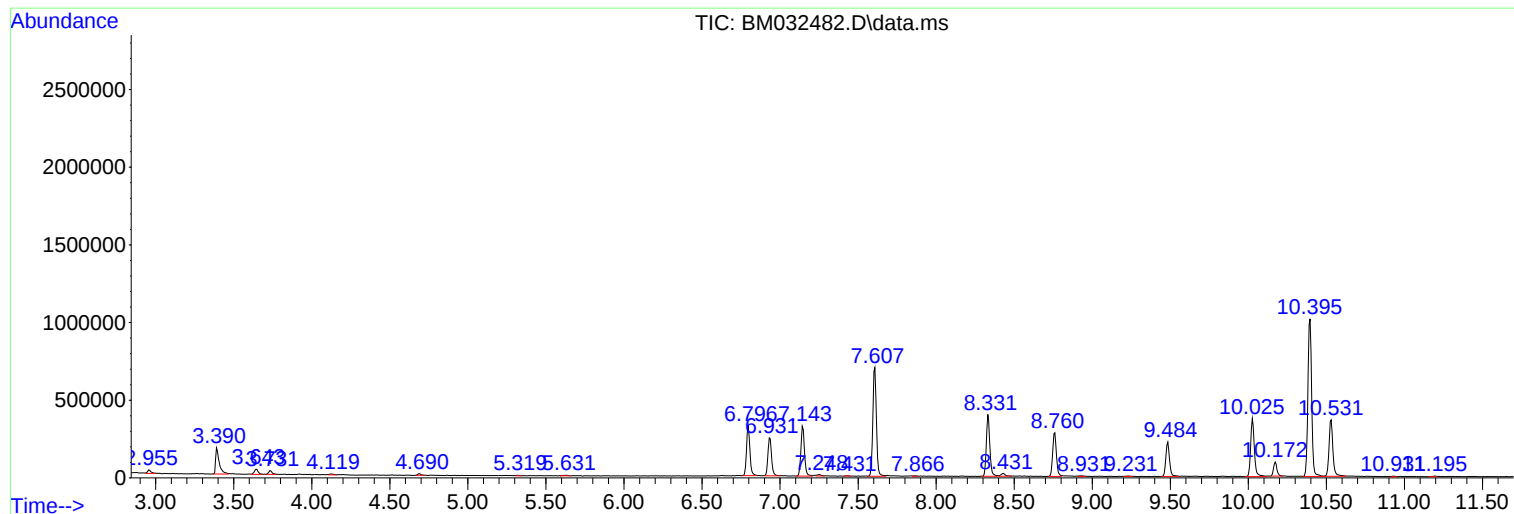

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032482.D
Acq On : 13 Oct 2021 06:22
Operator : CG/JU
Sample : M4128-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101121\
Data File : BM032482.D
Acq On : 13 Oct 2021 06:22
Operator : CG/JU
Sample : M4128-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
