

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
 Data File : BM048014.D
 Acq On : 11 Oct 2024 17:17
 Operator : RC/JU
 Sample : P4300-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.981	166	169	173	rVB4	9396	11603	0.66%	0.155%
2	4.893	322	324	325	rBV	3478	2317	0.13%	0.031%
3	5.028	345	347	348	rBV2	2318	1799	0.10%	0.024%
4	5.157	368	369	371	rBV2	2610	2050	0.12%	0.027%
5	5.593	440	443	446	rBV5	2971	3891	0.22%	0.052%
6	5.740	464	468	469	rBV4	2068	2847	0.16%	0.038%
7	5.781	473	475	478	rVB4	2205	1997	0.11%	0.027%
8	6.216	545	549	550	rBV4	2245	2736	0.15%	0.036%
9	6.569	607	609	612	rBV4	3306	2490	0.14%	0.033%
10	6.657	623	624	627	rVB3	2096	2119	0.12%	0.028%
11	6.857	656	658	662	rVB4	2528	2807	0.16%	0.037%
12	6.922	667	669	675	rVB4	3517	6060	0.34%	0.081%
13	7.040	686	689	691	rBV3	2605	2526	0.14%	0.034%
14	7.275	725	729	732	rVB5	2199	2216	0.13%	0.030%
15	7.563	776	778	780	rBV3	2395	1857	0.10%	0.025%
16	7.598	780	784	787	rVB5	2369	3166	0.18%	0.042%
17	7.710	799	803	804	rVB4	2722	3097	0.17%	0.041%
18	7.781	807	815	831	rBV	382060	689667	38.93%	9.197%
19	8.222	888	890	893	rBV4	1860	2473	0.14%	0.033%
20	8.681	965	968	971	rBV4	1966	2329	0.13%	0.031%
21	8.787	984	986	991	rVB4	1907	2433	0.14%	0.032%
22	9.363	1077	1084	1091	rBV6	7289	16000	0.90%	0.213%
23	9.628	1126	1129	1132	rBV4	1817	2016	0.11%	0.027%
24	9.722	1143	1145	1147	rVB3	2280	1943	0.11%	0.026%
25	9.751	1147	1150	1152	rBV3	1706	2420	0.14%	0.032%
26	9.822	1158	1162	1165	rVB4	2702	3026	0.17%	0.040%
27	9.986	1186	1190	1191	rBV4	2078	2666	0.15%	0.036%
28	10.104	1207	1210	1213	rVB3	2170	3051	0.17%	0.041%
29	10.181	1220	1223	1226	rBV4	2313	2497	0.14%	0.033%
30	10.257	1235	1236	1240	rBV4	1912	2035	0.11%	0.027%
31	10.322	1245	1247	1249	rBV3	2188	2521	0.14%	0.034%
32	10.381	1255	1257	1261	rVB4	3285	3025	0.17%	0.040%
33	10.433	1263	1266	1270	rBV6	2023	3308	0.19%	0.044%
34	10.475	1270	1273	1275	rBV3	1880	2141	0.12%	0.029%
35	10.575	1282	1290	1304	rBV	452335	860361	48.57%	11.473%
36	10.686	1307	1309	1317	rVV5	8676	17112	0.97%	0.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
 Data File : BM048014.D
 Acq On : 11 Oct 2024 17:17
 Operator : RC/JU
 Sample : P4300-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	10.828	1331	1333	1336	rBV3	1920	1789	0.10%	0.024%
38	11.022	1361	1366	1368	rBV5	1432	2391	0.13%	0.032%
39	11.469	1439	1442	1443	rBV3	2150	1949	0.11%	0.026%
40	11.528	1450	1452	1455	rVV3	2399	2315	0.13%	0.031%
41	11.563	1455	1458	1460	rVB3	1936	2216	0.13%	0.030%
42	11.857	1504	1508	1512	rVB5	5210	8609	0.49%	0.115%
43	12.280	1578	1580	1584	rBV4	3018	3059	0.17%	0.041%
44	12.375	1593	1596	1599	rBV4	1633	2287	0.13%	0.030%
45	12.539	1620	1624	1626	rBV4	1426	1967	0.11%	0.026%
46	12.657	1641	1644	1646	rVB3	1798	2089	0.12%	0.028%
47	13.116	1720	1722	1726	rVV3	2094	2570	0.15%	0.034%
48	13.210	1736	1738	1742	rVB2	2691	2574	0.15%	0.034%
49	13.404	1769	1771	1773	rBV	2464	2515	0.14%	0.034%
50	13.527	1789	1792	1794	rVB3	2034	1851	0.10%	0.025%
51	13.545	1794	1795	1799	rBV4	1638	2025	0.11%	0.027%
52	13.592	1799	1803	1807	rBV4	1850	2886	0.16%	0.038%
53	13.857	1844	1848	1850	rBV3	3864	3848	0.22%	0.051%
54	13.963	1864	1866	1870	rBV6	2202	3199	0.18%	0.043%
55	14.151	1894	1898	1900	rBV3	1612	2178	0.12%	0.029%
56	14.263	1912	1917	1922	rBV5	7994	18055	1.02%	0.241%
57	14.416	1936	1943	1960	rBV	685350	1091018	61.59%	14.549%
58	14.739	1995	1998	2001	rVB2	1750	2039	0.12%	0.027%
59	14.874	2018	2021	2023	rBV4	2135	2648	0.15%	0.035%
60	14.933	2026	2031	2033	rBV3	2028	2809	0.16%	0.037%
61	15.033	2045	2048	2051	rVB5	1536	1943	0.11%	0.026%
62	15.063	2051	2053	2056	rBV4	1502	1902	0.11%	0.025%
63	15.404	2110	2111	2115	rVB3	2433	2652	0.15%	0.035%
64	15.445	2115	2118	2120	rVB3	1507	1944	0.11%	0.026%
65	15.474	2120	2123	2124	rBV	2675	2888	0.16%	0.039%
66	15.674	2155	2157	2159	rBV3	2149	1807	0.10%	0.024%
67	15.727	2164	2166	2169	rVB3	1703	2137	0.12%	0.028%
68	15.910	2195	2197	2199	rBV2	1782	2068	0.12%	0.028%
69	15.986	2208	2210	2212	rBV2	2696	2122	0.12%	0.028%
70	16.198	2244	2246	2247	rBV2	2376	2019	0.11%	0.027%
71	16.415	2279	2283	2286	rBV5	2012	2659	0.15%	0.035%
72	16.610	2312	2316	2319	rBV5	2306	3547	0.20%	0.047%
73	16.657	2321	2324	2327	rVB4	1902	2038	0.12%	0.027%
74	16.933	2369	2371	2372	rBV	2362	1922	0.11%	0.026%
75	17.157	2403	2409	2424	rBV	735074	1176522	66.42%	15.689%
76	17.451	2455	2459	2462	rVV5	1928	2954	0.17%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
 Data File : BM048014.D
 Acq On : 11 Oct 2024 17:17
 Operator : RC/JU
 Sample : P4300-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	17.480	2462	2464	2467	rVB4	2573	2581	0.15%	0.034%
78	17.692	2497	2500	2501	rBV2	2716	2796	0.16%	0.037%
79	17.815	2520	2521	2524	rBV2	3996	3827	0.22%	0.051%
80	17.886	2531	2533	2535	rVB3	3109	2610	0.15%	0.035%
81	17.921	2536	2539	2540	rVV3	2740	1966	0.11%	0.026%
82	18.009	2553	2554	2557	rBV3	2663	2569	0.15%	0.034%
83	18.051	2557	2561	2569	rBV4	26768	58732	3.32%	0.783%
84	18.668	2664	2666	2667	rBV2	3545	2526	0.14%	0.034%
85	18.904	2704	2706	2707	rVB2	4346	2066	0.12%	0.028%
86	19.103	2738	2740	2742	rBV2	4079	3912	0.22%	0.052%
87	19.327	2775	2778	2785	rBV8	14934	26554	1.50%	0.354%
88	21.380	3121	3127	3142	rBV	939880	1560973	88.12%	20.816%
89	24.362	3627	3634	3652	rVB	698828	1771363	100.00%	23.621%




Sum of corrected areas: 7499087

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
Data File : BM048014.D
Acq On : 11 Oct 2024 17:17
Operator : RC/JU
Sample : P4300-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

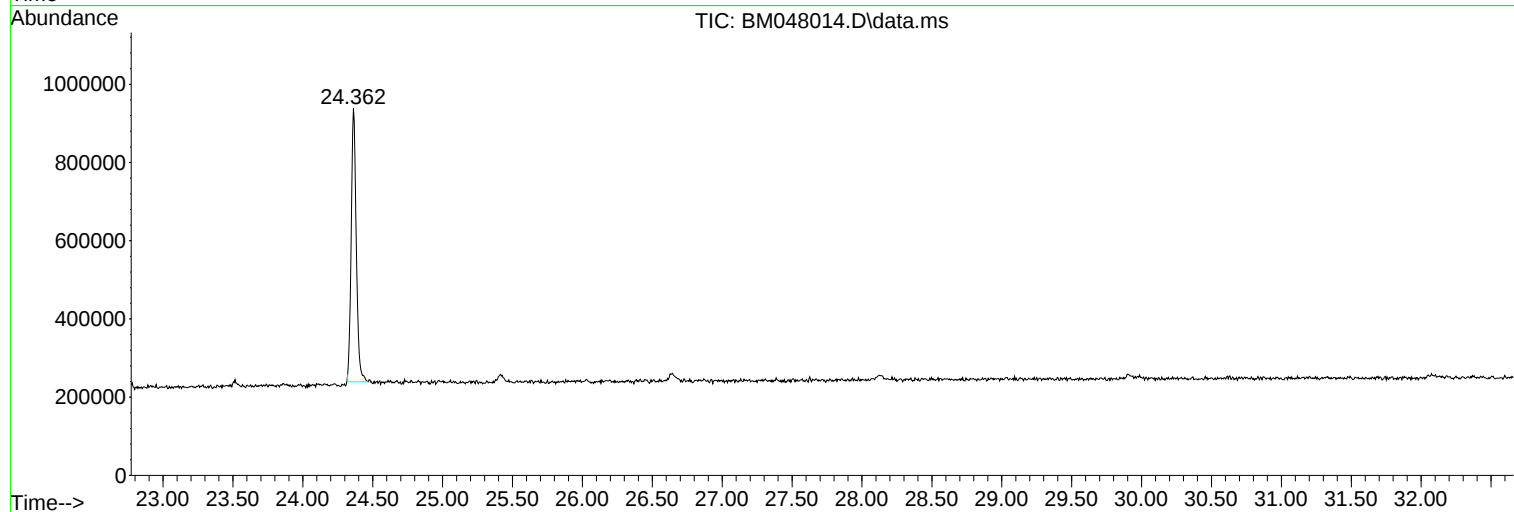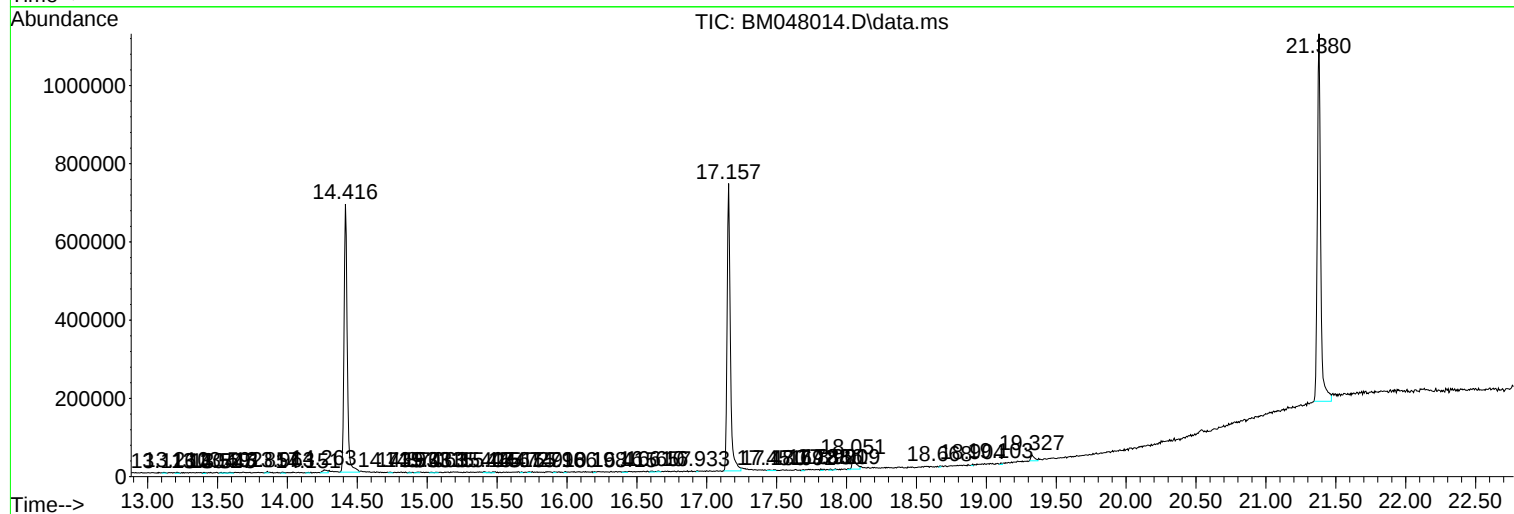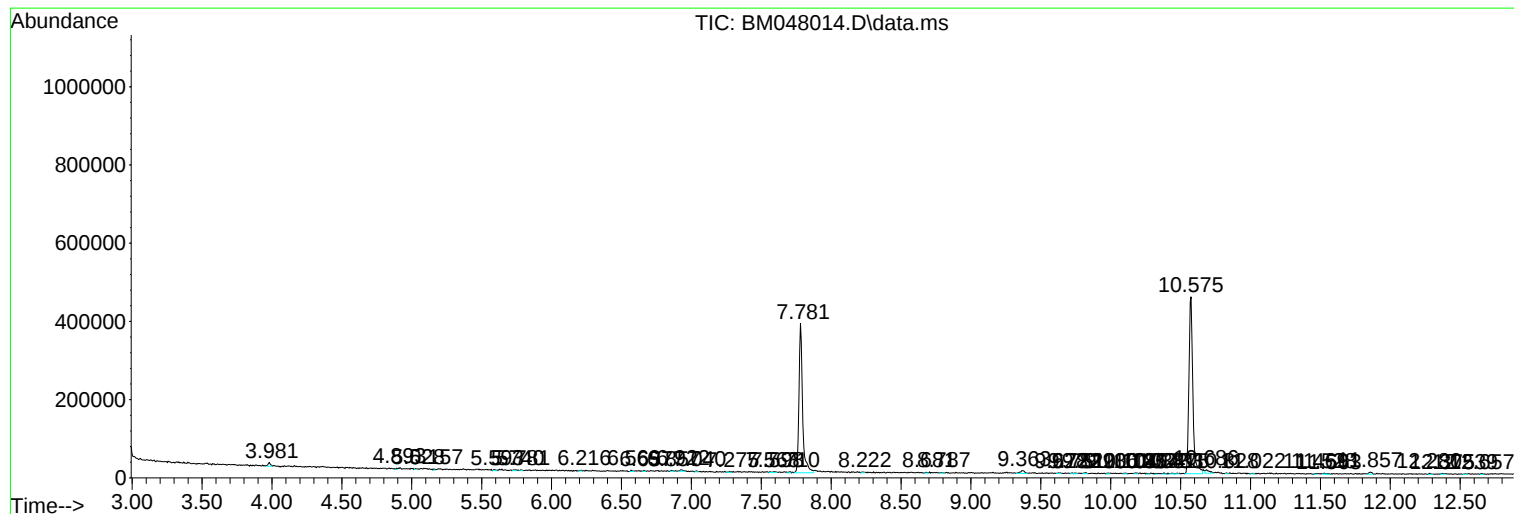

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
Data File : BM048014.D
Acq On : 11 Oct 2024 17:17
Operator : RC/JU
Sample : P4300-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101124\
Data File : BM048014.D
Acq On : 11 Oct 2024 17:17
Operator : RC/JU
Sample : P4300-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc