

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
 Data File : BM017139.D
 Acq On : 12 Oct 2018 20:31
 Operator : MJ/SJ
 Sample : J5362-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 12 23:40:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	215349	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1012813	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	584809	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1240784	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	921128	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	926801	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	23532	5.43	ng/uL	0.00
5) Phenol-d5	6.86	99	137659	7.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	358221	32.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	427923	28.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	273410	19.38	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	277248	37.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	290952	38.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	525194	33.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	3147	0.17	ng/ul	0.00
44) Dimethylphthalate-d6	13.74	166	1806233	38.93	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	2250165	37.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	24401	2.78	ng/ul	0.00
58) Fluorene-d10	15.33	176	1612090	39.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	166436	22.75	ng/ul	0.00
71) Anthracene-d10	17.18	188	2324714	39.23	ng/ul	0.00
79) Pyrene-d10	19.47	212	2146395	51.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	1903009	40.11	ng/ul	0.00


Target Compounds				Ovalue	
46) 2,6-Dinitrotoluene	13.75	165	12439	1.608	ng/ul# 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017139.D
Acq On : 12 Oct 2018 20:31
Operator : MJ/SJ
Sample : J5362-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 12 23:40:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

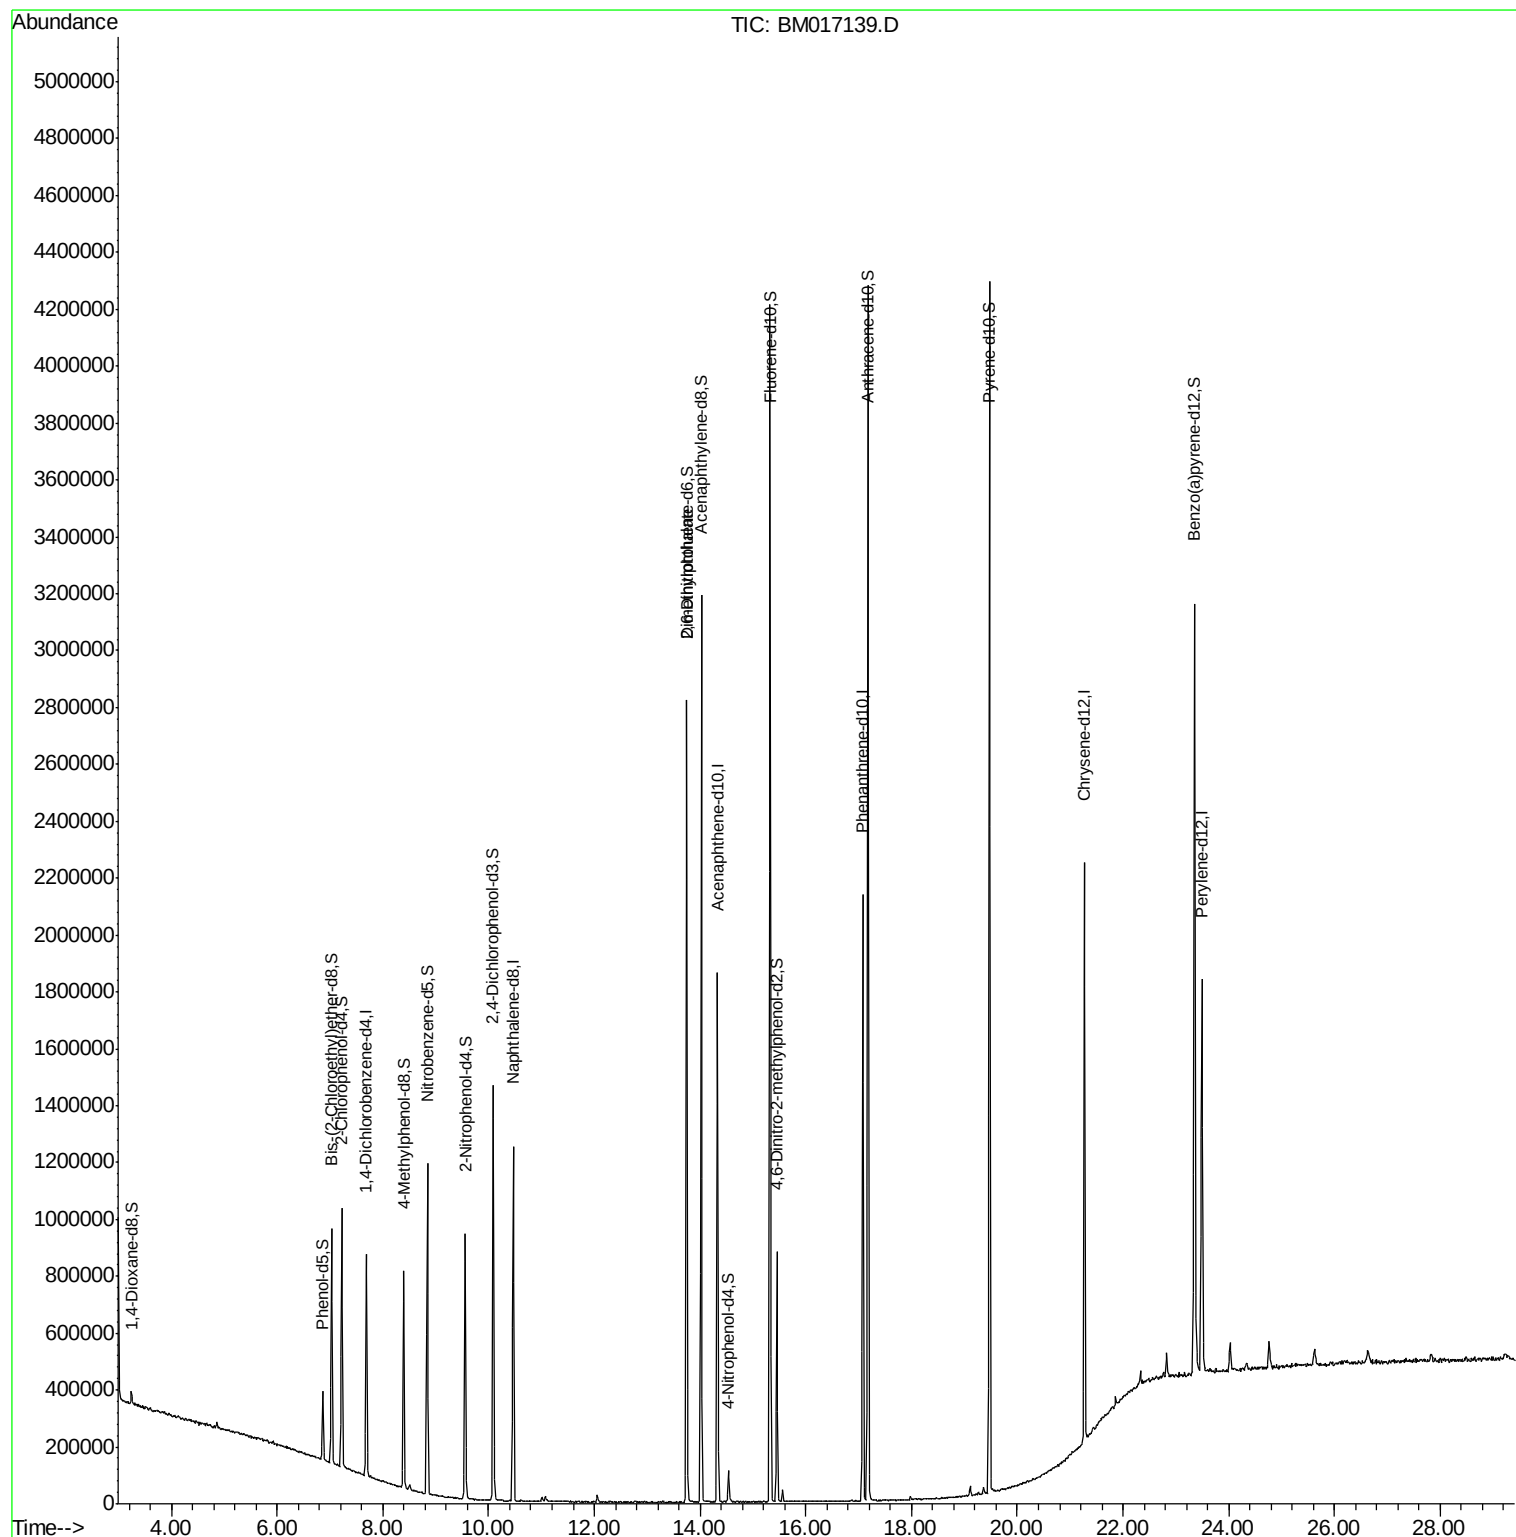

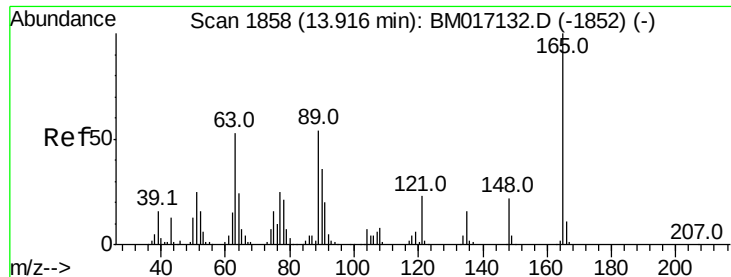

#46
 2,6-Dinitrotoluene
 Concen: 1.608 ng/ul
 RT: 13.75 min Scan# 1830
 Delta R.T. -0.16 min
 Lab File: BM017139.D
 Acq: 12 Oct 2018 20:31

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.0	64.6#
121	25.8	18.0	27.0

