


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017135.D
Acq On : 12 Oct 2018 18:07
Operator : MJ/SJ
Sample : J5362-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

Sohil
10/15/2018 3:57:51 PM

Quant Time: Oct 12 23:58:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

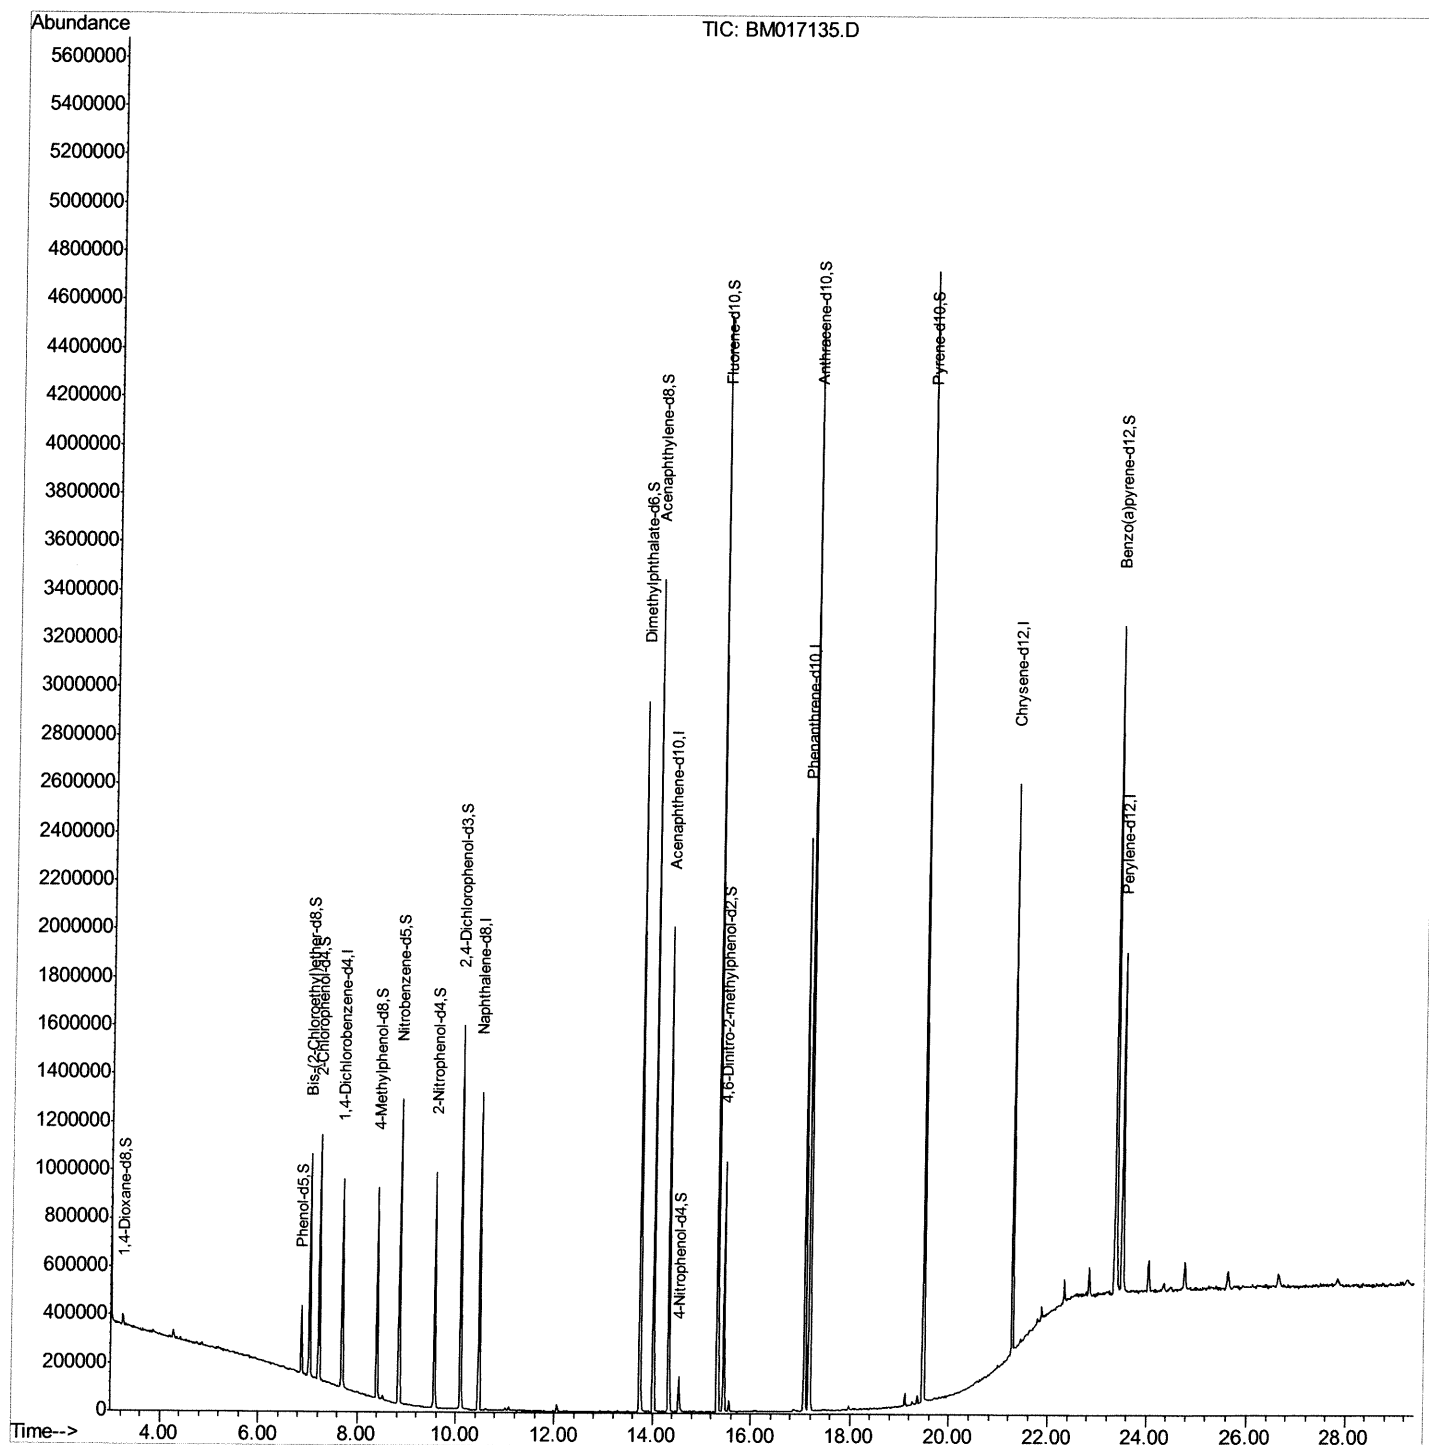

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017135.D
Acq On : 12 Oct 2018 18:07
Operator : MJ/SJ
Sample : J5362-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

Sohil
10/15/2018 3:57:51 PM

Quant Time: Oct 12 23:39:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

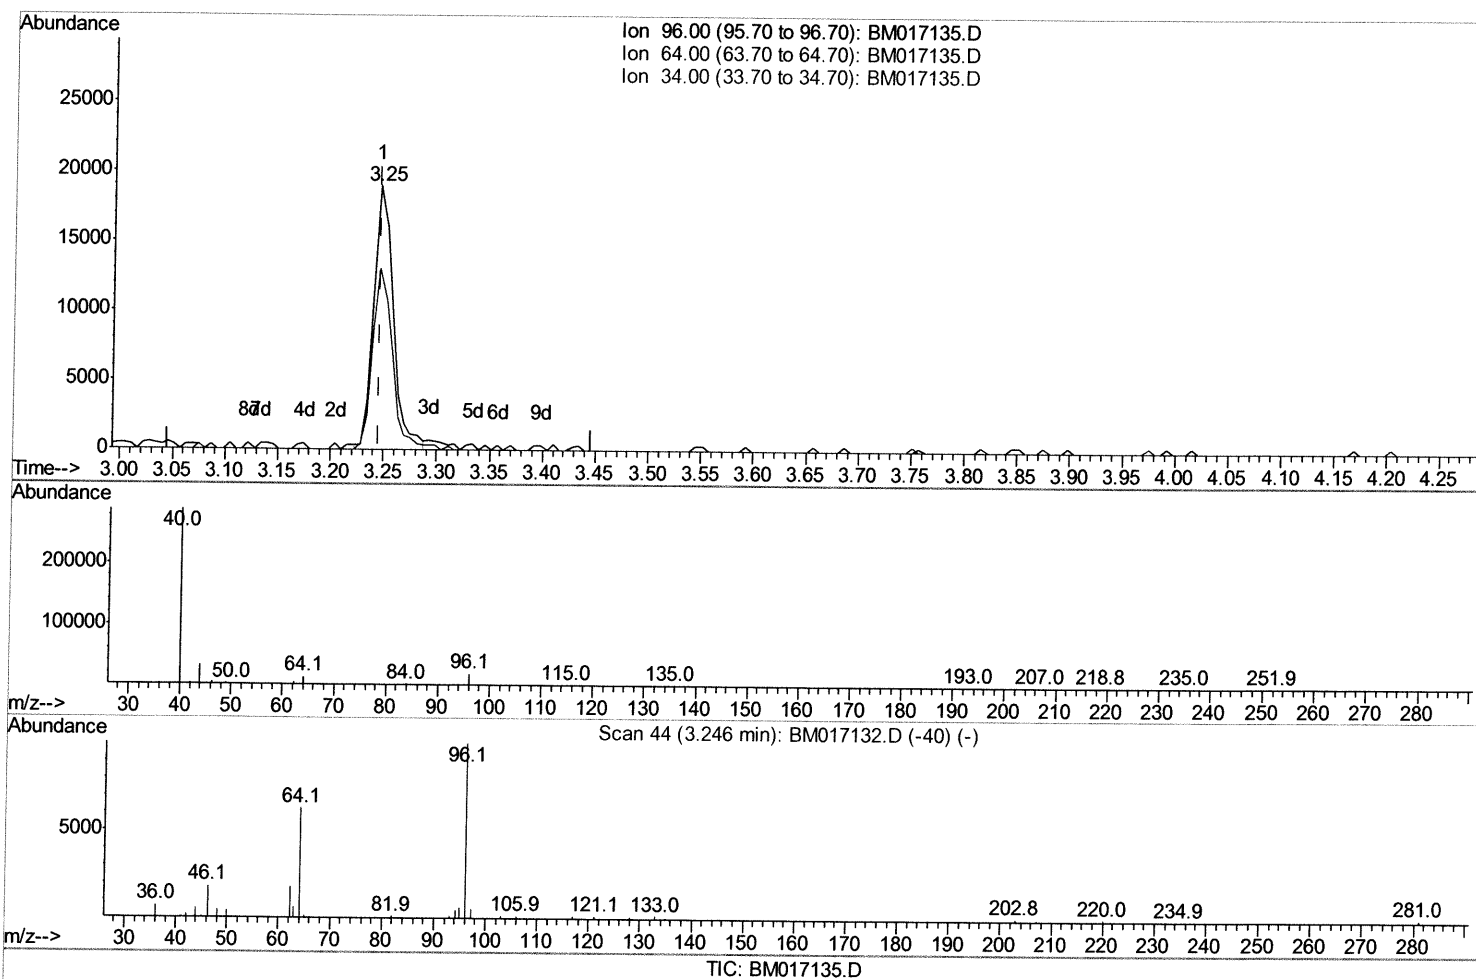

(3) 1,4-Dioxane-d8 (S)

3.246min (-0.000) 5.05ng/uL

response 24063

Ion	Exp%	Act%
96.00	100	100
64.00	69.60	68.65
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017135.D
Acq On : 12 Oct 2018 18:07
Operator : MJ/SJ
Sample : J5362-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

Sohil
10/15/2018 3:57:51 PM

Quant Time: Oct 12 23:39:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

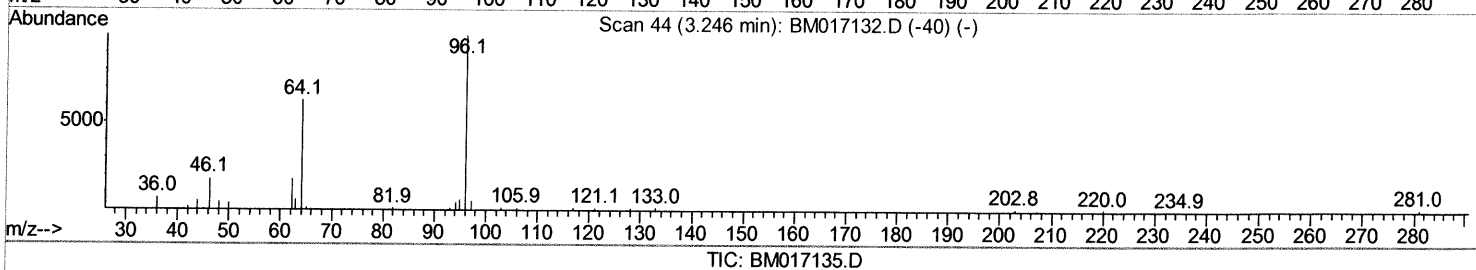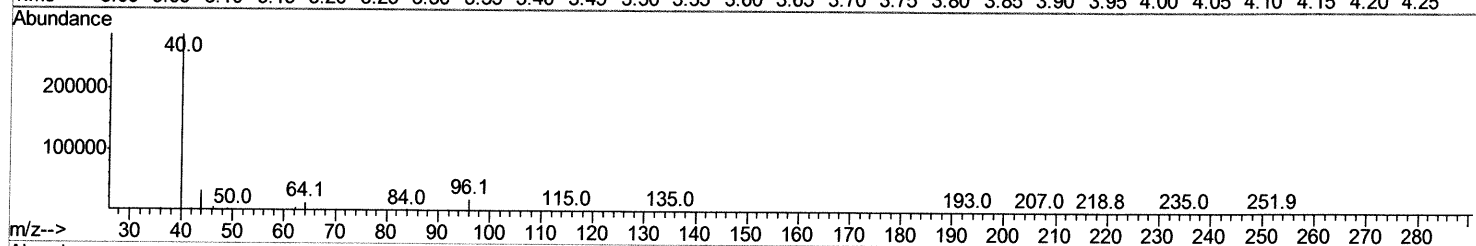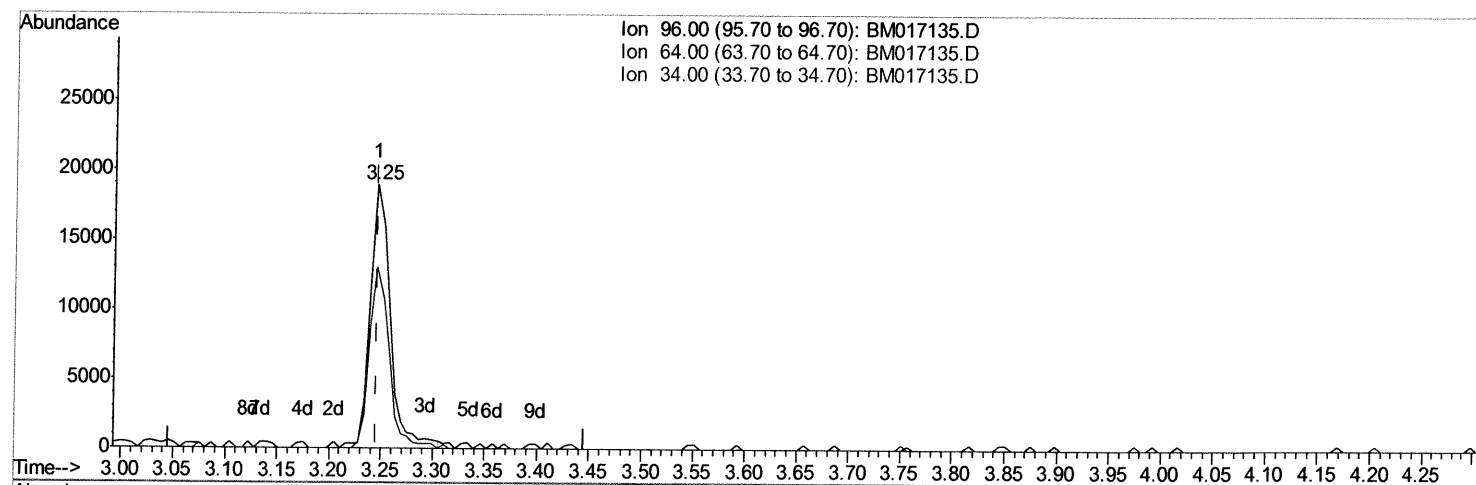

(3) 1,4-Dioxane-d8 (S)

3.246min (-0.000) 5.24ng/uL m> SJ 10/16/18

response 24963

Ion	Exp%	Act%
96.00	100	100
64.00	69.60	68.65
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
 Data File : BM017135.D
 Acq On : 12 Oct 2018 18:07
 Operator : MJ/SJ
 Sample : J5362-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AL5

Manual Integrations
 APPROVED

Sohil
 10/15/2018 3:57:51 PM

Quant Time: Oct 12 23:58:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	237019	20.00	nq/ul	0.00
18) Naphthalene-d8	10.46	136	1114917	20.00	nq/ul	0.00
36) Acenaphthene-d10	14.33	164	636486	20.00	nq/ul	0.00
62) Phenanthrene-d10	17.08	188	1396112	20.00	nq/ul	0.00
78) Chrysene-d12	21.27	240	1056030	20.00	nq/ul	0.00
86) Perylene-d12	23.49	264	1001839	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	24963m)	5.24	nq/uL	0.00
5) Phenol-d5	6.86	99	160850	8.12	nq/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	391097	32.55	nq/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	487834	29.61	nq/ul	0.00
13) 4-Methylphenol-d8	8.39	113	320158	20.62	nq/ul	0.00
19) Nitrobenzene-d5	8.84	128	309457	37.98	nq/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	325757	39.29	nq/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	599621	35.15	nq/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	5341	0.26	nq/ul	0.00
44) Dimethylphthalate-d6	13.74	166	1937066	38.36	nq/ul	0.00
47) Acenaphthylene-d8	14.02	160	2444049	37.86	nq/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	32610	3.42	nq/ul	0.00
58) Fluorene-d10	15.33	176	1736106	38.60	nq/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	198900	24.16	nq/ul	0.00
71) Anthracene-d10	17.18	188	2545013	38.17	nq/ul	0.00
79) Pyrene-d10	19.47	212	2430259	51.01	nq/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	2002369	39.04	ng/ul	0.00

51 10/16/18

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed