


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017137.D
Acq On : 12 Oct 2018 19:19
Operator : MJ/SJ
Sample : J5362-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL2

Manual Integrations
APPROVED

Sohil
10/15/2018 3:57:54 PM

Quant Time: Oct 13 00:08:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

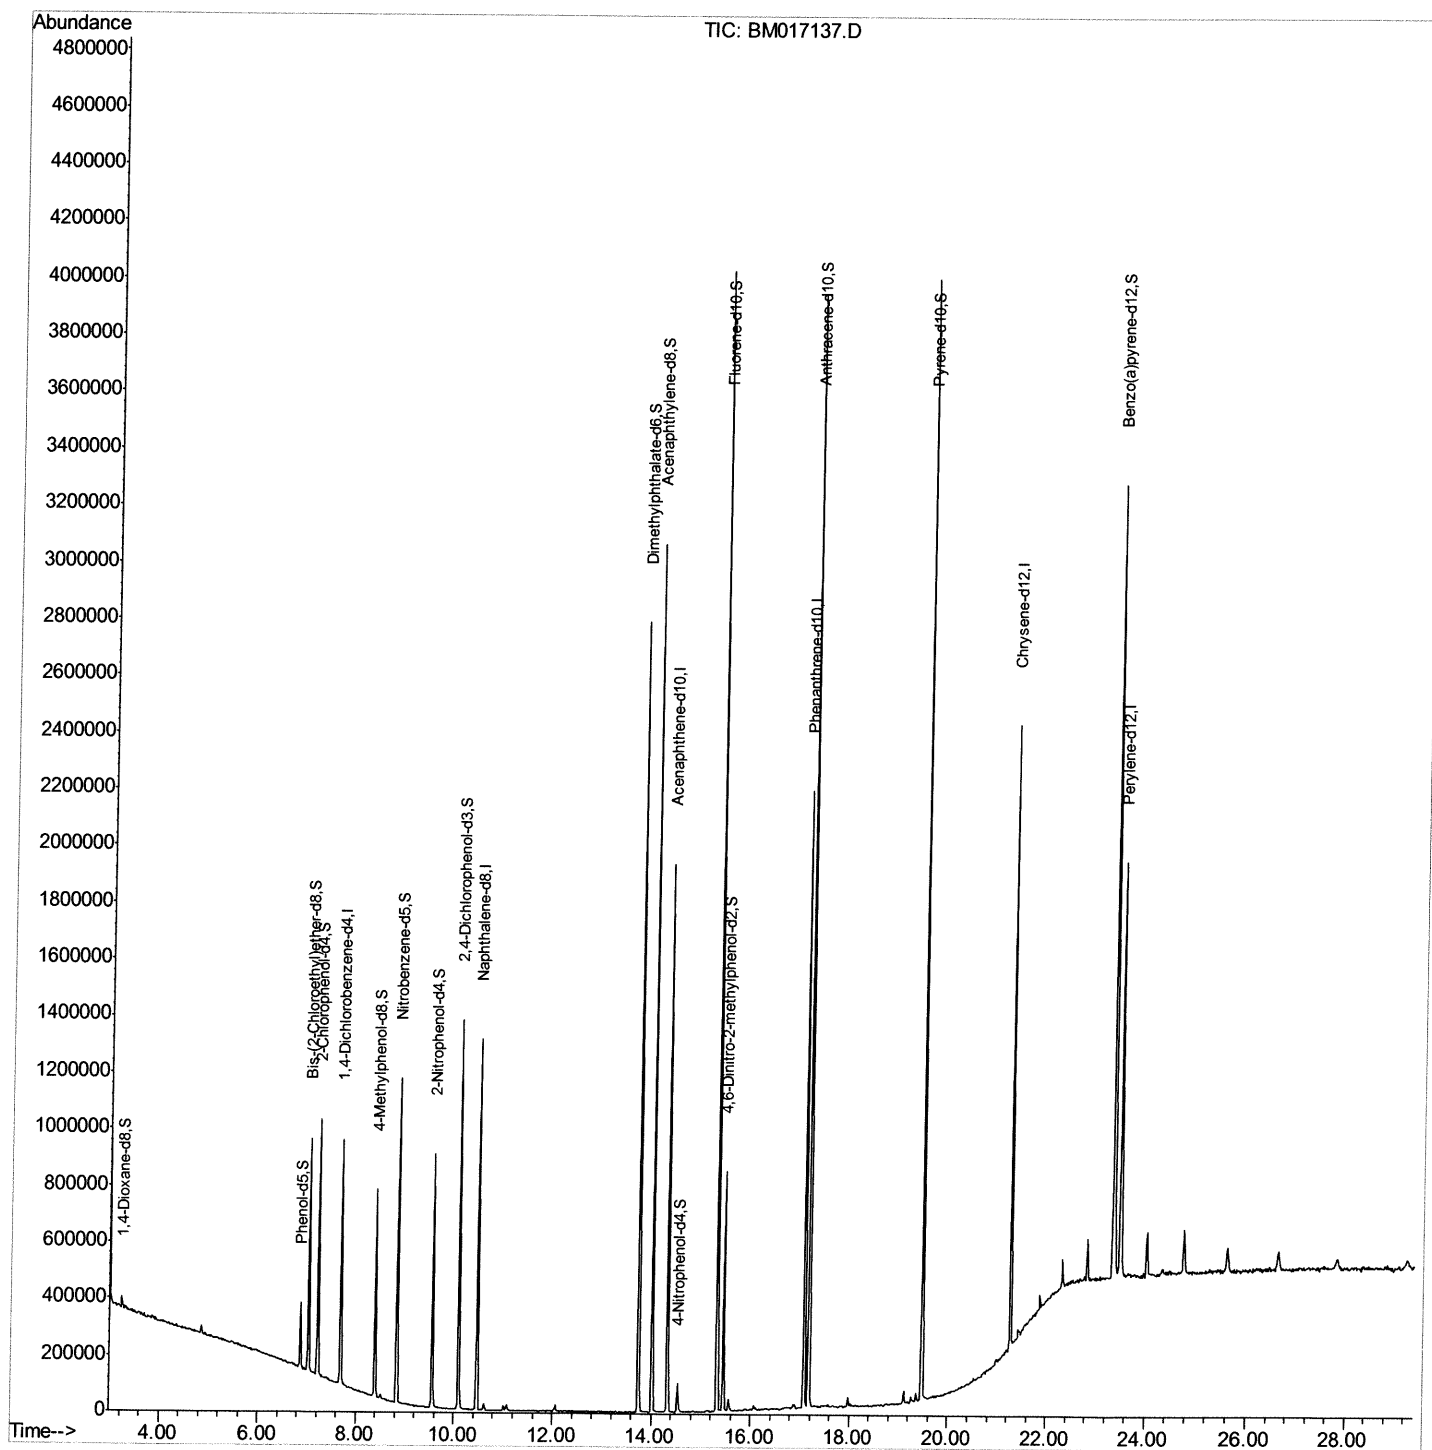

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
 Data File : BM017137.D
 Acq On : 12 Oct 2018 19:19
 Operator : MJ/SJ
 Sample : J5362-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AL2

Manual Integrations
 APPROVED

Sohil
 10/15/2018 3:57:54 PM

Quant Time: Oct 12 23:39:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

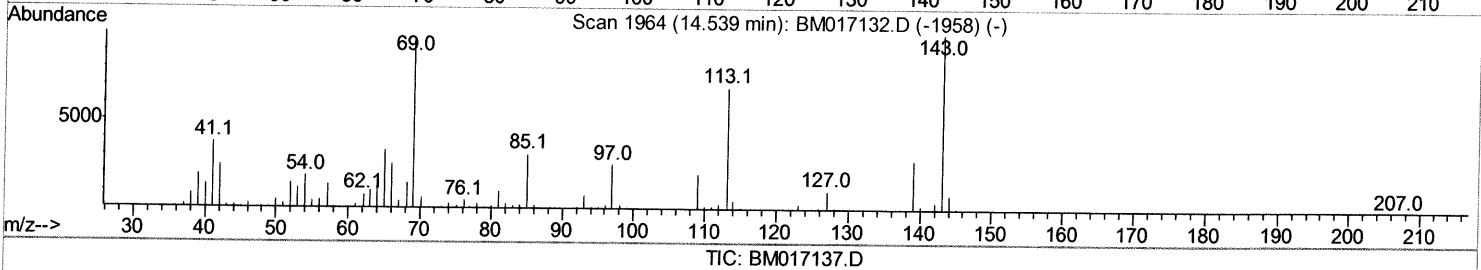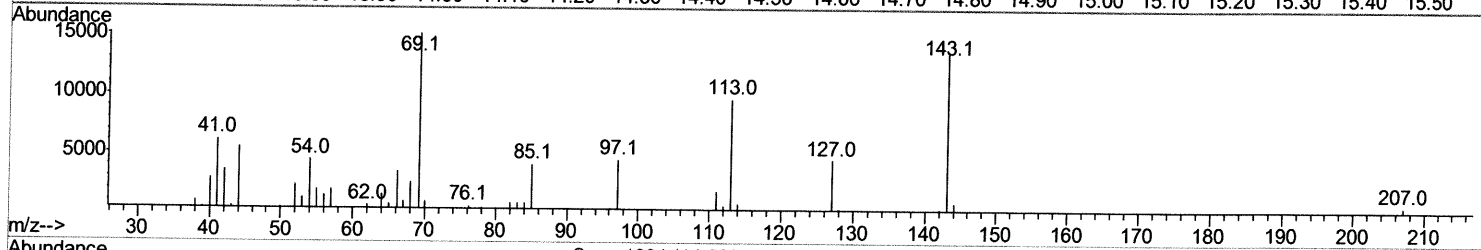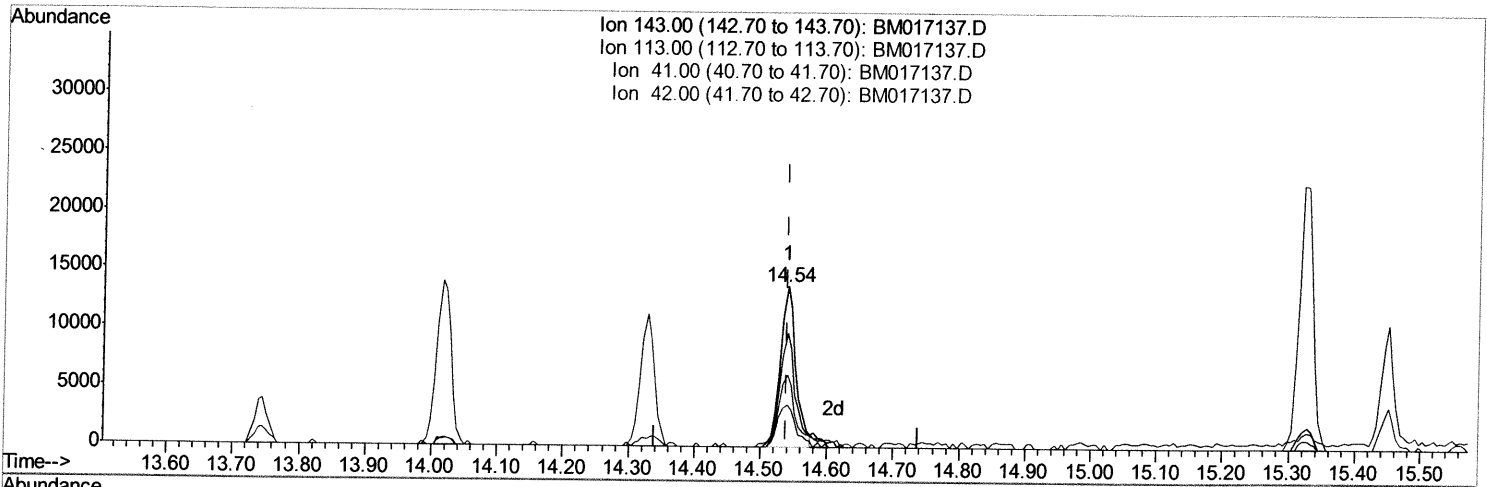

(52) 4-Nitrophenol-d4 (S)
 14.539min (-0.000) 2.39ng/ul
 response 22191

Ion	Exp%	Act%
143.00	100	100
113.00	66.60	70.97
41.00	36.20	44.92#
42.00	24.80	26.46

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
Data File : BM017137.D
Acq On : 12 Oct 2018 19:19
Operator : MJ/SJ
Sample : J5362-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C0AL2

Manual Integrations
APPROVED

Sohil
10/15/2018 3:57:54 PM

Quant Time: Oct 12 23:39:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

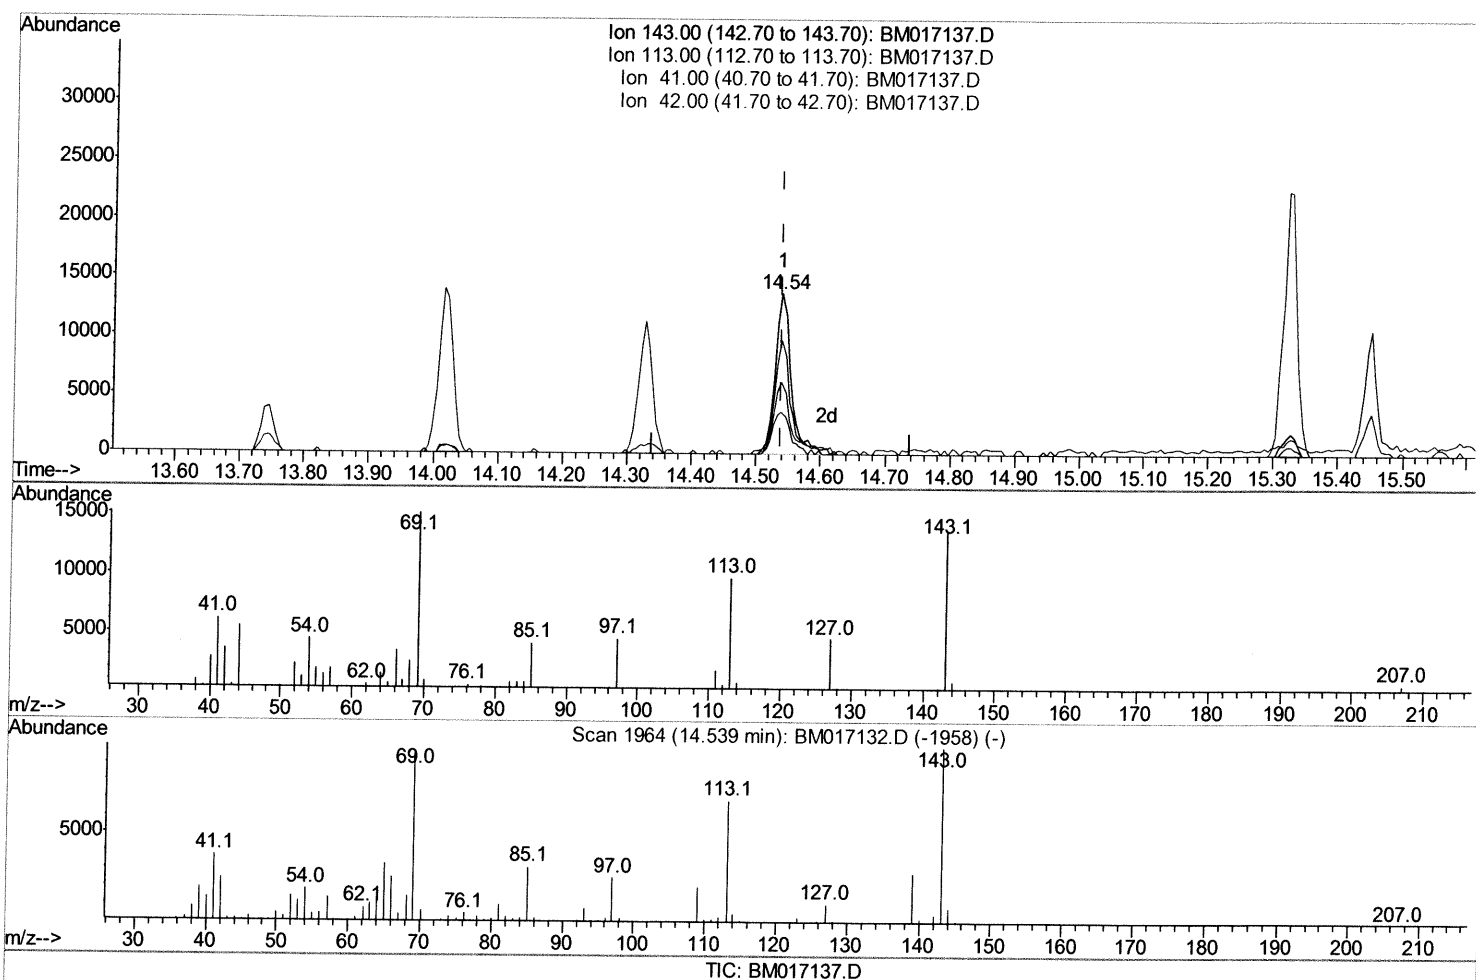

(52) 4-Nitrophenol-d4 (S)

14.539min (-0.000) 2.55ng/ul m> SJ 10/16/18

response 23596

Ion	Exp%	Act%
143.00	100	100
113.00	66.60	70.97
41.00	36.20	44.92#
42.00	24.80	26.46

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM101218\
 Data File : BM017137.D
 Acq On : 12 Oct 2018 19:19
 Operator : MJ/SJ
 Sample : J5362-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AL2

Manual Integrations
 APPROVED

Sohil
 10/15/2018 3:57:54 PM

Quant Time: Oct 13 00:08:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	231231	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1098333	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	618134	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1298326	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1023683	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1052313	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	20705	4.45	ng/uL	0.00
5) Phenol-d5	6.86	99	133491	6.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	356646	30.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	427025	26.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	267269	17.65	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	280244	34.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	293318	35.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	525510	31.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	13468	0.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.74	166	1771514	36.12	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	2242452	35.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	23596m	2.55	ng/ul	0.00
58) Fluorene-d10	15.33	176	1567729	35.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	158727	20.73	ng/ul	0.00
71) Anthracene-d10	17.18	188	2189583	35.31	ng/ul	0.00
79) Pyrene-d10	19.47	212	2027253	43.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	1995292	37.04	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

53 10/16/18