

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101218\
 Data File : BM017136.D
 Acq On : 12 Oct 2018 18:43
 Operator : MJ/SJ
 Sample : J5422-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0920

Quant Time: Oct 12 23:39:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	210687	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1002525	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	590878	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1412386	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1403863	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1176540	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	22879	5.40	ng/uL	0.00
5) Phenol-d5	6.86	99	130500	7.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	346866	32.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	415227	28.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	264354	19.16	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	272037	37.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	284527	38.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	524196	34.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	42939	2.33	ng/ul	0.00
44) Dimethylphthalate-d6	13.74	166	1867131	39.83	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	2366938	39.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	33948	3.83	ng/ul	0.00
58) Fluorene-d10	15.33	176	1705096	40.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	237138	28.47	ng/ul	0.00
71) Anthracene-d10	17.18	188	2768812	41.04	ng/ul	0.00
79) Pyrene-d10	19.48	212	3102882	49.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	2558212	42.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.79	163	125649	2.707	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101218\
Data File : BM017136.D
Acq On : 12 Oct 2018 18:43
Operator : MJ/SJ
Sample : J5422-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0920

Quant Time: Oct 12 23:39:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

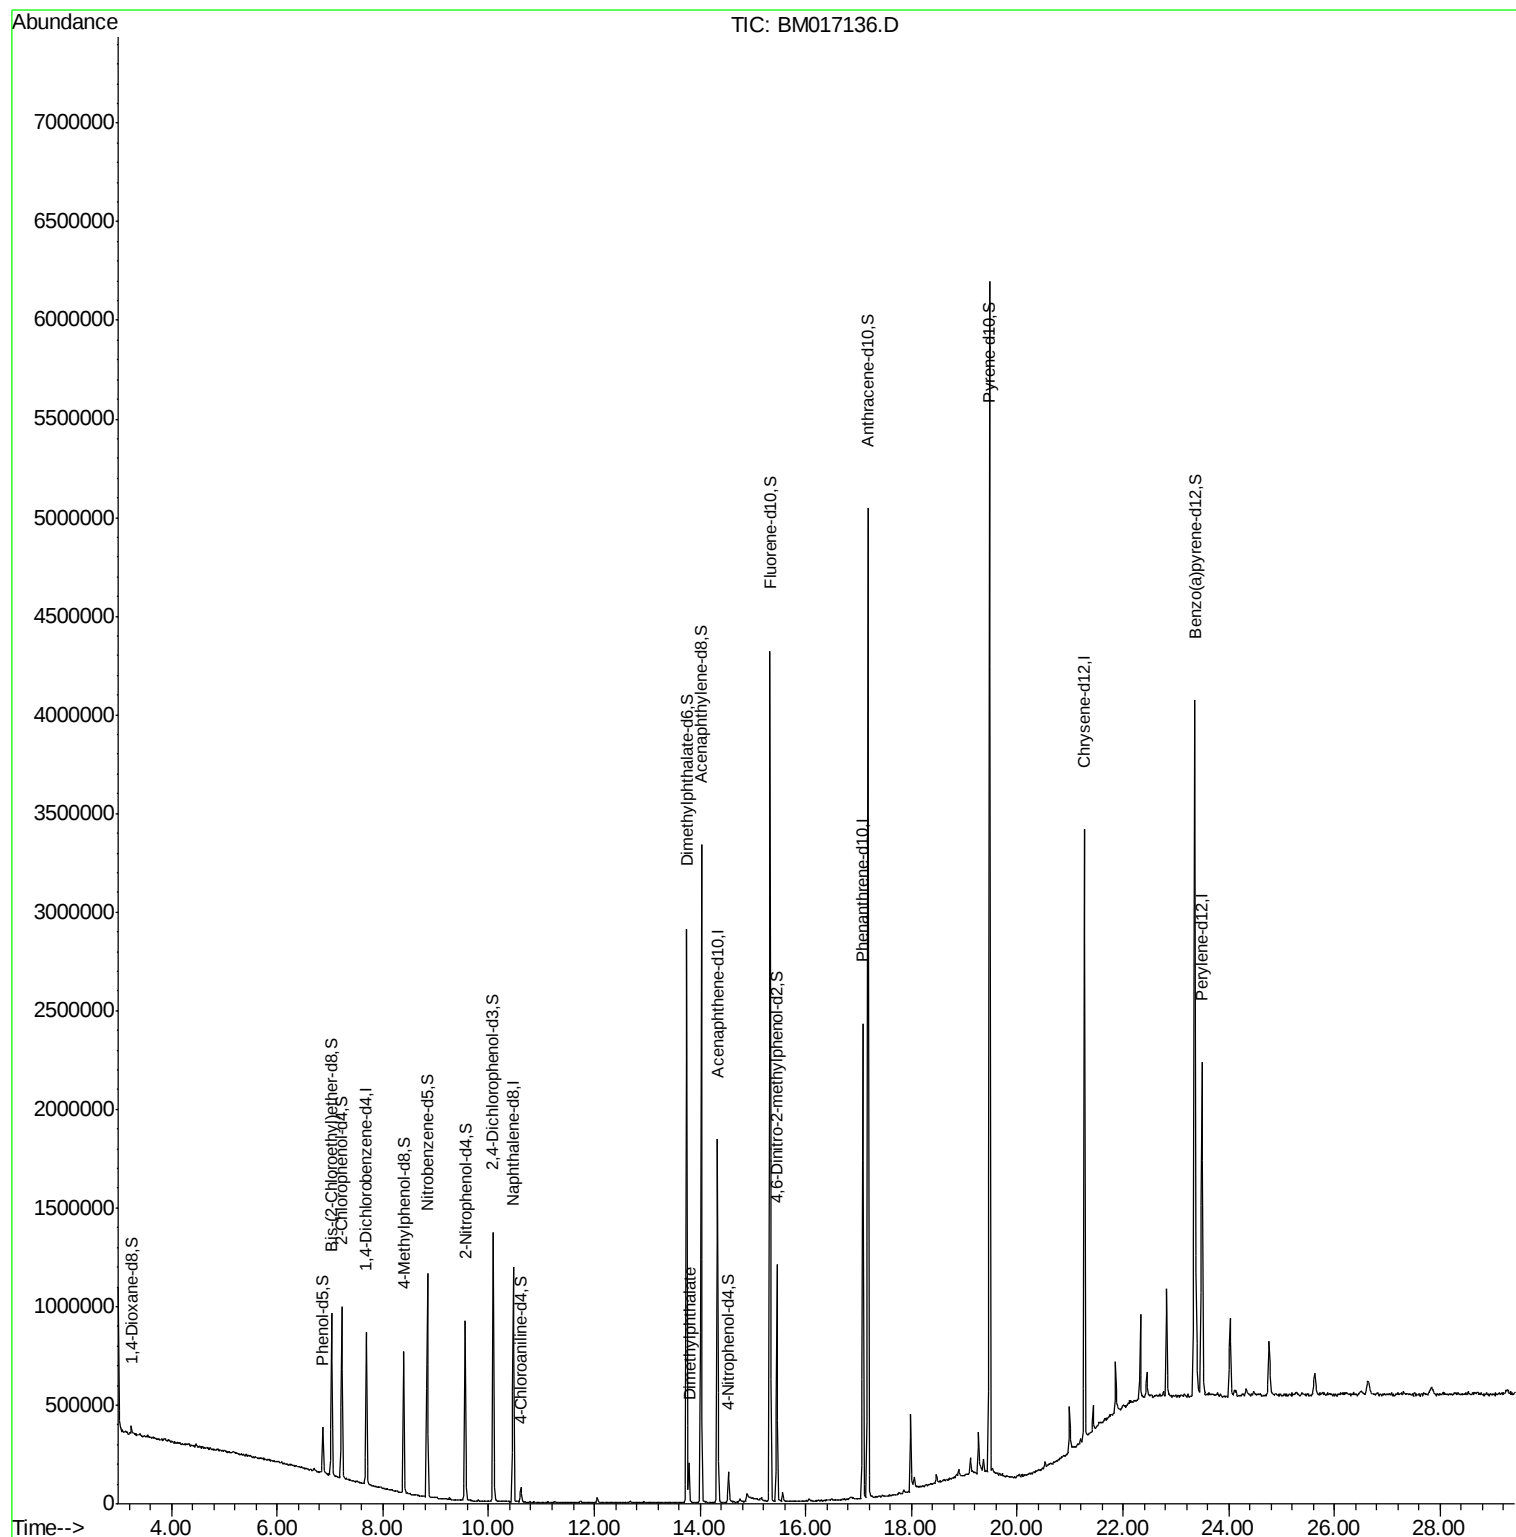

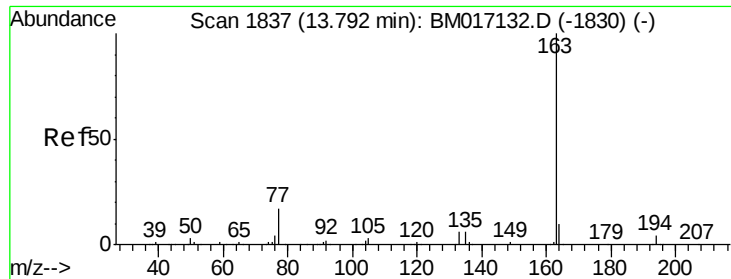

#45

Dimethylphthalate

Concen: 2.707 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BM017136.D


Acq: 12 Oct 2018 18:43

Instrument :

BNA_M

ClientSampleId :

C0920

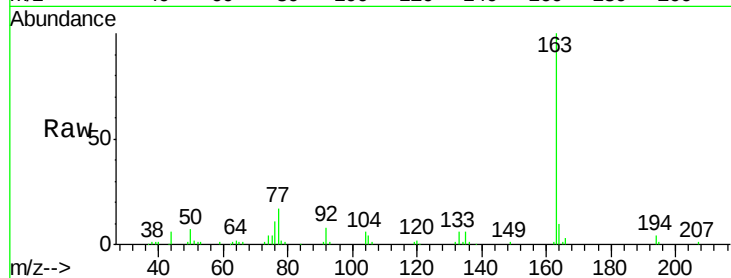


Tgt Ion:163 Resp: 125649

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9

164 10.3 8.0 12.0

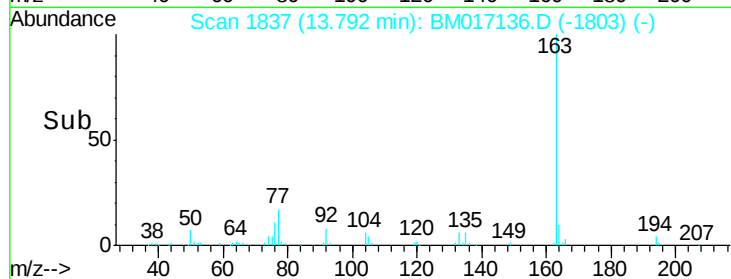

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

