
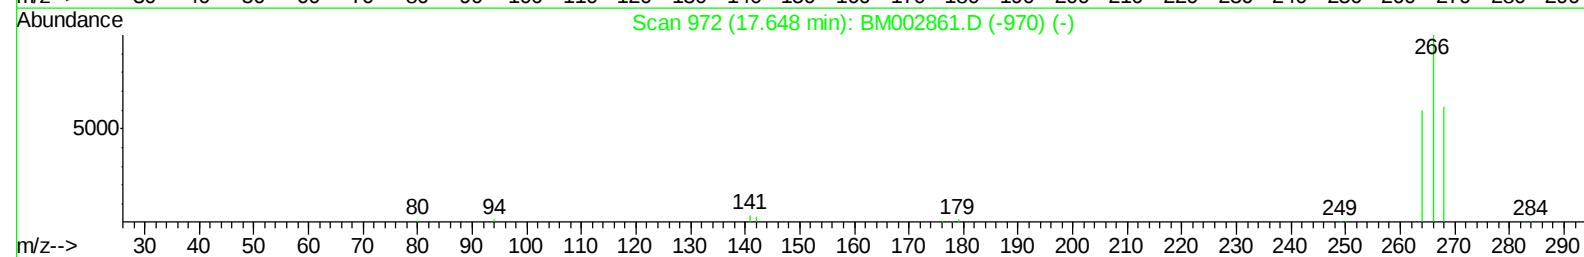
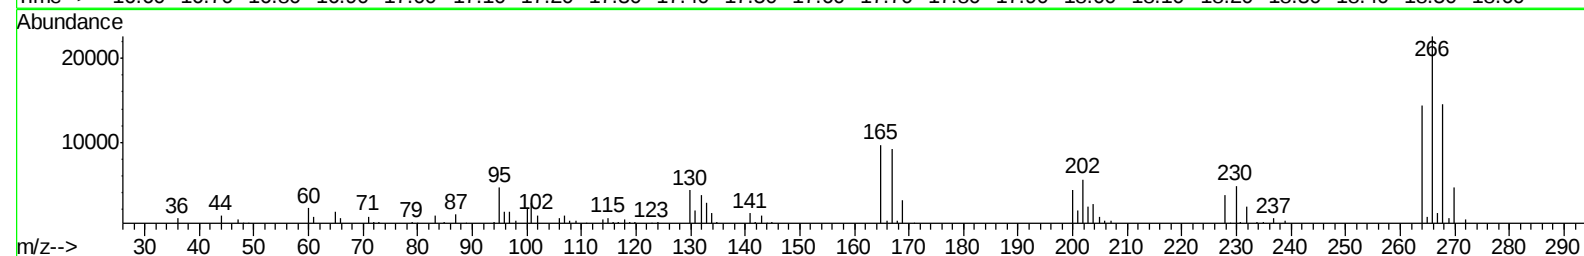


Data Path : V:\HPCHEM1\BNA M\Data\BM101315\
 Data File : BM002890.D
 Acq On : 13 Oct 2015 17:21
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 20:04:46 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM100715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 08 14:09:33 2015
 Response via : Initial Calibration

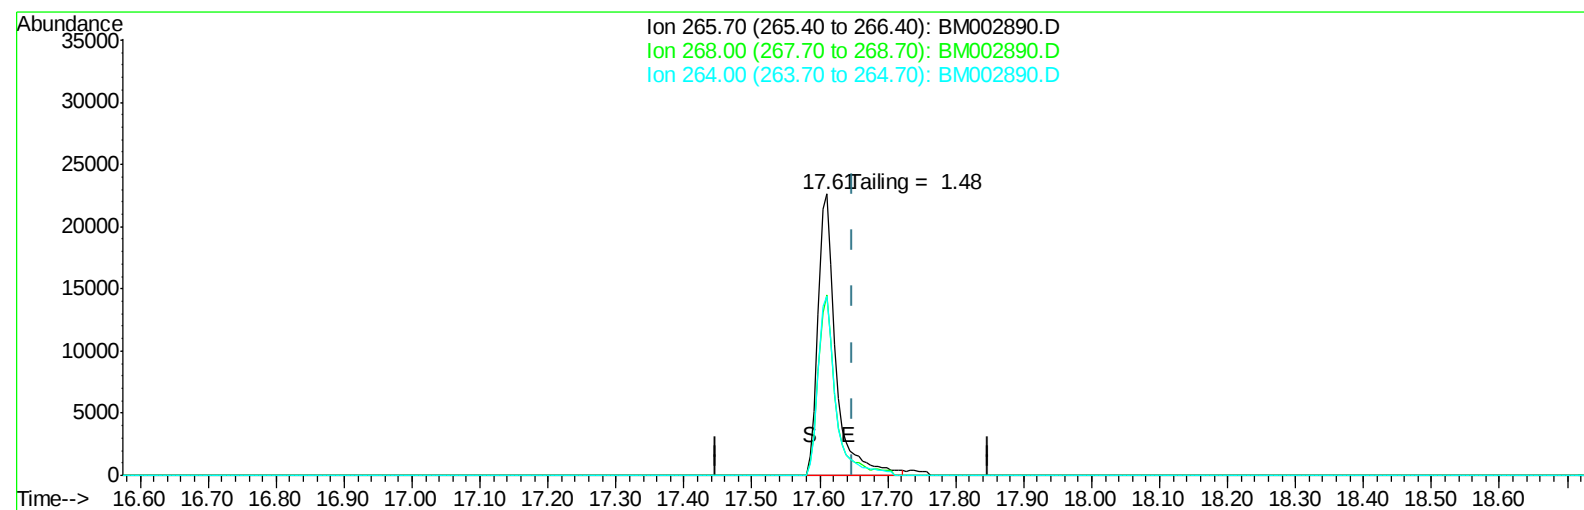

TIC: BM002890.D

(22) Pentachlorophenol




17.610min (-0.038) 0.00ng

response 41124

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	63.99
264.00	63.90	63.52
0.00	0.00	0.00

Data Path : V:\HPCHEM1\BNA M\Data\BM101315\
Data File : BM002890.D
Acq On : 13 Oct 2015 17:21
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 20:04:46 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM100715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 14:09:33 2015
Response via : Initial Calibration

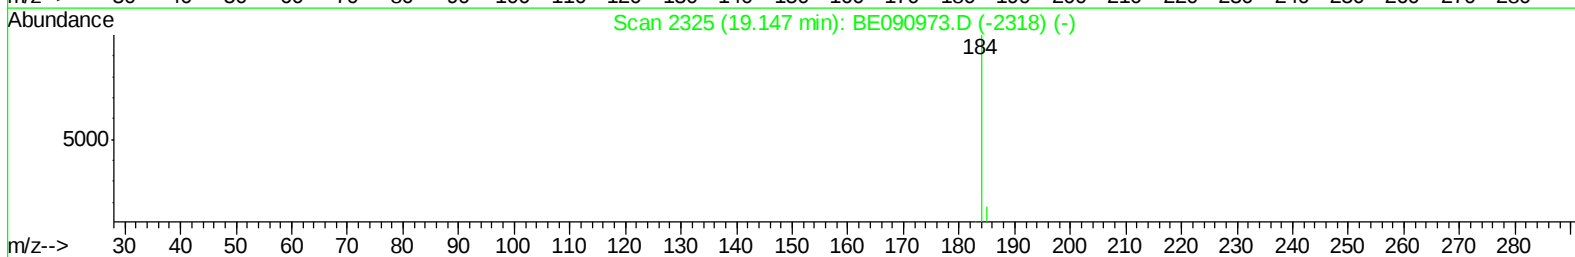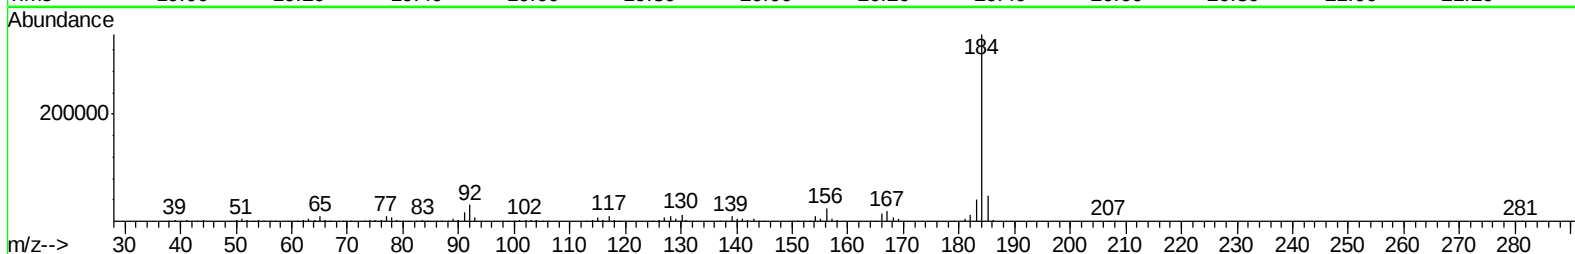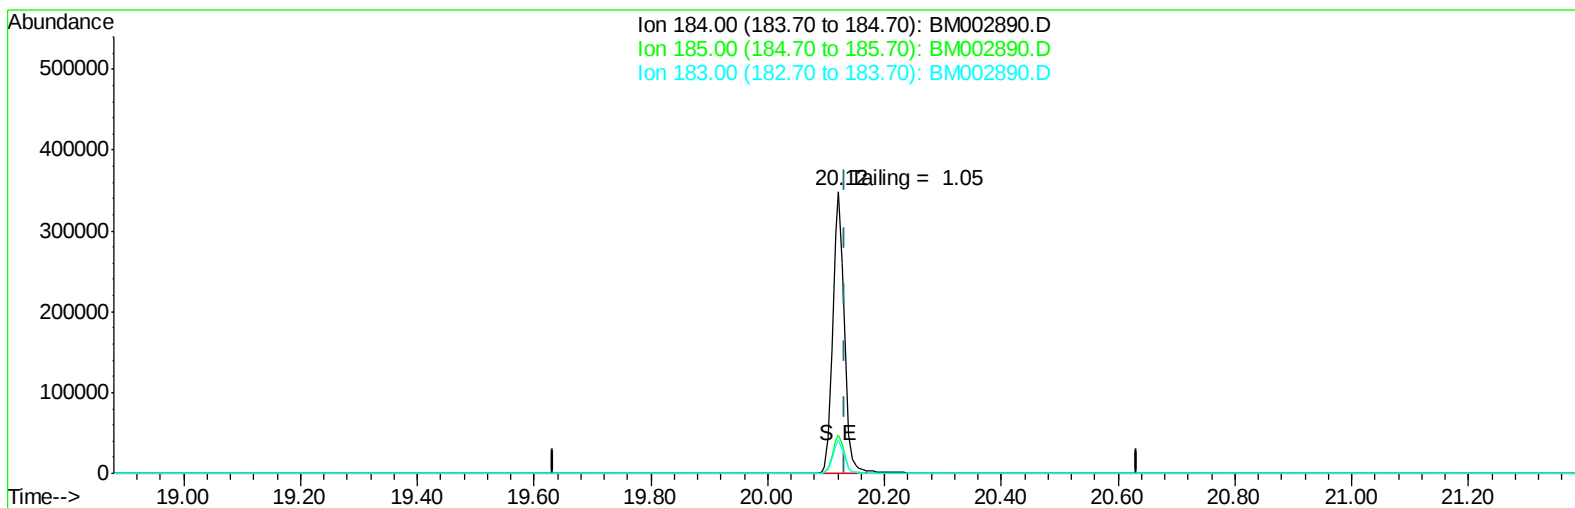

TIC: BM002890.D

(27) Benzidine

20.121min (-0.012) 0.00ng

response 478279

Ion	Exp%	Act%
184.00	100	100
185.00	27.90	13.72#
183.00	20.50	11.61#
0.00	0.00	0.00