


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101315\
Data File : BM002890.D
Acq On : 13 Oct 2015 17:21
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-ACID-BM0101315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 14 17:36:42 2015

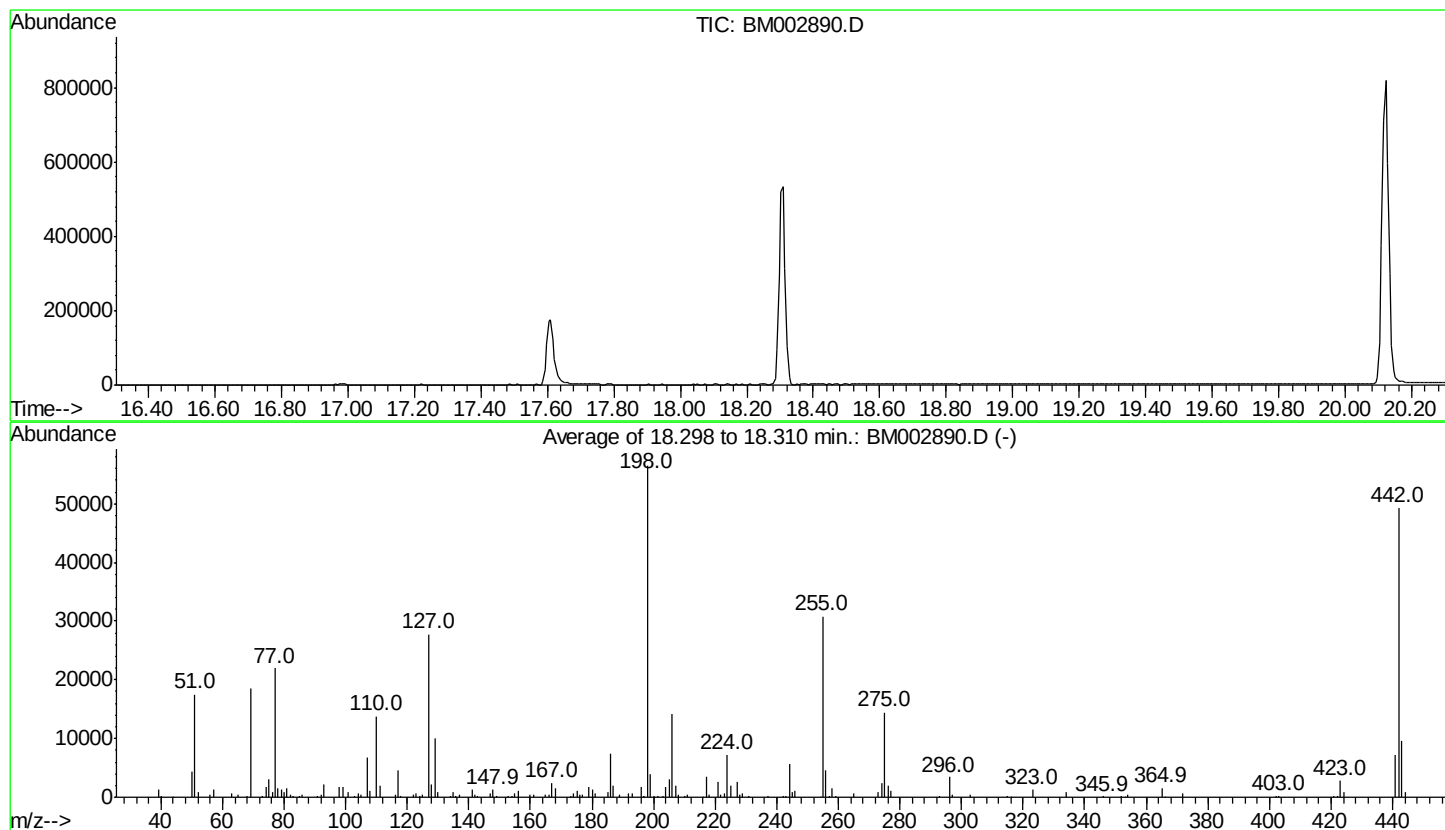

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	17478	PASS
68	69	0.00	2	1.5	287	PASS
69	198	0.00	100	32.8	18536	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	27733	PASS
197	198	0.00	2	0.2	130	PASS
198	198	100	100	100.0	56480	PASS
199	198	5	9	6.9	3887	PASS
275	198	10	60	25.5	14400	PASS
365	198	1	100	2.9	1628	PASS
441	442	0.01	24	14.8	7275	PASS
442	198	50	100	87.3	49314	PASS
443	442	15	24	19.6	9671	PASS