

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101317\
 Data File : BM012162.D
 Acq On : 14 Oct 2017 08:04
 Operator : SJ/JU
 Sample : I5649-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-42(7-9)-100217

Manual Integrations
 APPROVED

Sohil
 6/22/2018 5:57:57 PM

Quant Time: Jun 22 17:51:37 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 15 05:27:50 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	190192	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	746617	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	411606	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	849992	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	926975	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	1007292	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	16479	4.12	ng/uL	0.00
5) Phenol-d5	6.99	99	313591	20.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	255489	27.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	343055	26.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	308494	23.22	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	174989	30.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	196717	29.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	324859	25.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	276859	23.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	1086837	29.88	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	1383467	31.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	47603	8.70	ng/ul	0.01
57) Fluorene-d10	15.47	176	948521	31.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	71684	12.29	ng/ul	0.00
70) Anthracene-d10	17.32	188	1398791	33.28	ng/ul	0.00
76) Pyrene-d10	19.62	212	1553140	33.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1652859	34.04	ng/ul	0.00

Target Compounds

					Qvalue
16) 4-Methylphenol	8.59	108	14937	1.130 ng/ul#	77
28) Naphthalene	10.67	128	42177	1.092 ng/ul	97
44) Dimethylphthalate	13.93	163	223271m	6.126 ng/ul	
49) Acenaphthene	14.53	153	101612	3.489 ng/ul	98
53) Dibenzofuran	14.87	168	51197	1.221 ng/ul	97
58) Fluorene	15.52	166	124573	3.576 ng/ul	94
69) Phenanthrene	17.26	178	1939688	40.114 ng/ul	99
71) Anthracene	17.36	178	439382	8.777 ng/ul	98
72) Carbazole	17.63	167	60865	1.437 ng/ul#	90
74) Fluoranthene	19.28	202	3486414	59.746 ng/ul#	92
77) Pyrene	19.64	202	3329776	54.391 ng/ul#	92
80) Benzo(a)anthracene	21.39	228	2294878	38.047 ng/ul	98
82) Chrysene	21.44	228	2088351	36.877 ng/ul	97
85) Benzo(b)fluoranthene	23.02	252	2708711	41.207 ng/ul#	97
86) Benzo(k)fluoranthene	23.06	252	729951m	11.523 ng/ul	
88) Benzo(a)pyrene	23.62	252	2028173	32.736 ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	26.09	276	1242791	18.889 ng/ul#	96
90) Dibenzo(a,h)anthracene	26.09	278	352778	6.378 ng/ul#	86
91) Benzo(g,h,i)perylene	26.82	276	1034336	19.195 ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101317\
Data File : BM012162.D
Acq On : 14 Oct 2017 08:04
Operator : SJ/JU
Sample : I5649-12
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Manual Integrations
APPROVED

Sohil
6/22/2018 5:57:57 PM

Quant Time: Jun 22 17:51:37 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 15 05:27:50 2017
Response via : Initial Calibration

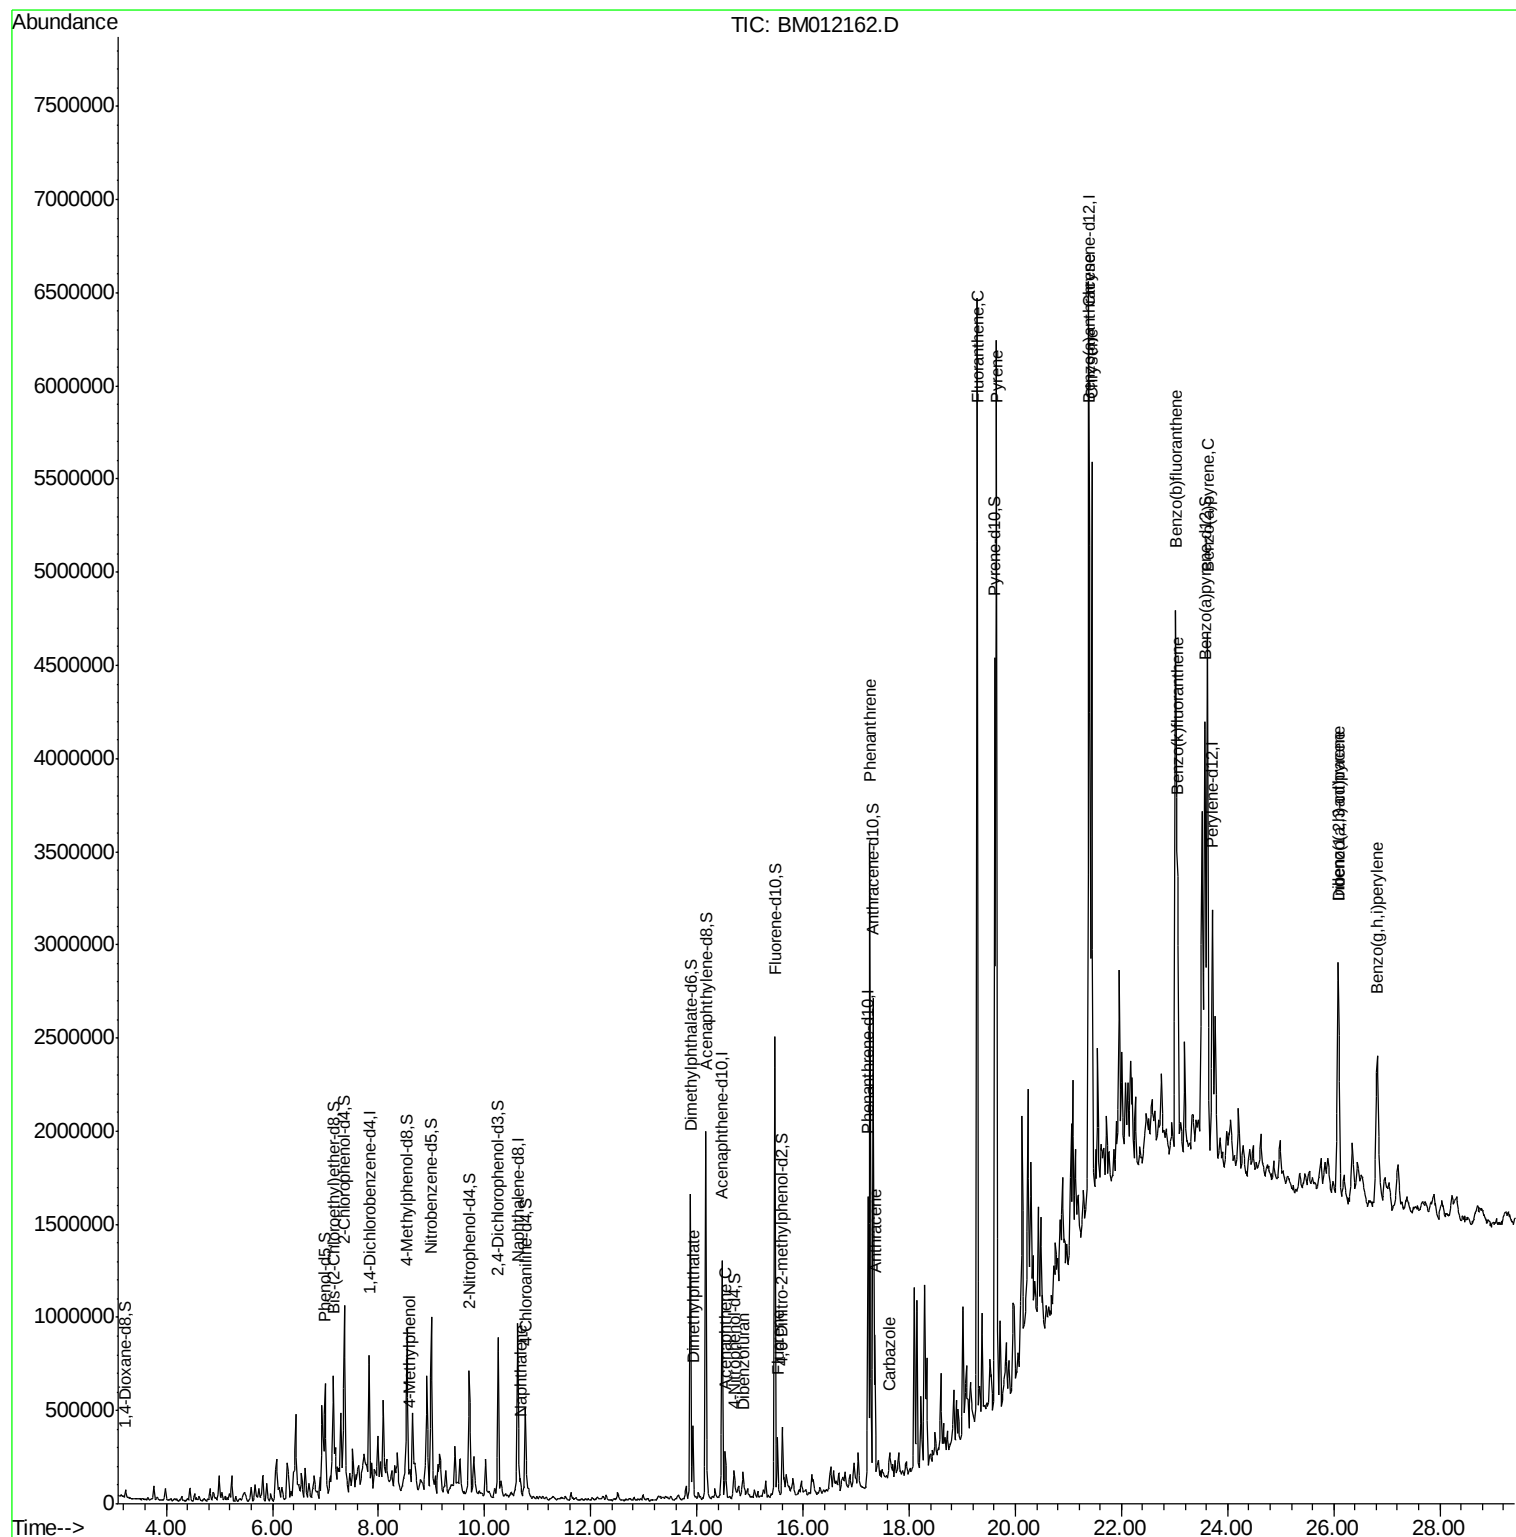

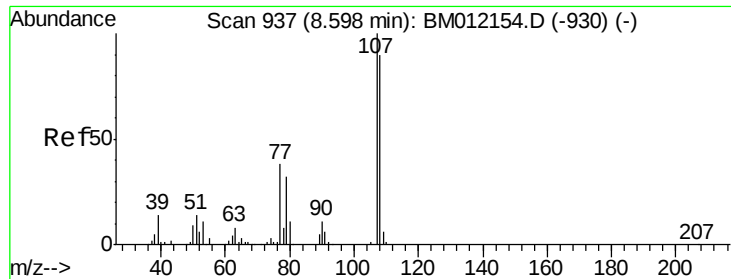

#16

4-Methylphenol

Concen: 1.130 ng/ul

RT: 8.59 min Scan# 936

Delta R.T. -0.01 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Instrument :

BNA_M

ClientSampleId :

B-42(7-9)-100217

Tgt Ion:108 Resp: 14937

Ion Ratio Lower Upper

108 100





107 129.6 84.9 127.3#

Manual Integrations

APPROVED

Sohil

6/22/2018 5:57:57 PM

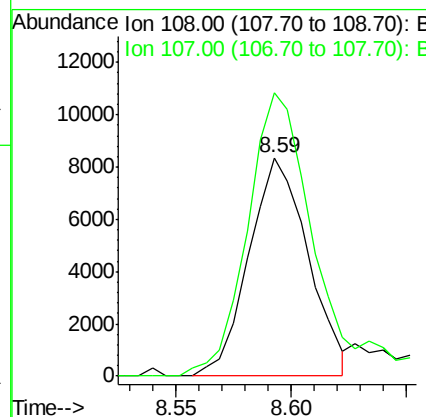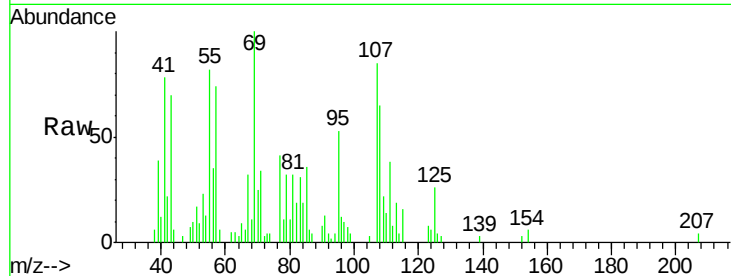

#28

Naphthalene

Concen: 1.092 ng/ul

RT: 10.67 min Scan# 1290

Delta R.T. 0.00 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04




Tgt Ion:128 Resp: 42177


Ion Ratio Lower Upper

128 100

129 12.9 8.8 13.2

127 14.1 10.6 16.0

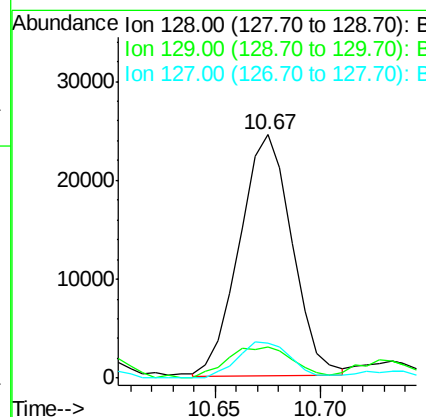

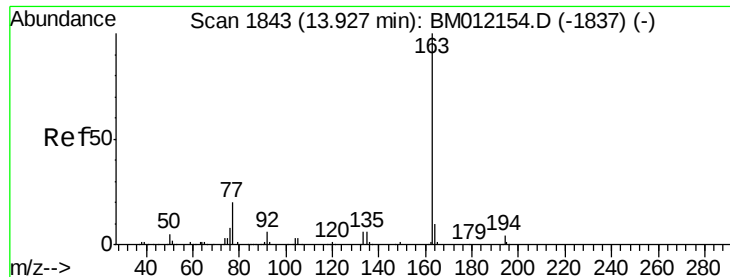





#44
Dimethylphthalate
Concen: 6.126 ng/ul m
RT: 13.93 min Scan# 1843
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	223271		
194	4.4		3.5	5.3
164	10.0		8.2	12.4




Manual Integrations
APPROVED


Sohil
6/22/2018 5:57:57 PM

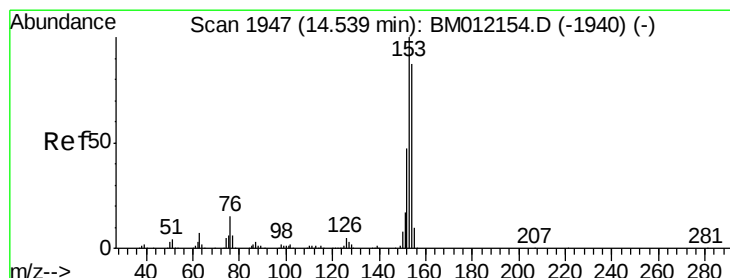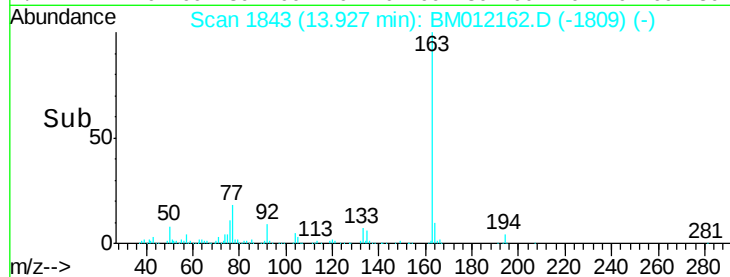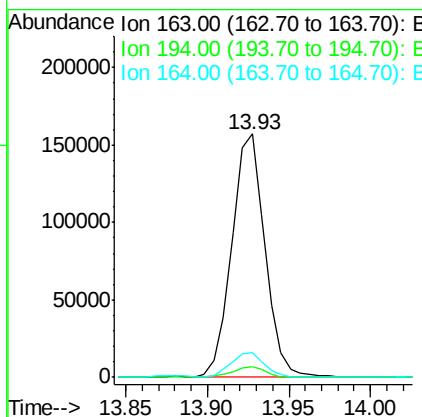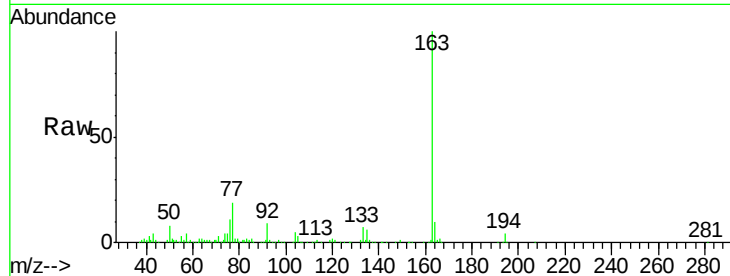

#49
Acenaphthene
Concen: 3.489 ng/ul
RT: 14.53 min Scan# 1946
Delta R.T. -0.01 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	101612		
152	48.7		37.6	56.4
154	90.1		70.4	105.6

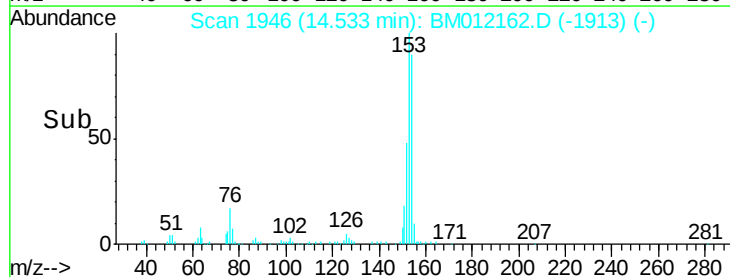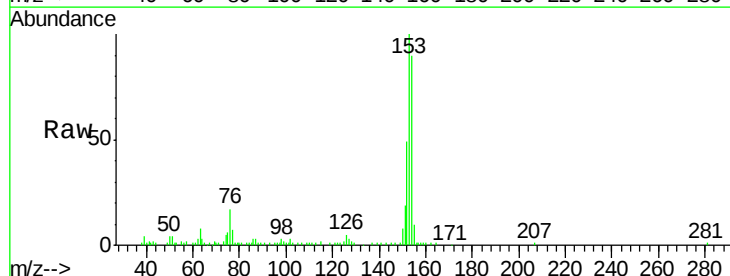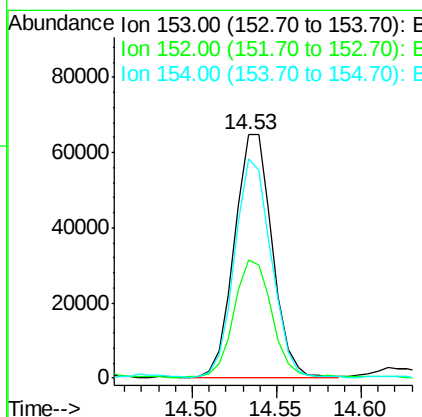

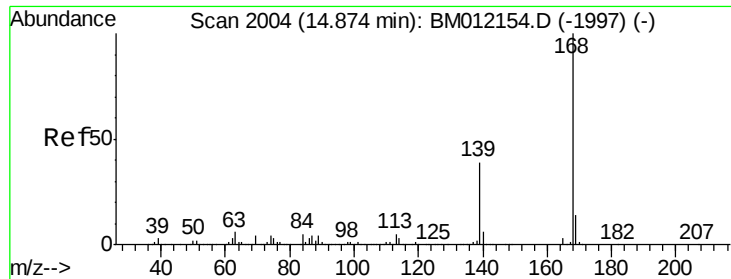





#53
Dibenzenofuran
Concen: 1.221 ng/ul
RT: 14.87 min Scan# 2004
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Tgt Ion	Ratio	Lower	Upper
168	100		
139	36.9	30.8	46.2




Manual Integrations
APPROVED


Sohil
6/22/2018 5:57:57 PM

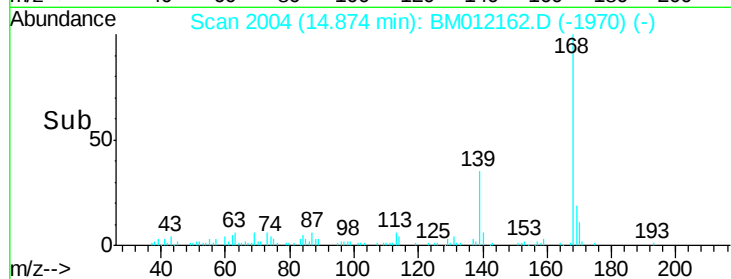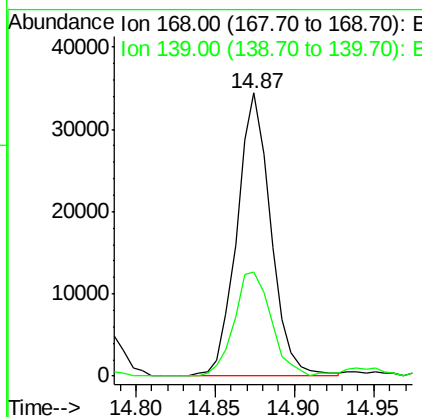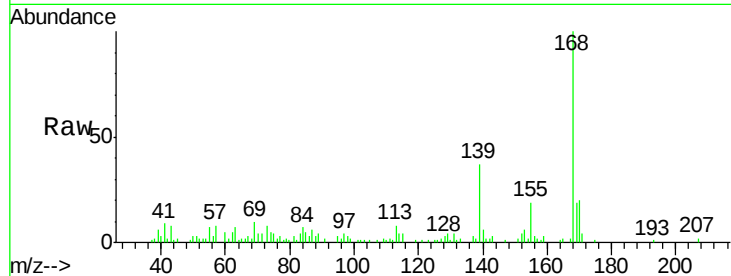

#58
Fluorene
Concen: 3.576 ng/ul
RT: 15.52 min Scan# 2114
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Lower	Upper
166	100		
165	103.8	77.9	116.9
167	15.1	10.6	16.0

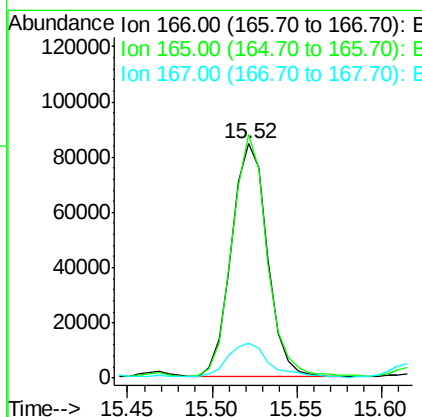







#69
Phenanthrene
Concen: 40.114 ng/ul
RT: 17.26 min Scan# 2410
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.6	19.0
176	19.1	14.9	22.3




Manual Integrations
APPROVED


Sohil
6/22/2018 5:57:57 PM

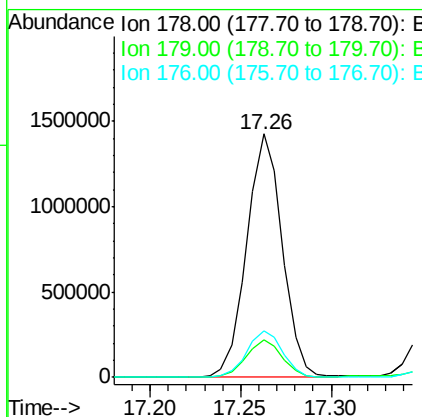

#71
Anthracene
Concen: 8.777 ng/ul
RT: 17.36 min Scan# 2426
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.8	11.7	17.5
176	18.5	14.6	21.8

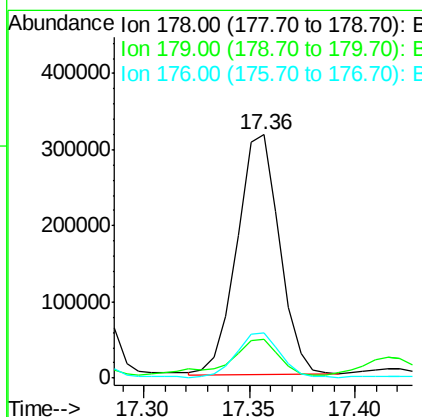



#72

Carbazole

Concen: 1.437 ng/ul

RT: 17.63 min Scan# 2472

Delta R.T. 0.00 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Instrument :

BNA_M





ClientSampleId :

B-42(7-9)-100217

Tgt Ion	Ratio	Lower	Upper
167	100		
166	27.0	17.1	25.7#
139	15.0	10.0	15.0

Manual Integrations
APPROVED

Sohil
6/22/2018 5:57:57 PM

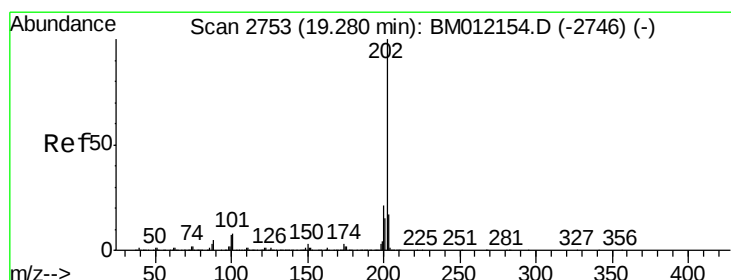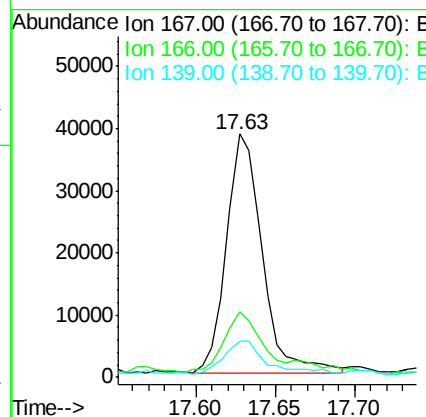

#74

Fluoranthene

Concen: 59.746 ng/ul




RT: 19.28 min Scan# 2753


Delta R.T. 0.00 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.7	4.6	7.0#
100	6.7	3.4	5.2#

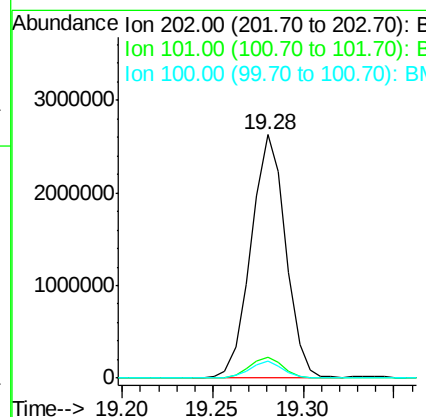

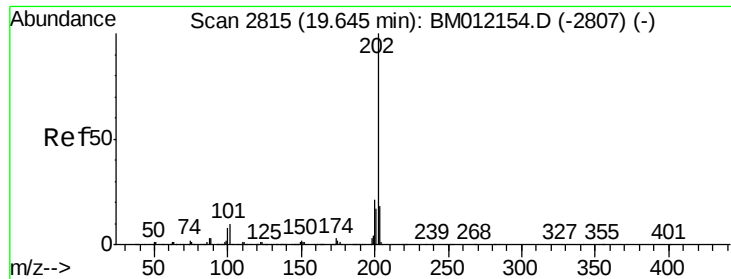

#77

Pyrene

Concen: 54.391 ng/ul

RT: 19.64 min Scan# 2815

Delta R.T. 0.00 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Instrument :

BNA_M





ClientSampleId :

B-42(7-9)-100217

Tgt Ion:	202	Resp:	3329776
Ion Ratio	Lower	Upper	
202	100		
101	10.0	5.1	7.7#
100	8.1	4.9	7.3#

Manual Integrations
APPROVED

Sohil
6/22/2018 5:57:57 PM

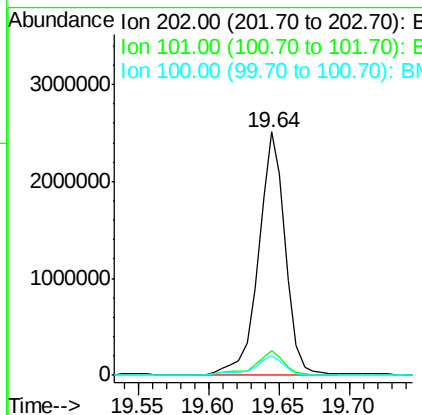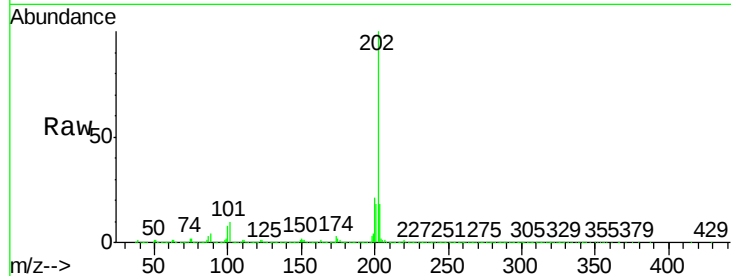

#80

Benzo(a)anthracene

Concen: 38.047 ng/ul




RT: 21.39 min Scan# 3111


Delta R.T. 0.00 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Tgt Ion:	228	Resp:	2294878
Ion Ratio	Lower	Upper	
228	100		
229	20.7	15.4	23.0
226	27.1	21.4	32.0

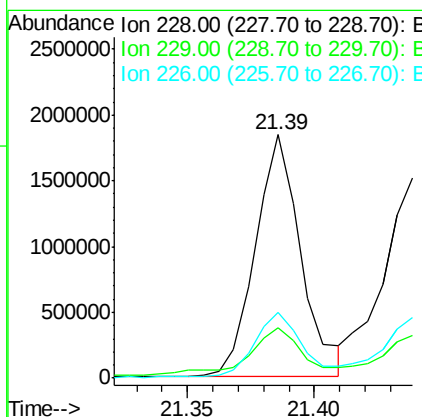

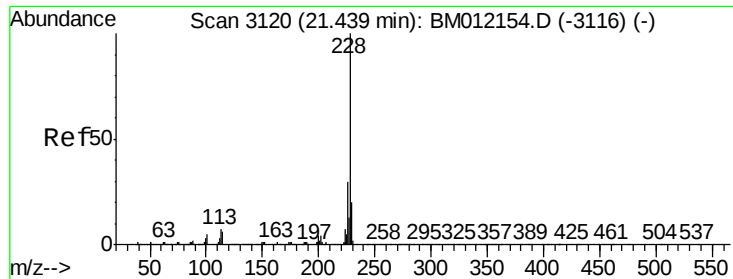





#82
Chrysene
Concen: 36.877 ng/u1
RT: 21.44 min Scan# 3120
Delta R.T. 0.00 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Tgt Ion:	228	Resp:	2088351
Ion Ratio	Lower	Upper	
228	100		
226	30.6	23.4	35.2
229	21.6	15.5	23.3




Manual Integrations
APPROVED


Sohil
6/22/2018 5:57:57 PM

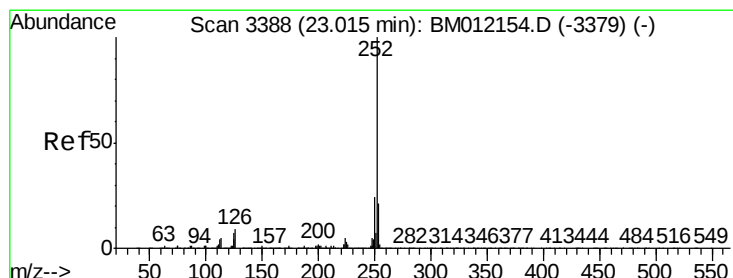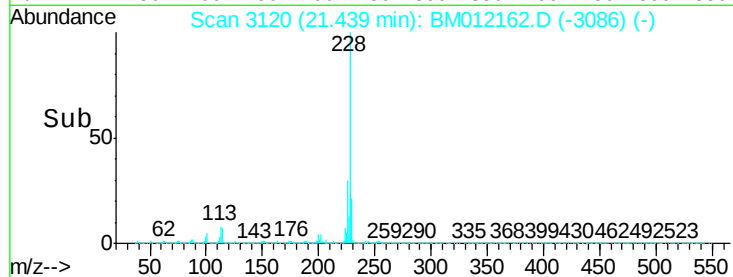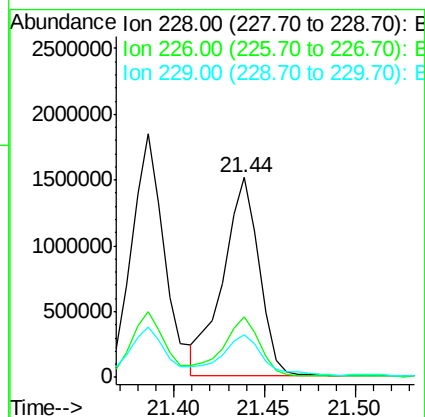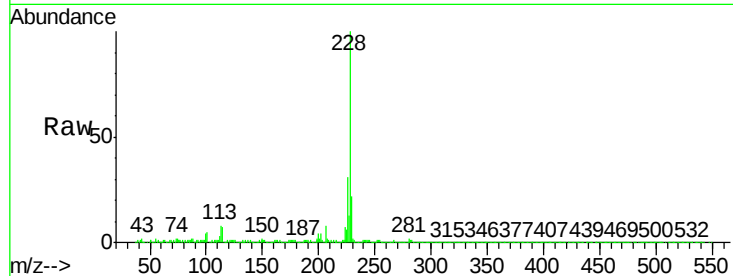

#85
Benzo(b)fluoranthene
Concen: 41.207 ng/u1
RT: 23.02 min Scan# 3389
Delta R.T. 0.01 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Tgt Ion:	252	Resp:	2708711
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.9	26.9
125	8.4	3.6	5.4#

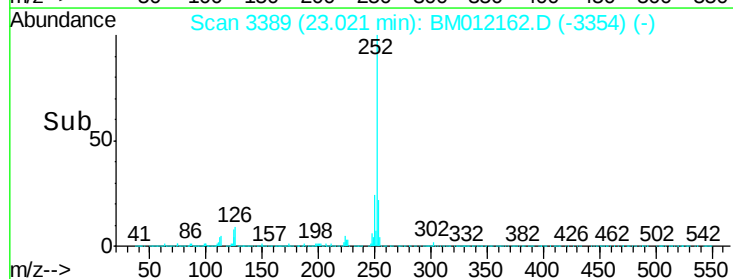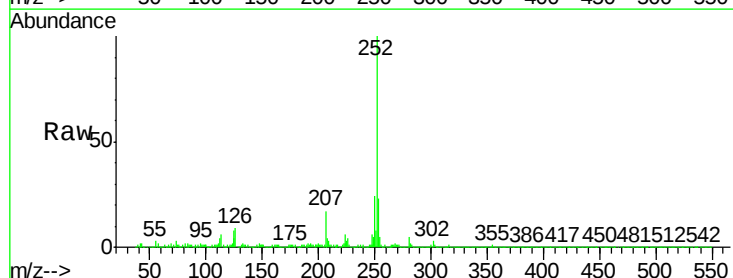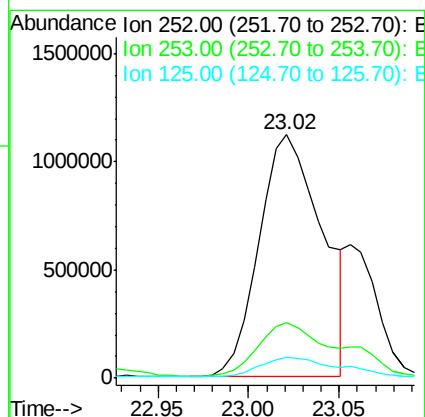

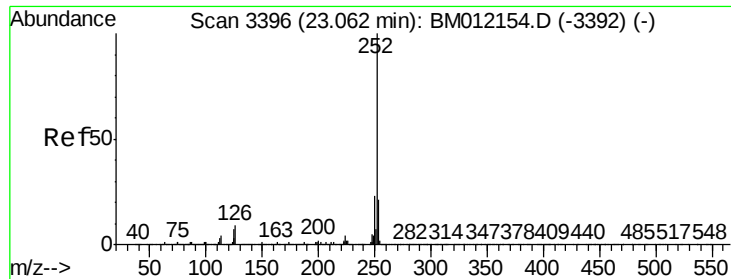





#86
Benzo(k)fluoranthene
Concen: 11.523 ng/ul m
RT: 23.06 min Scan# 3395
Delta R.T. -0.01 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Instrument :
BNA_M
ClientSampleId :
B-42(7-9)-100217

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.1	25.7
125	8.6	3.4	5.2




Manual Integrations
APPROVED


Sohil
6/22/2018 5:57:57 PM

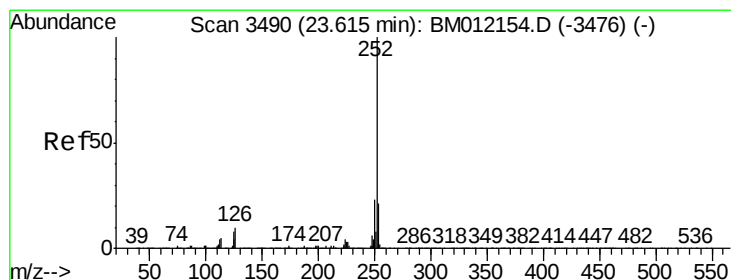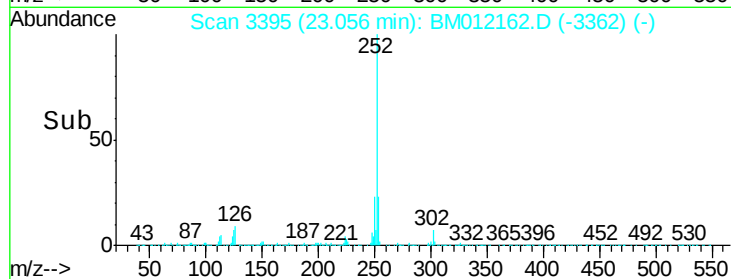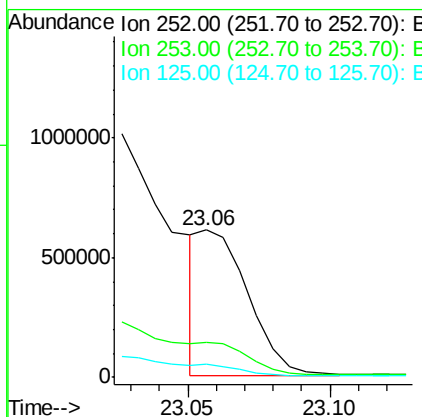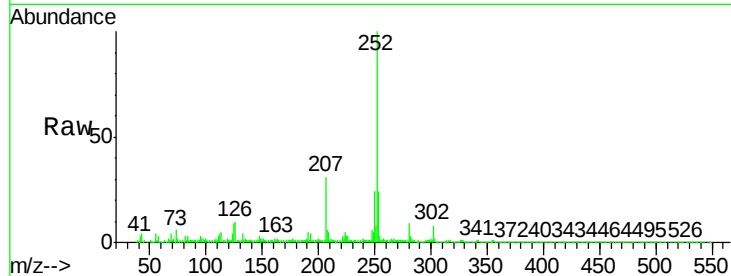

#88
Benzo(a)pyrene
Concen: 32.736 ng/ul
RT: 23.62 min Scan# 3491
Delta R.T. 0.01 min
Lab File: BM012162.D
Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	18.2	27.2
125	8.4	4.0	6.0

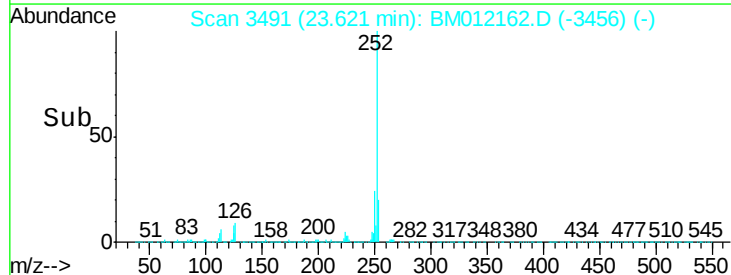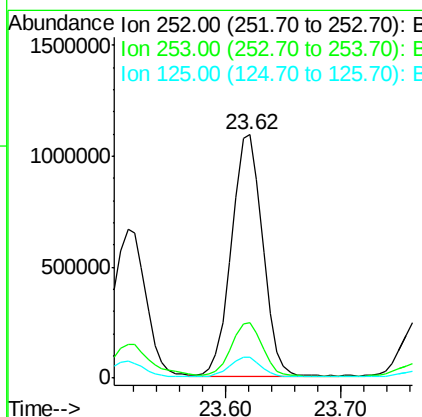

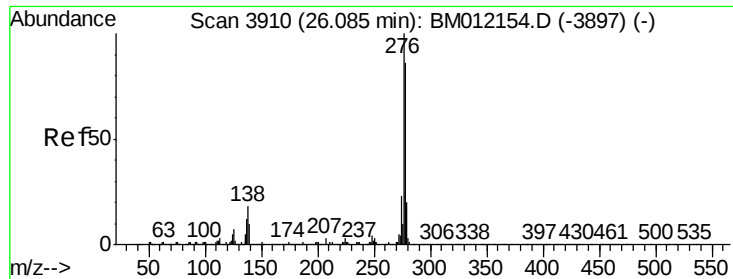





#89
 Indeno(1,2,3-cd)pyrene
 Concen: 18.889 ng/ul
 RT: 26.09 min Scan# 3910
 Delta R.T. 0.00 min
 Lab File: BM012162.D
 Acq: 14 Oct 2017 08:04

Instrument :
 BNA_M
 ClientSampleId :
 B-42(7-9)-100217

Tgt Ion	Ratio	Lower	Upper
276	100		
138	15.7	9.3	13.9#
277	25.1	19.9	29.9




Manual Integrations
 APPROVED




Sohil
 6/22/2018 5:57:57 PM

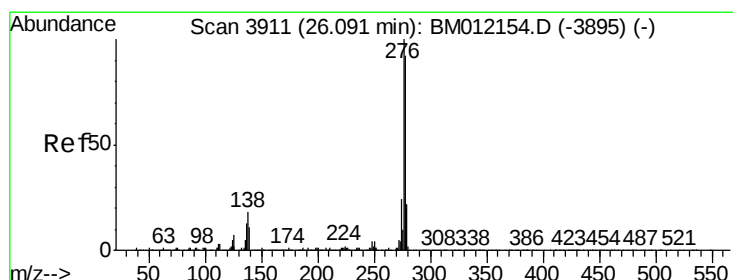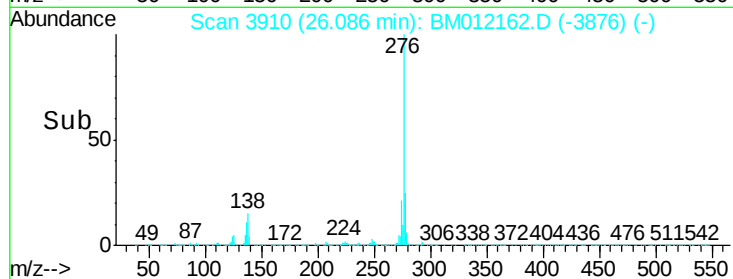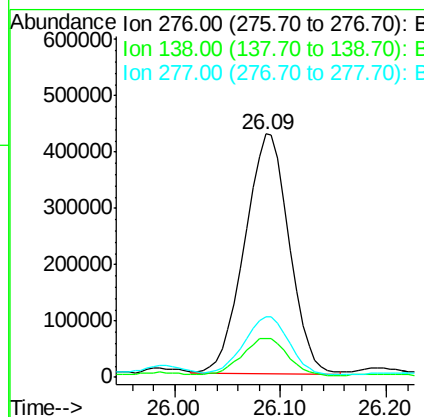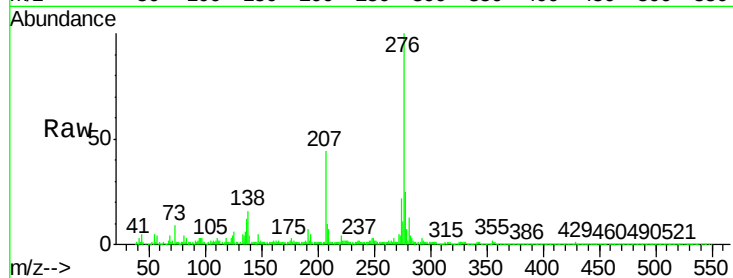

#90
 Dibenzo(a,h)anthracene
 Concen: 6.378 ng/ul
 RT: 26.09 min Scan# 3910
 Delta R.T. -0.01 min
 Lab File: BM012162.D
 Acq: 14 Oct 2017 08:04

Tgt Ion	Ratio	Lower	Upper
278	100		
139	16.2	5.8	8.8#
279	28.4	18.6	27.8#

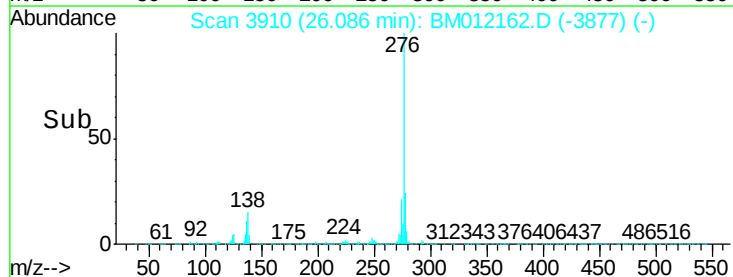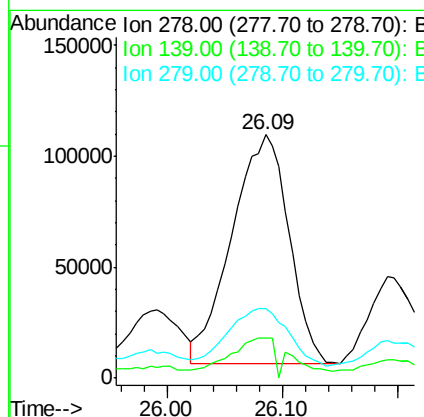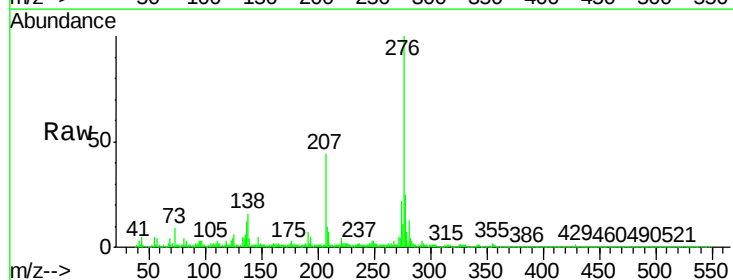

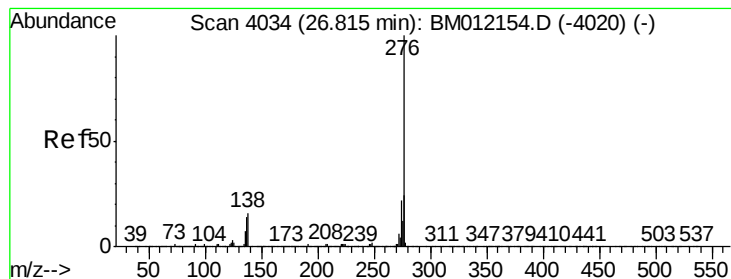

#91

Benzo(g,h,i)perylene

Concen: 19.195 ng/ul

RT: 26.82 min Scan# 4035

Delta R.T. 0.01 min

Lab File: BM012162.D

Acq: 14 Oct 2017 08:04

Instrument :

BNA_M

ClientSampleId :

B-42(7-9)-100217

Tgt Ion: 276 Resp: 1034336

Ion Ratio Lower Upper

276 100

138 15.4 8.5 12.7#

277 25.6 18.6 28.0

Manual Integrations

APPROVED

Sohil

6/22/2018 5:57:57 PM

