

Data Path : Z:\HPCHEM1\BNA_M\Data\BM101317\
 Data File : BM012147.D
 Acq On : 13 Oct 2017 22:37
 Operator : SJ/JU
 Sample : I5772-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE2N6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	37	rVB	50974	84141	1.15%	0.134%
2	6.992	658	664	677	rBV	197851	360032	4.93%	0.574%
3	7.151	682	691	703	rBV	673319	1085038	14.85%	1.730%
4	7.357	719	726	740	rBV	801606	1327969	18.17%	2.117%
5	7.822	799	805	820	rBV	667873	1162645	15.91%	1.853%
6	8.539	920	927	945	rBV	623972	1121867	15.35%	1.788%
7	8.992	996	1004	1024	rBV	943916	1646885	22.54%	2.625%
8	9.716	1119	1127	1139	rBV	862268	1513905	20.72%	2.413%
9	10.257	1212	1219	1234	rBV	1098308	2092724	28.64%	3.336%
10	10.628	1275	1282	1296	rVB	988065	1708036	23.38%	2.723%
11	13.886	1829	1836	1853	rBV	2691443	3915336	53.58%	6.241%
12	14.174	1877	1885	1899	rBV	2900046	4316605	59.08%	6.881%
13	14.480	1930	1937	1948	rVB2	1583376	2543826	34.81%	4.055%
14	14.704	1969	1975	1989	rBV	140993	333280	4.56%	0.531%
15	15.474	2099	2106	2113	rBV	3679351	5407955	74.01%	8.620%
16	15.615	2124	2130	2142	rBV	1272919	1917635	26.24%	3.057%
17	15.710	2142	2146	2154	rVB	51726	81738	1.12%	0.130%
18	17.227	2397	2404	2413	rBV2	2221920	3281850	44.91%	5.231%
19	17.327	2414	2421	2439	rVV	4355794	6192300	84.75%	9.870%
20	18.098	2547	2552	2559	rBV2	118838	192105	2.63%	0.306%
21	19.256	2743	2749	2755	rBV	79822	156818	2.15%	0.250%
22	19.374	2766	2769	2775	rBV	219655	314615	4.31%	0.501%
23	19.621	2805	2811	2819	rBV	5398148	7234570	99.01%	11.532%
24	21.403	3109	3114	3121	rBV	2917591	3871891	52.99%	6.172%
25	23.580	3477	3484	3499	rVB2	3497693	7306936	100.00%	11.647%
26	23.721	3503	3508	3516	rVB2	1842935	3565447	48.80%	5.683%


Sum of corrected areas: 62736149

Data Path : Z:\HPCHEM1\BNA_M\Data\BM101317\
Data File : BM012147.D
Acq On : 13 Oct 2017 22:37
Operator : SJ/JU
Sample : I5772-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2N6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

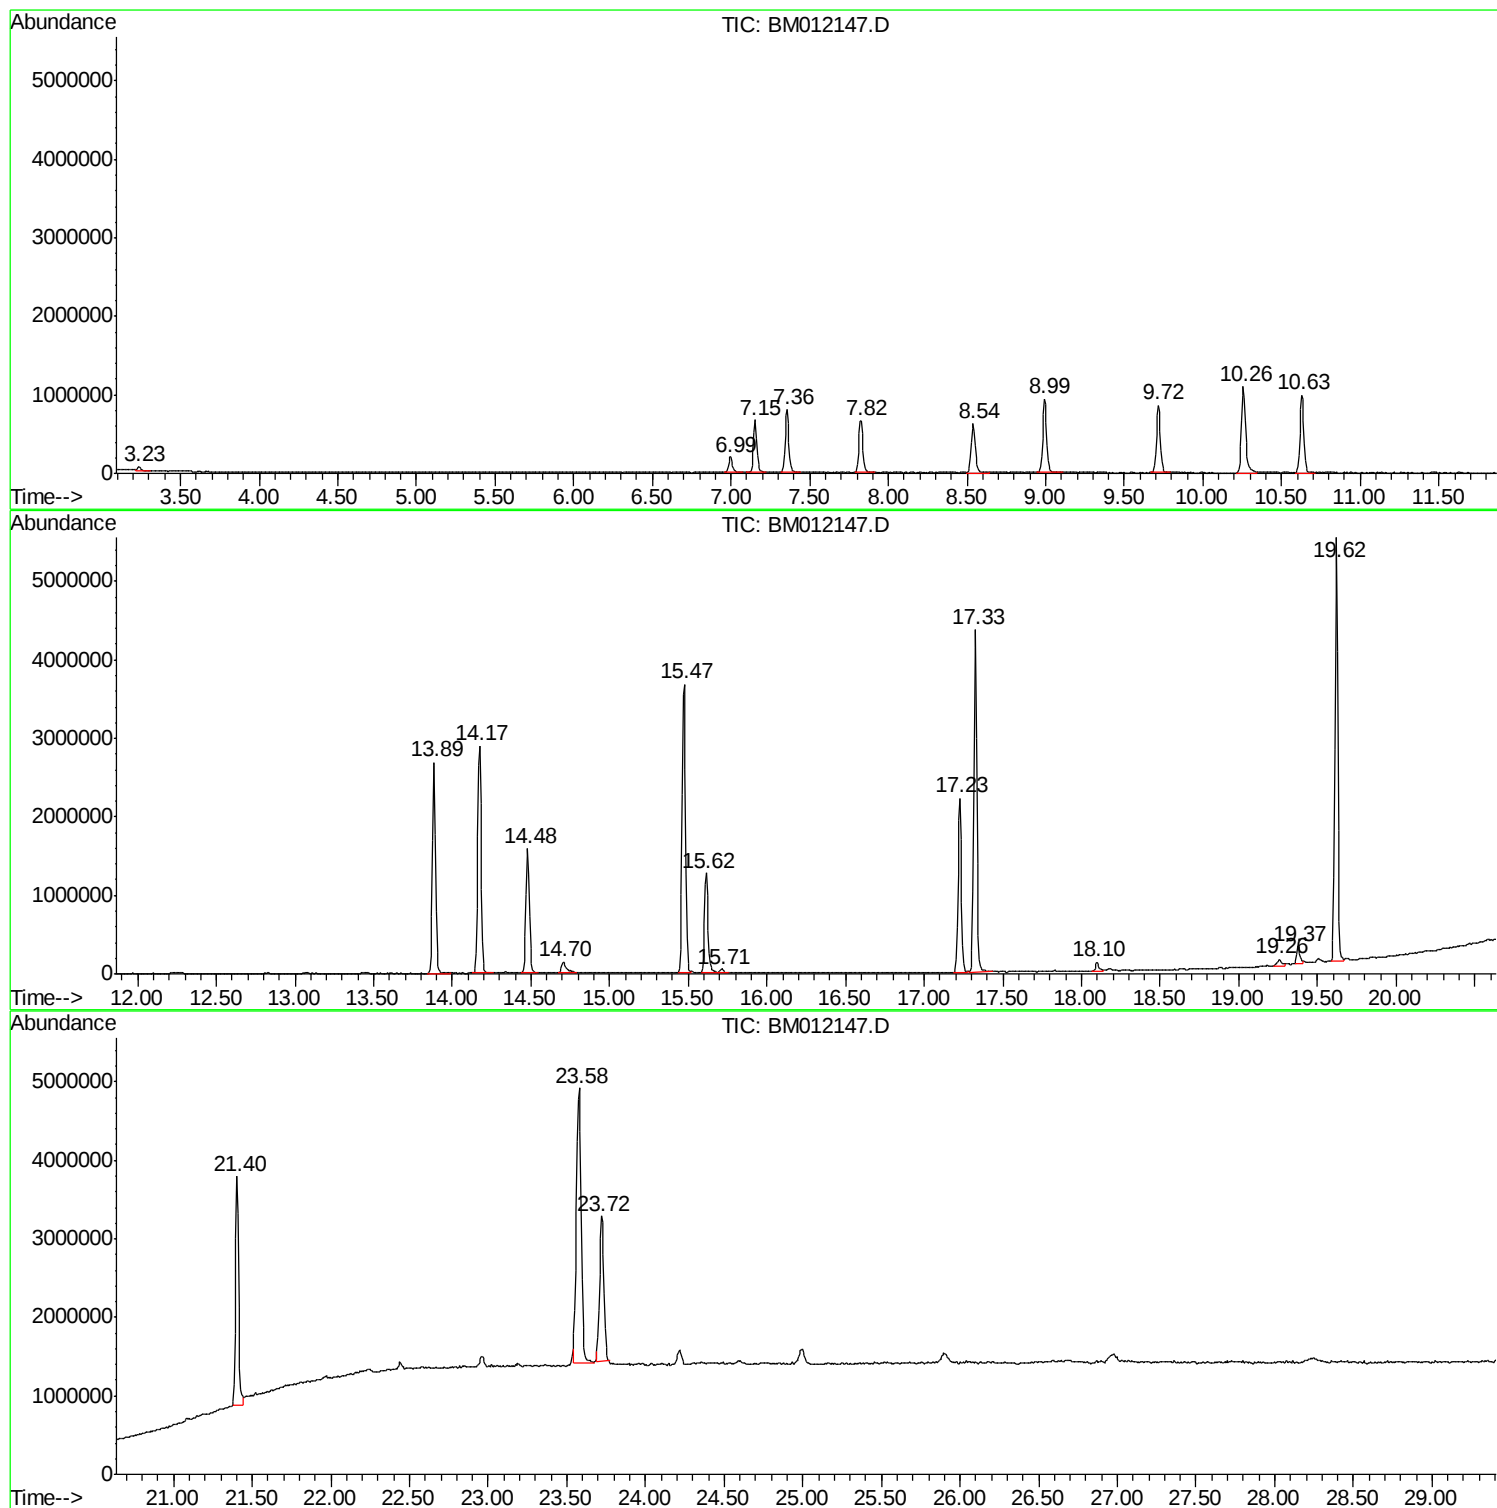

Data Path : Z:\HPCHEM1\BNA_M\Data\BM101317\
Data File : BM012147.D
Acq On : 13 Oct 2017 22:37
Operator : SJ/JU
Sample : I5772-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2N6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM101317\
Data File : BM012147.D
Acq On : 13 Oct 2017 22:37
Operator : SJ/JU
Sample : I5772-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2N6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc