

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101318\
 Data File : BM017151.D
 Acq On : 13 Oct 2018 17:33
 Operator : MJ/SJ
 Sample : J5400-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 15 12:27:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 12 23:37:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	198040	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	903502	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	516405	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1151643	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1013549	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	889758	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds


					Qvalue
37) 1,2,4,5-Tetrachlorobenzene	12.50	216	106542	6.008 ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.12	216	204285	11.115 ng/uL	96
77) Fluoranthene	19.14	202	134804	1.802 ng/ul	99
80) Pyrene	19.50	202	60649	1.033 ng/ul	98
85) Chrysene	21.30	228	71780	1.221 ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101318\
Data File : BM017151.D
Acq On : 13 Oct 2018 17:33
Operator : MJ/SJ
Sample : J5400-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Quant Time: Oct 15 12:27:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 12 23:37:04 2018
Response via : Initial Calibration

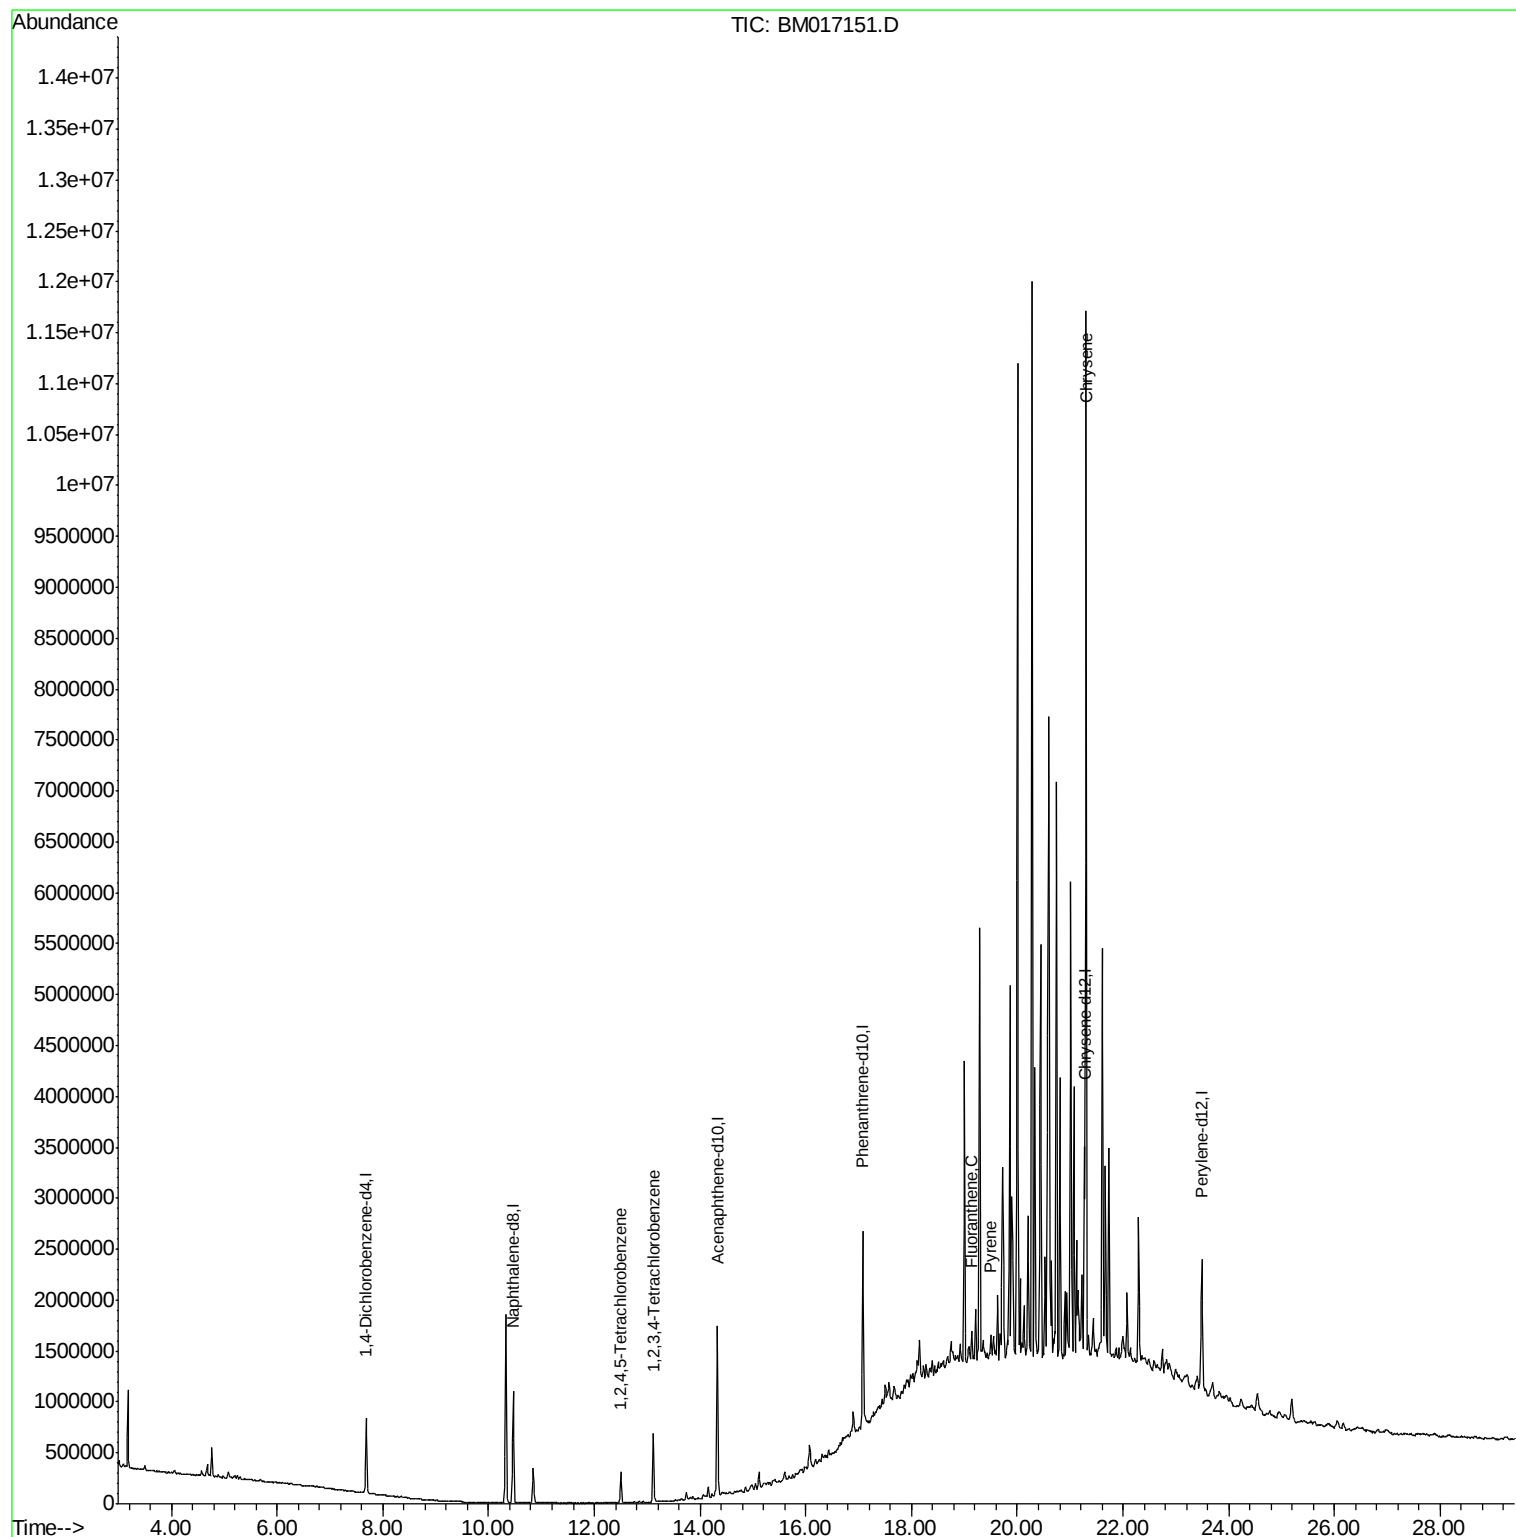


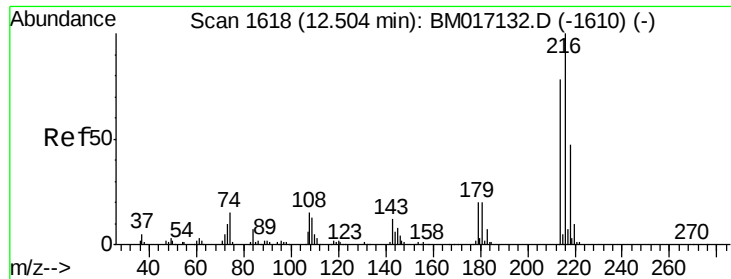


#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 6.008 ng/ul
 RT: 12.50 min Scan# 1618
 Delta R.T. -0.00 min
 Lab File: BM017151.D
 Acq: 13 Oct 2018 17:33

Tgt Ion:	216	Resp:	106542
Ion	Ratio	Lower	Upper
216	100		
214	78.1	61.0	91.6
179	20.4	16.6	24.8
108	14.3	12.7	19.1

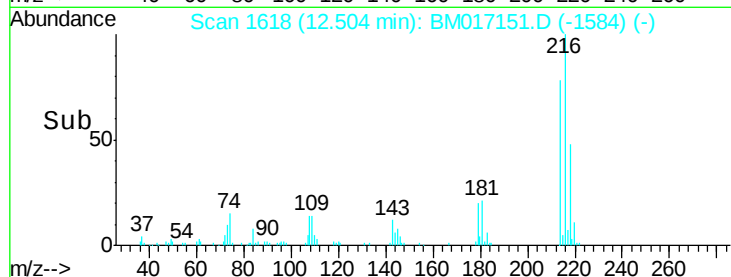
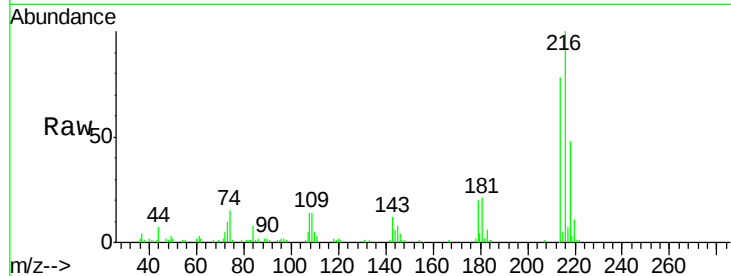


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E

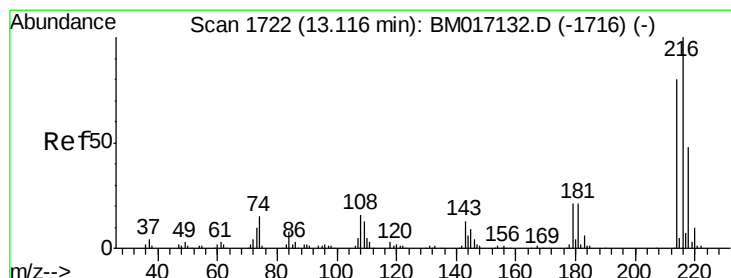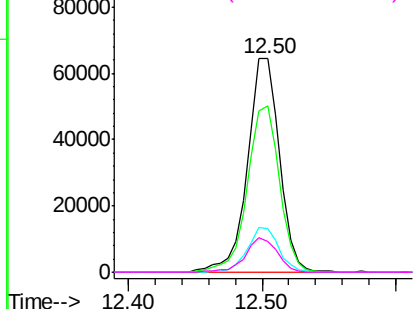



#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 11.115 ng/uL
 RT: 13.12 min Scan# 1722
 Delta R.T. -0.00 min
 Lab File: BM017151.D
 Acq: 13 Oct 2018 17:33

Tgt Ion:	216	Resp:	204285
Ion	Ratio	Lower	Upper
216	100		
214	80.4	61.6	92.4
218	49.5	37.8	56.6

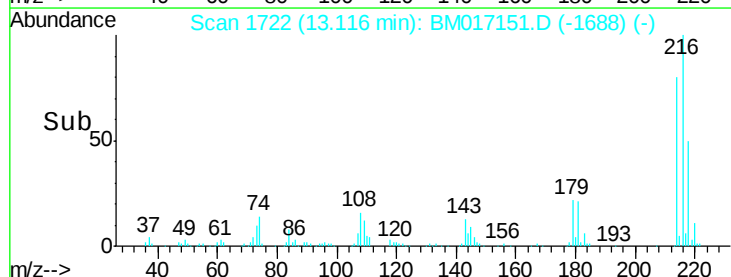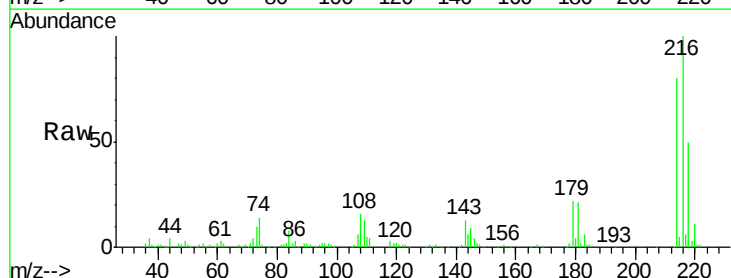


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

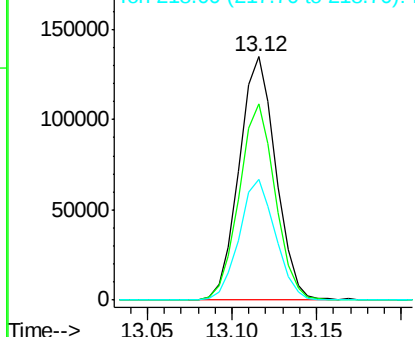



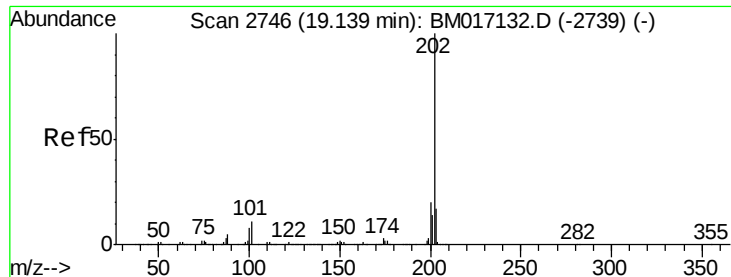


#77
 Fluoranthene
 Concen: 1.802 ng/ul
 RT: 19.14 min Scan# 2746
 Delta R.T. -0.00 min
 Lab File: BM017151.D
 Acq: 13 Oct 2018 17:33

Tgt Ion:	202	Resp:	134804
Ion Ratio	Lower	Upper	
202	100		
101	10.6	8.3	12.5
100	8.8	6.6	9.8

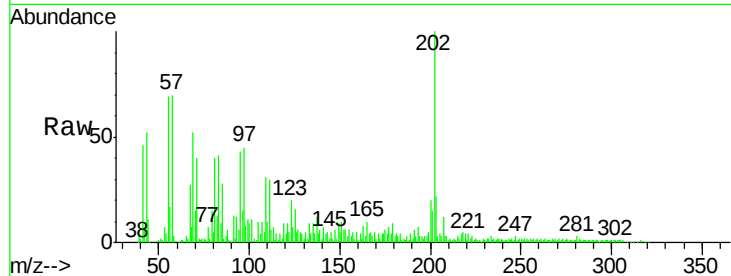


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

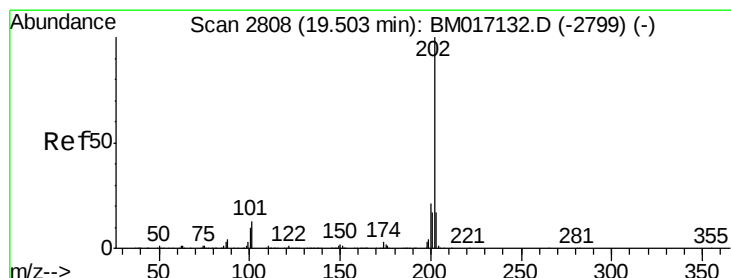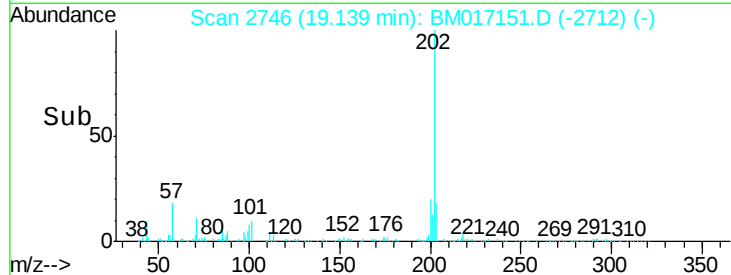
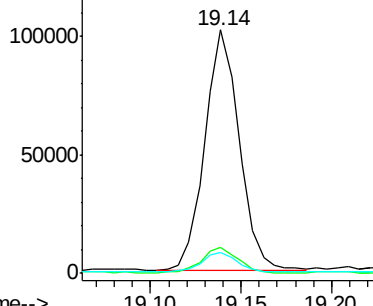



#80
 Pyrene
 Concen: 1.033 ng/ul
 RT: 19.50 min Scan# 2808
 Delta R.T. -0.00 min
 Lab File: BM017151.D
 Acq: 13 Oct 2018 17:33

Tgt Ion:	202	Resp:	60649
Ion Ratio	Lower	Upper	
202	100		
101	13.4	10.8	16.2
100	12.4	8.9	13.3

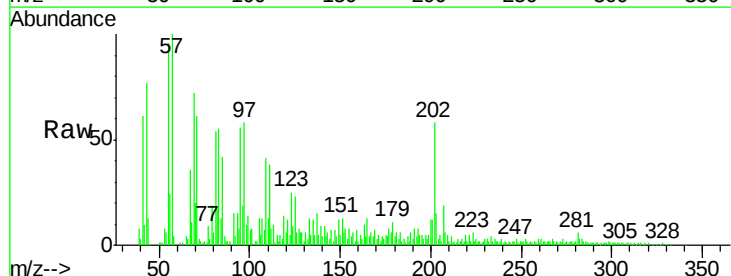


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

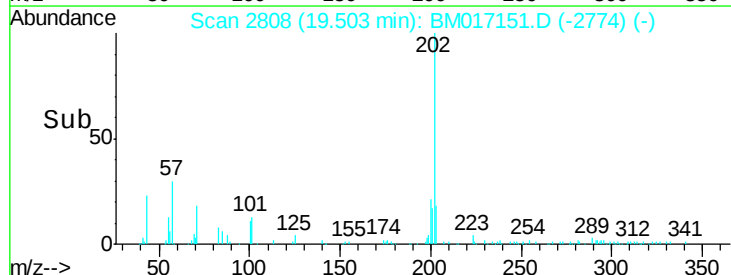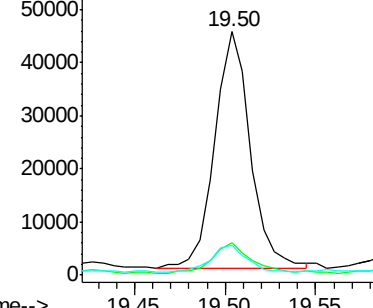

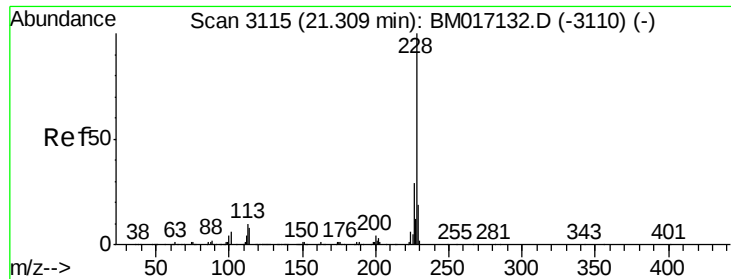

#85
 Chrysene
 Concen: 1.221 ng/ul
 RT: 21.30 min Scan# 3114
 Delta R.T. -0.01 min
 Lab File: BM017151.D
 Acq: 13 Oct 2018 17:33

Tgt Ion: 228 Resp: 71780
 Ion Ratio Lower Upper
 228 100
 226 33.9 23.4 35.2
 229 33.8 15.6 23.4#

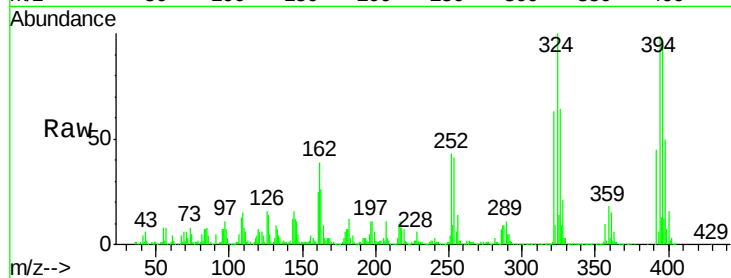

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E

