


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101318\
 Data File : BM017141.D
 Acq On : 13 Oct 2018 11:31
 Operator : MJ/SJ
 Sample : DFTPP18
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP18

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION
 Last Update : Fri Oct 12 23:37:04 2018

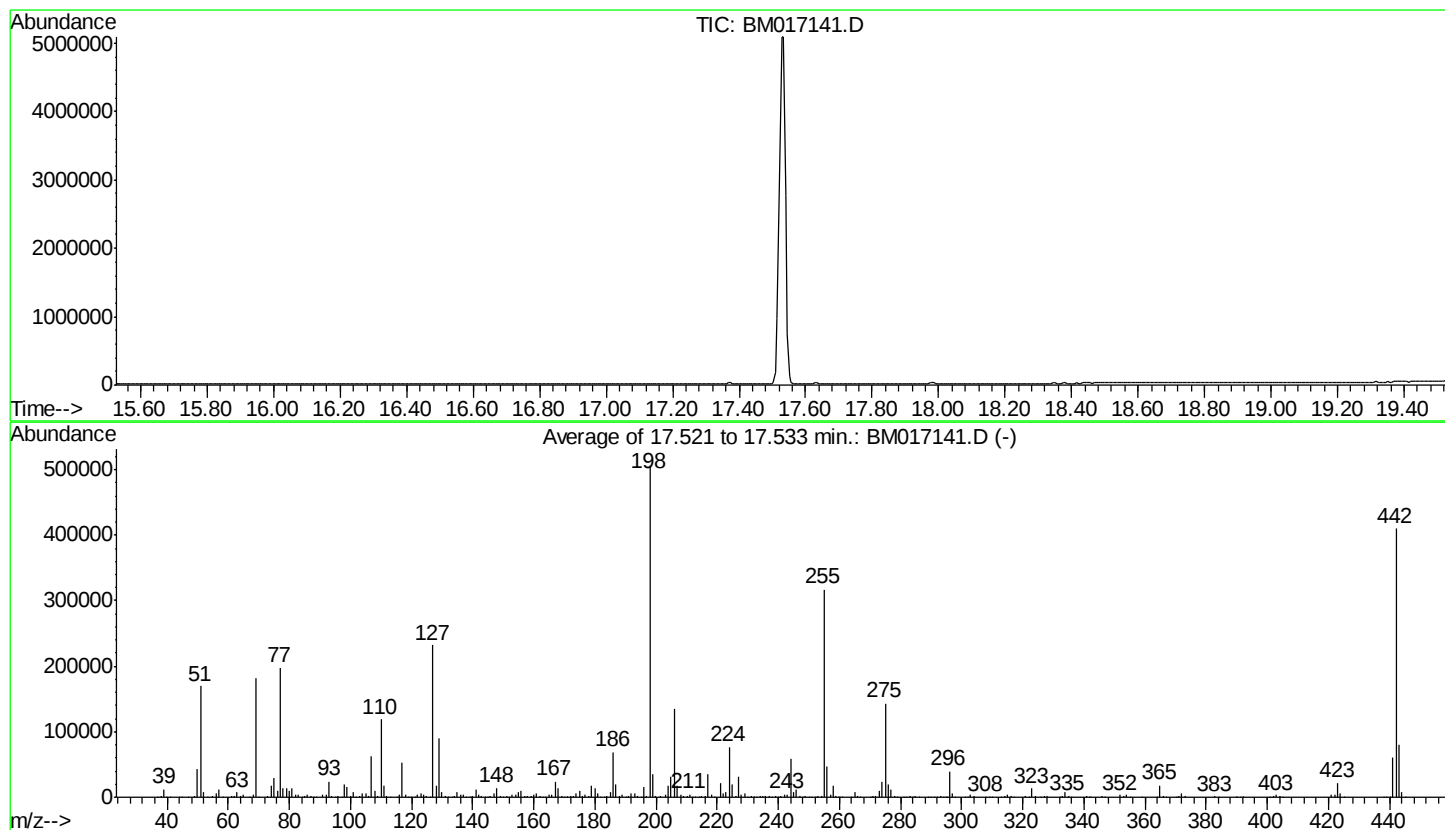

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	169365	PASS
68	69	0.00	2	2.0	3602	PASS
69	198	0.00	100	35.8	181141	PASS
70	69	0.00	2	0.5	915	PASS
127	198	10	80	45.9	232277	PASS
197	198	0.00	2	0.5	2748	PASS
198	198	100	100	100.0	506154	PASS
199	198	5	9	6.9	34722	PASS
275	198	10	60	28.3	143250	PASS
365	198	1	100	3.6	18188	PASS
441	198	0.01	100	12.1	61010	PASS
442	198	50	100	81.1	410282	PASS
443	442	15	24	19.5	80128	PASS