

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
 Data File : BM032488.D
 Acq On : 13 Oct 2021 10:20
 Operator : CG/JU
 Sample : PB139804BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB139804BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	392	399	416	rBV	4765646	6767385	46.80%	9.841%
2	6.801	666	674	688	rBV	4389127	7159973	49.52%	10.412%
3	7.601	804	810	823	rBV	845013	1344222	9.30%	1.955%
4	8.760	999	1007	1029	rBV	2900448	4649798	32.16%	6.762%
5	10.389	1278	1284	1302	rBV	1193430	1997971	13.82%	2.905%
6	12.872	1699	1706	1721	rBV	7386430	10949134	75.73%	15.922%
7	14.254	1934	1941	1955	rBV	2010695	2884391	19.95%	4.194%
8	15.742	2187	2194	2216	rBV	5591720	8210734	56.79%	11.940%
9	16.977	2398	2404	2416	rBV	2533364	3514499	24.31%	5.111%
10	19.601	2844	2850	2855	rBV	10558130	14458697	100.00%	21.026%
11	21.148	3108	3113	3123	rBV	2859436	3574914	24.73%	5.199%
12	23.289	3471	3477	3487	rVB2	1960677	3255376	22.52%	4.734%




Sum of corrected areas: 68767094

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
Data File : BM032488.D
Acq On : 13 Oct 2021 10:20
Operator : CG/JU
Sample : PB139804BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

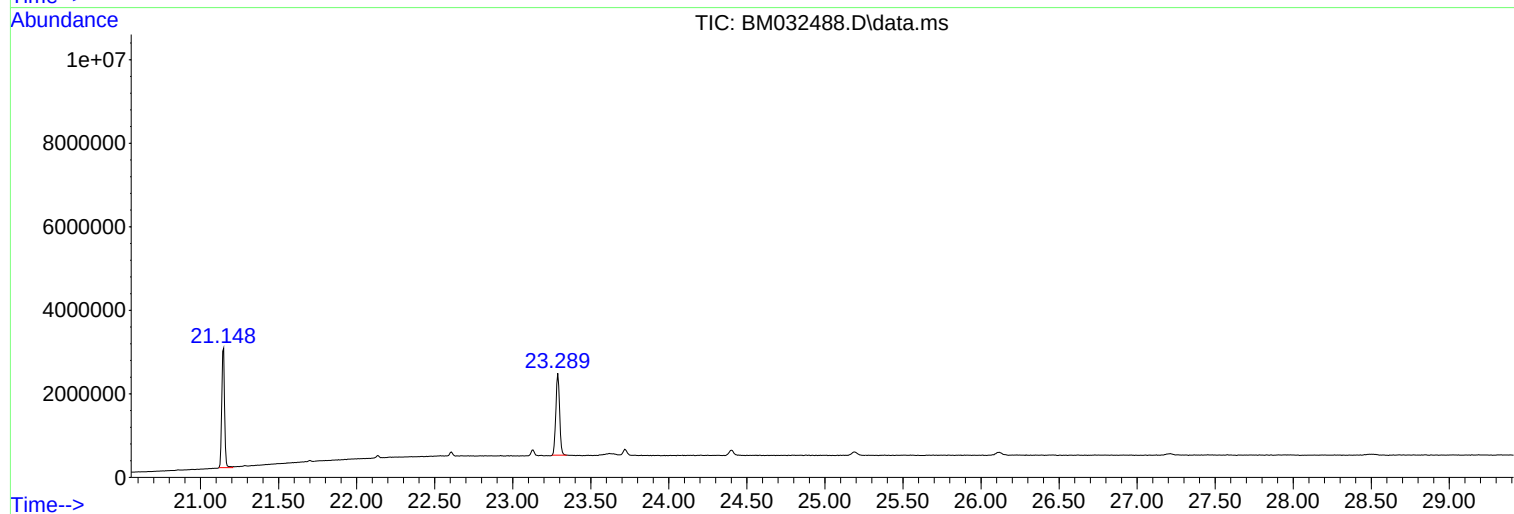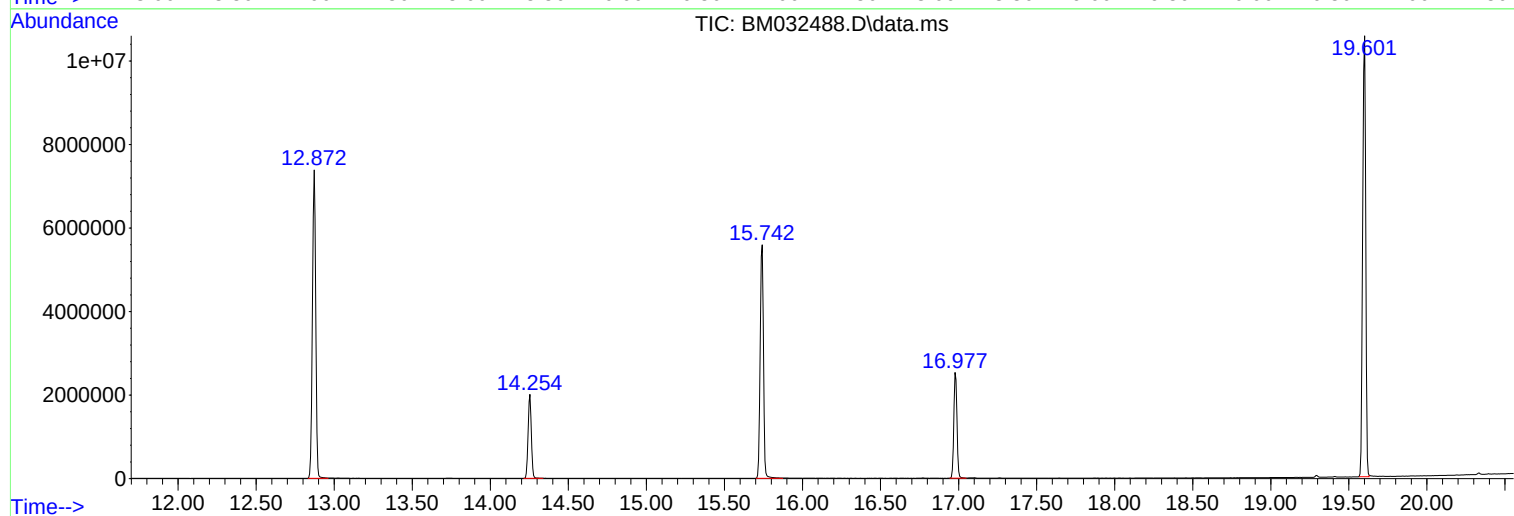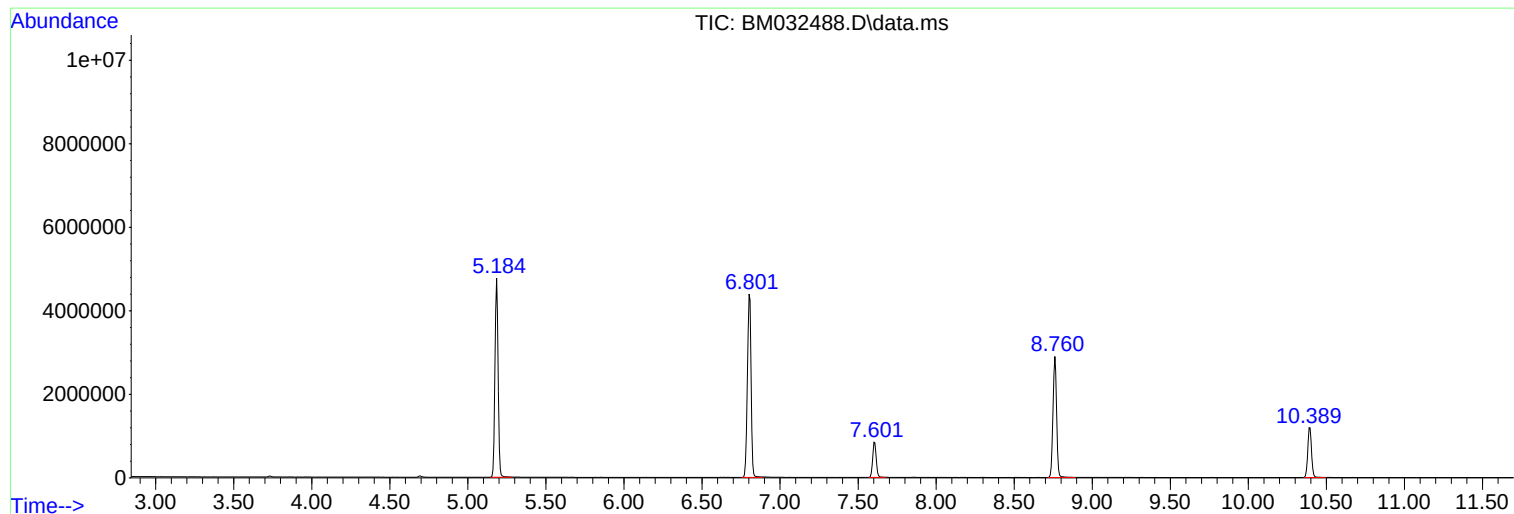

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
Data File : BM032488.D
Acq On : 13 Oct 2021 10:20
Operator : CG/JU
Sample : PB139804BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
Data File : BM032488.D
Acq On : 13 Oct 2021 10:20
Operator : CG/JU
Sample : PB139804BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------