


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
 Data File : BM032486.D
 Acq On : 13 Oct 2021 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 13 12:02:28 2021

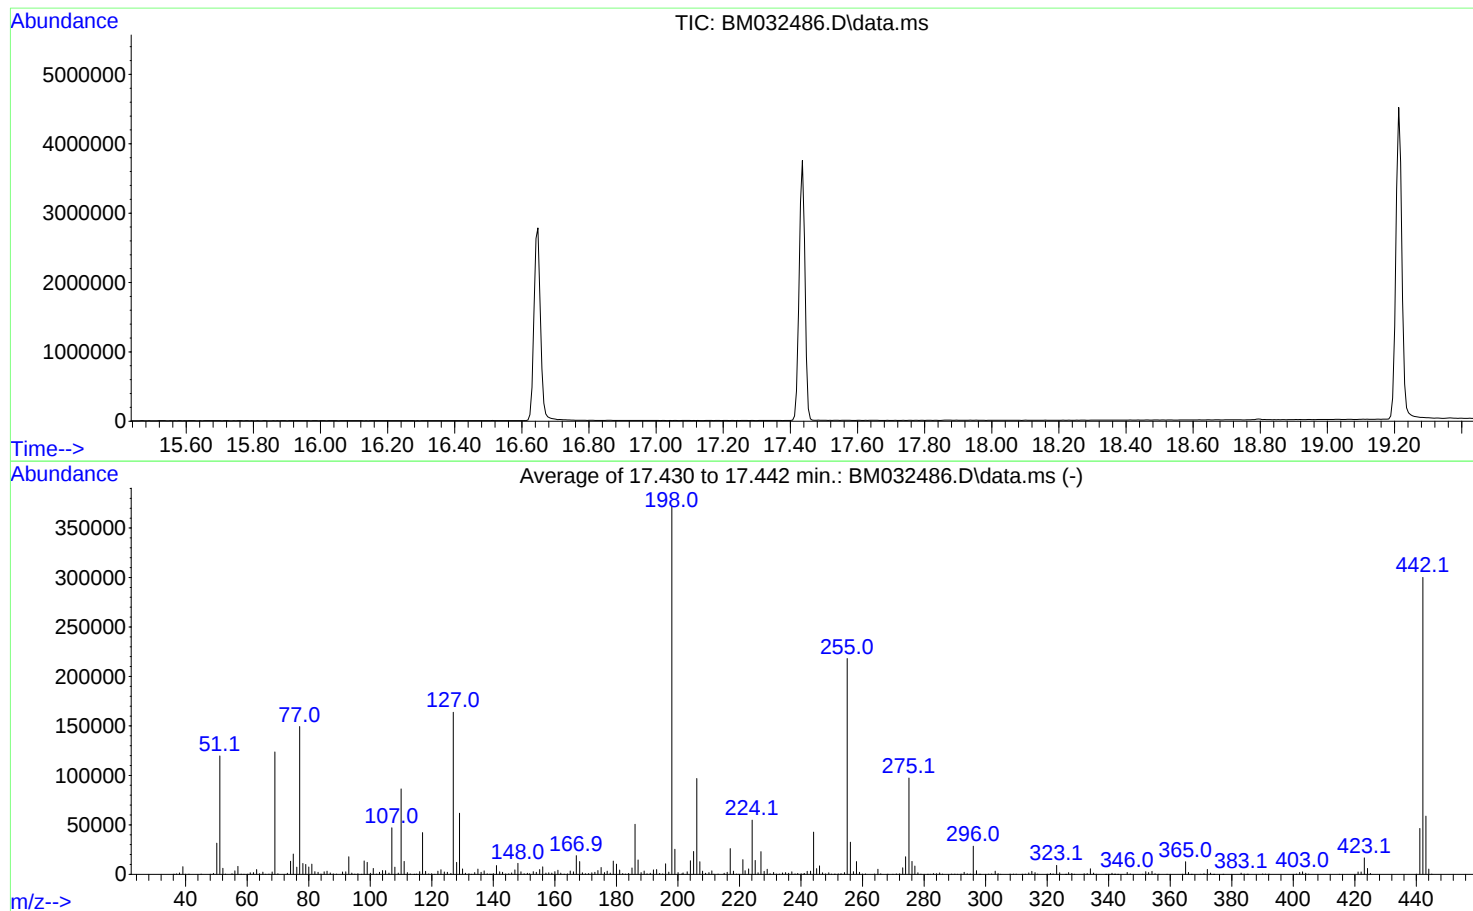




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	119640	PASS
68	69	0.00	2	1.9	2378	PASS
69	198	0.00	100	33.3	123699	PASS
70	69	0.00	2	0.6	725	PASS
127	198	10	80	44.1	163765	PASS
197	198	0.00	2	0.6	2329	PASS
198	198	100	100	100.0	371755	PASS
199	198	5	9	6.8	25341	PASS
275	198	10	60	26.2	97320	PASS
365	198	1	100	3.5	12839	PASS
441	198	0.01	100	12.5	46459	PASS
442	442	50	100	100.0	300181	PASS
443	442	15	24	19.6	58899	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
Data File : BM032486.D
Acq On : 13 Oct 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:32:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 12:02:28 2021
Response via : Initial Calibration

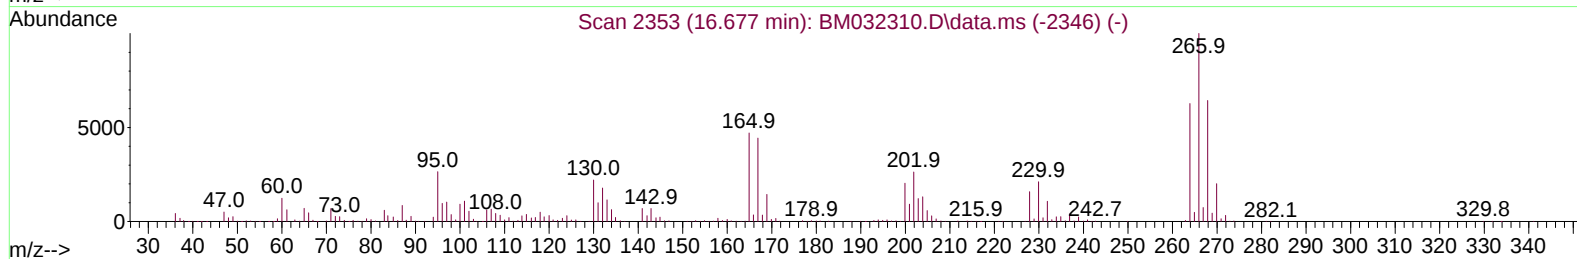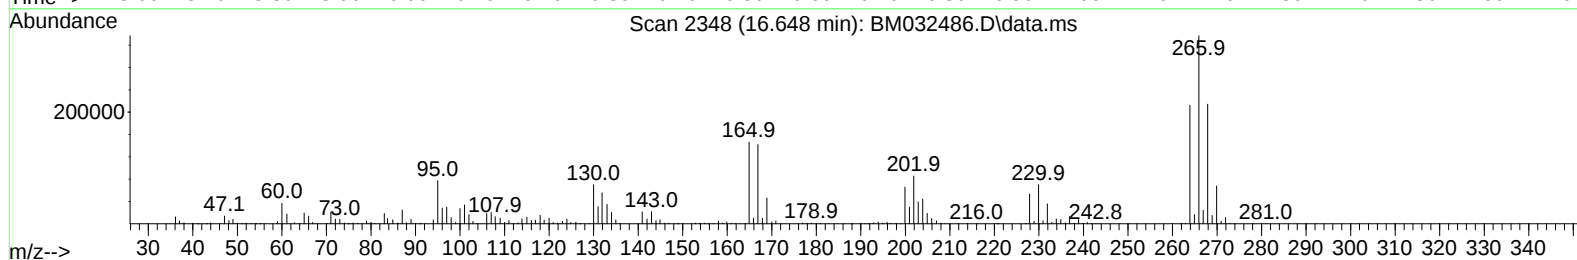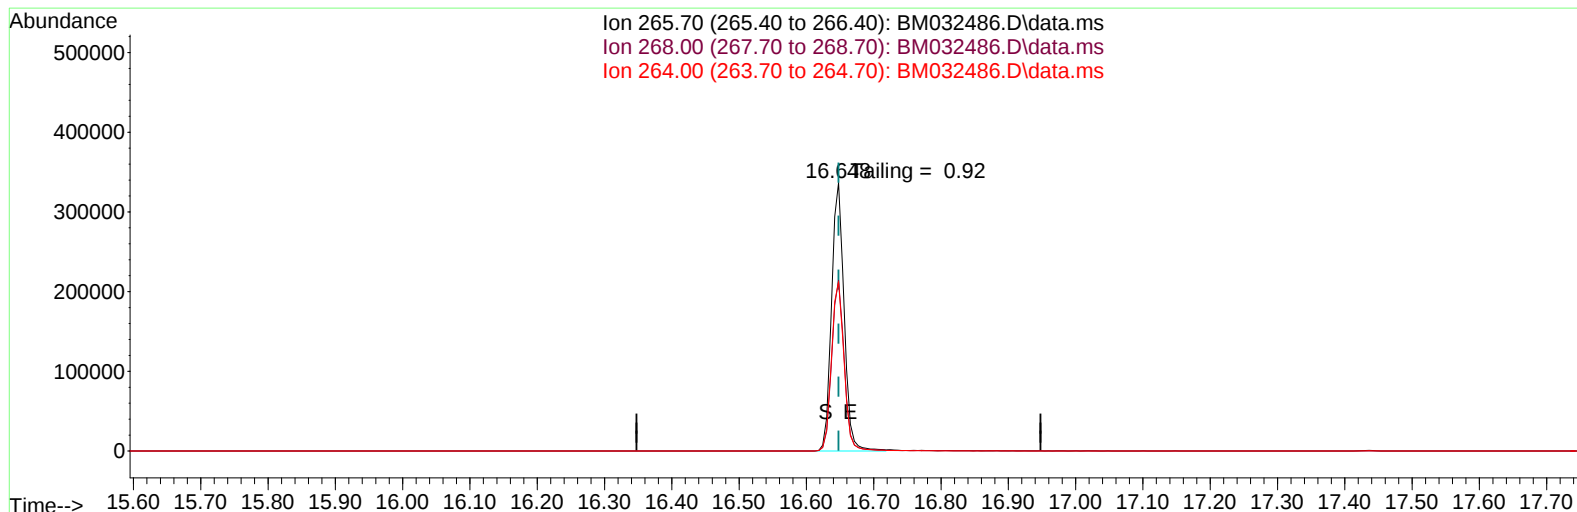

TIC: BM032486.D\data.ms

(70) Pentachlorophenol (C)

16.648min (-0.000) 73086.57 ng




response 439819

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.63
264.00	65.10	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101321\
Data File : BM032486.D
Acq On : 13 Oct 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:32:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 12:02:28 2021
Response via : Initial Calibration

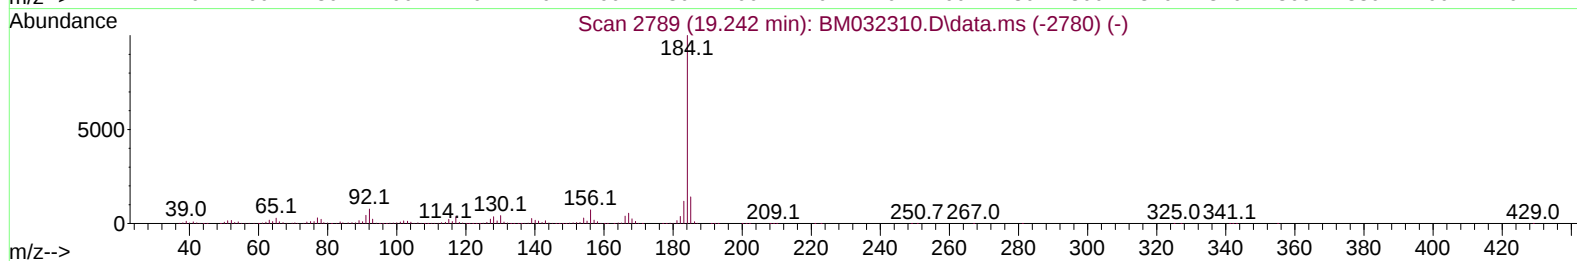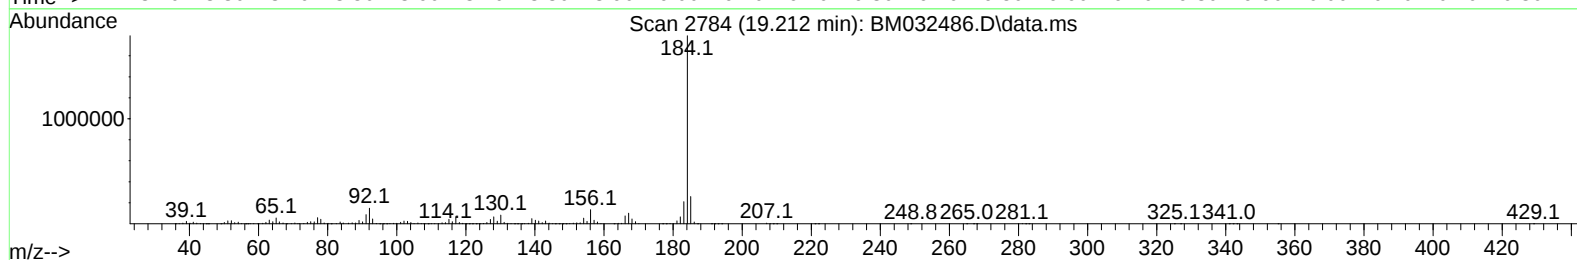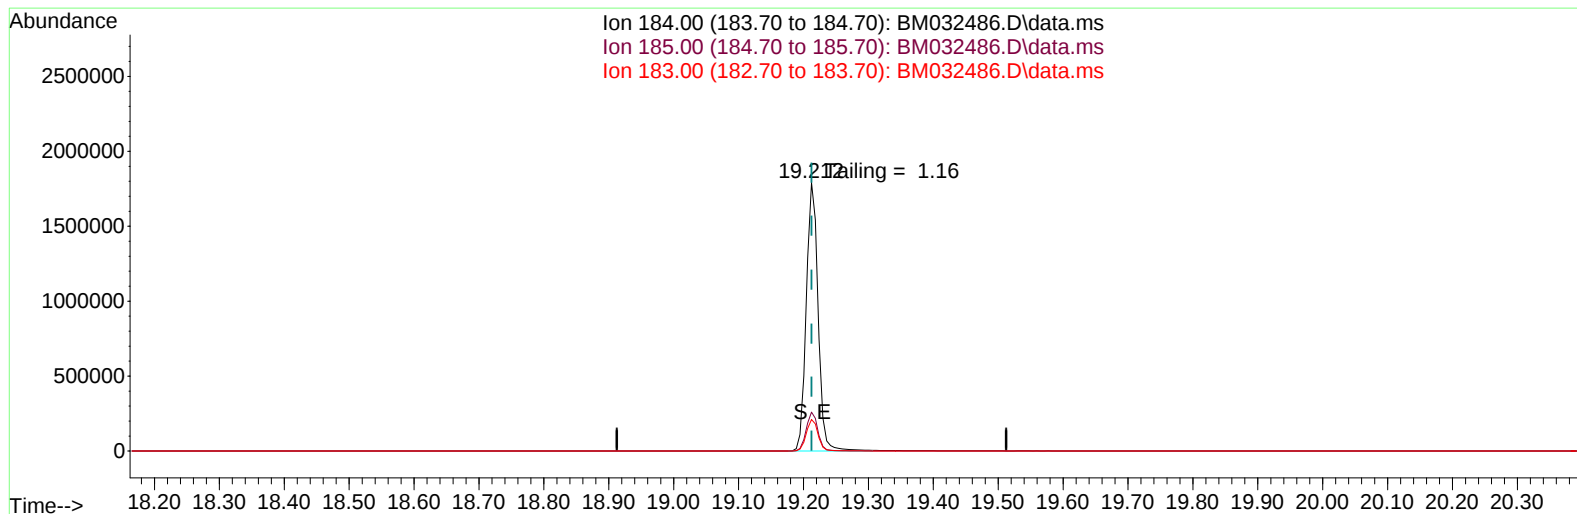

TIC: BM032486.D\data.ms

(77) Benzidine

19.212min (-0.000) 44580.89 ng

response 2290177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.51
183.00	11.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2021	BNA_M	<u>BM032486.D</u>
Compound Name	Response	Retention Time
DDT	1185502	20.453
DDD	44721	20.012
DDE	2331	19.512
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47052	1232554	3.82

Instrument :
BNA_M
ClientSampleId :
DFTPP