

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037021.D
 Acq On : 13 Oct 2022 17:32
 Operator : CG/JU
 Sample : N5026-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BX4

Quant Time: Oct 13 23:35:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	6896	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	25167	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.570	164	13914	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	27672	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240	17749	0.400	ng/ul	0.00
23) Perylene-d12	23.876	264	14436	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	34690	3.567	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	12189	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	26614	0.501	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.382	88	915	0.096	ng/ul#	73
20) Pyrene	19.693	202	3812	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.721	252	5539	0.106	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037021.D
Acq On : 13 Oct 2022 17:32
Operator : CG/JU
Sample : N5026-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BX4


Quant Time: Oct 13 23:35:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

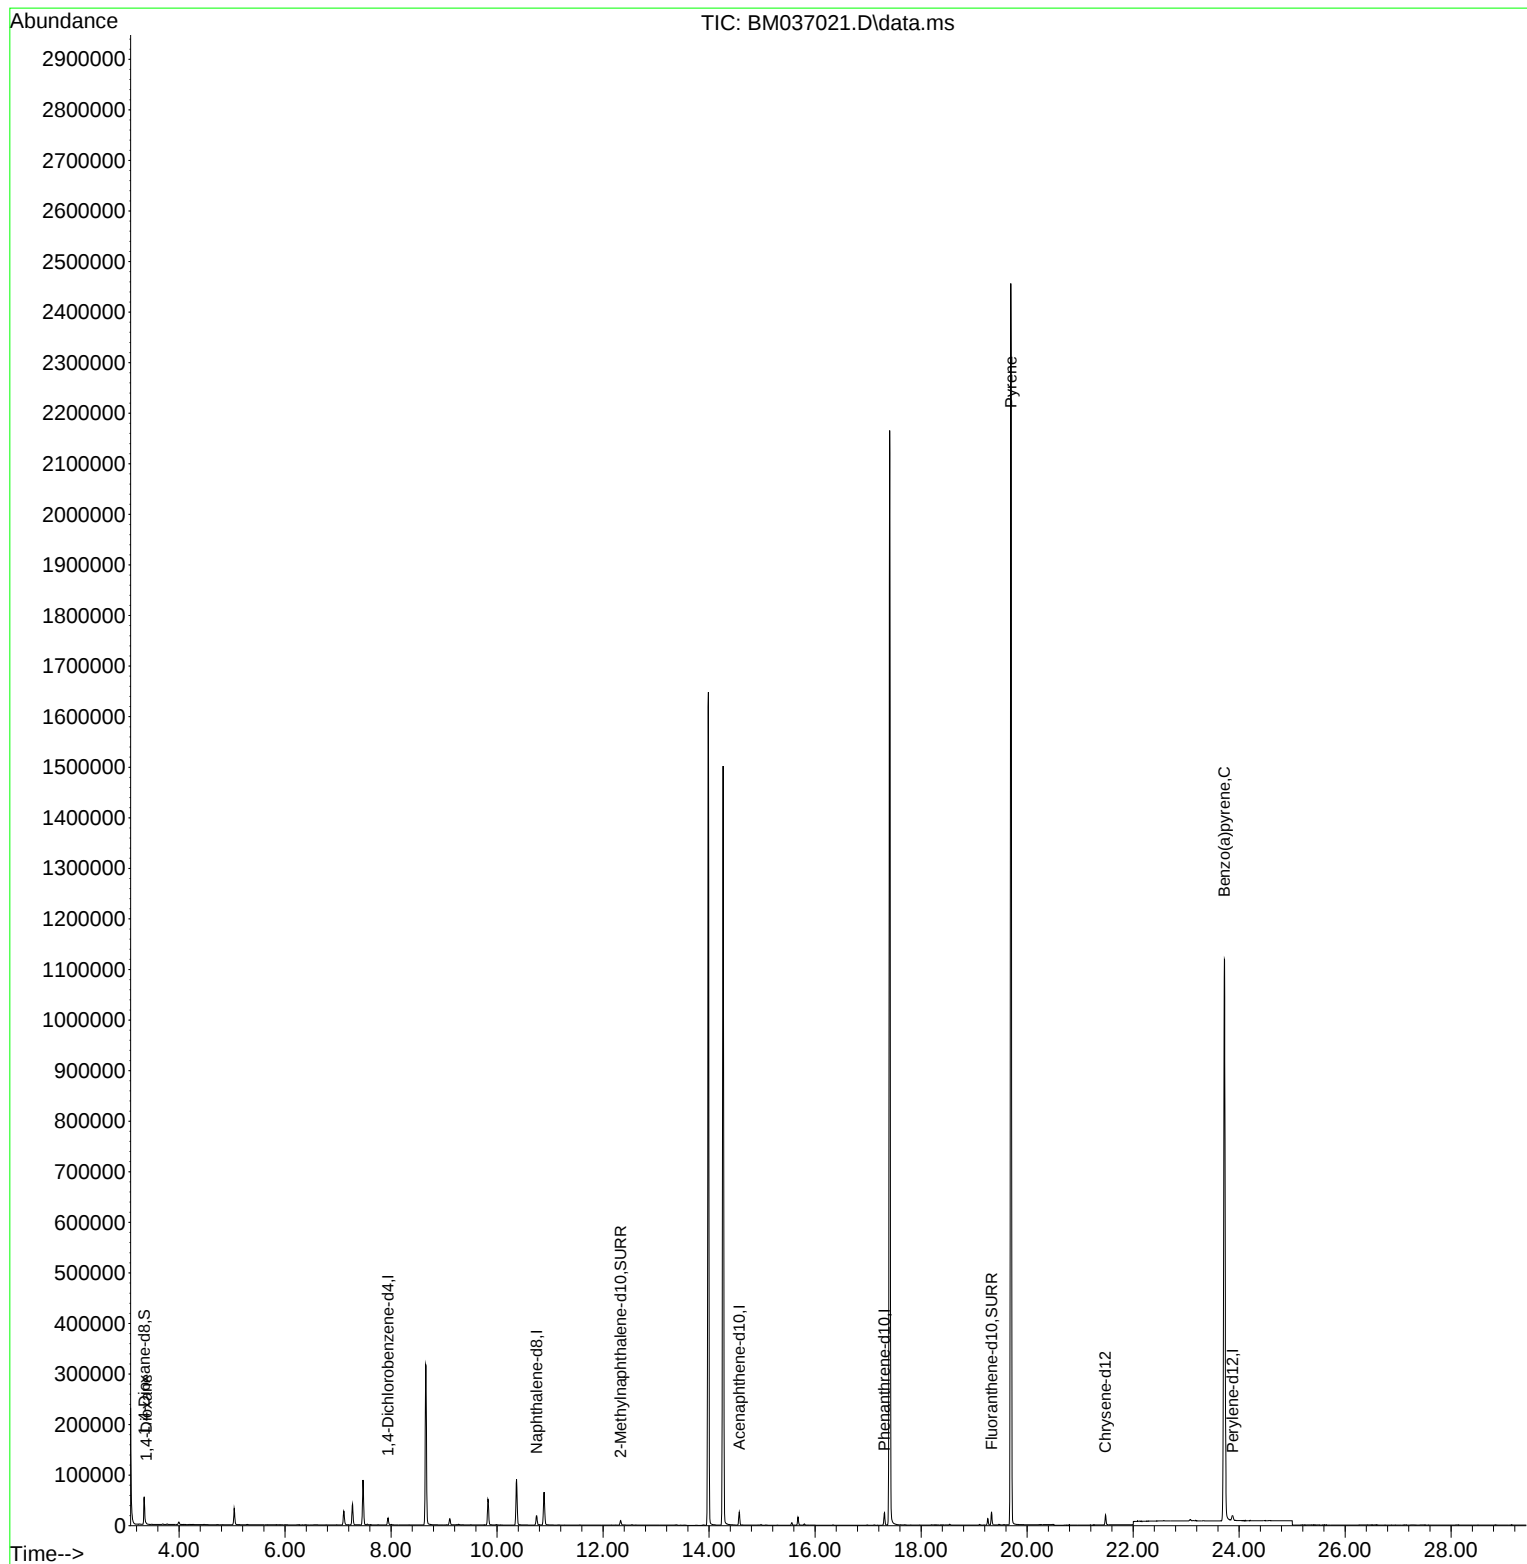



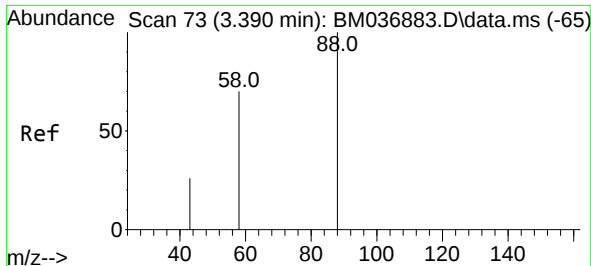


#2
1,4-Dioxane
Concen: 0.096 ng/ul
RT: 3.382 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM037021.D
Acq: 13 Oct 2022 17:32


Instrument :
BNA_M
ClientSampleId :
C0BX4

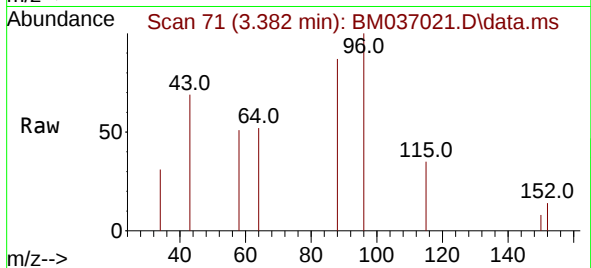



Tgt Ion: 88 Resp: 915
Ion Ratio Lower Upper
88 100
43 79.6 37.8 56.6#
58 59.1 42.6 63.8

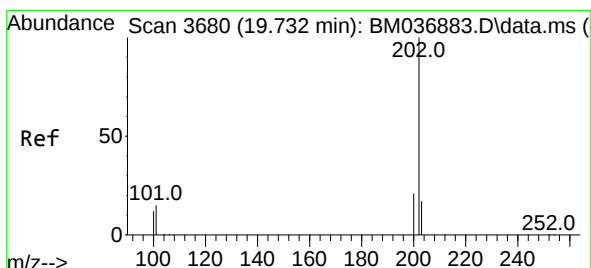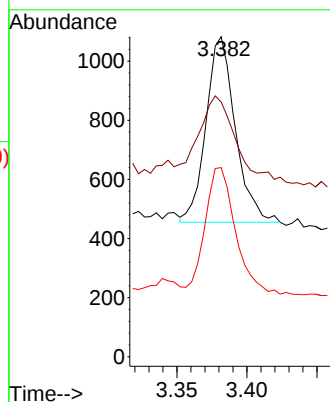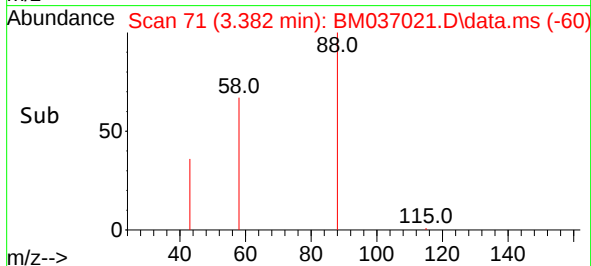


#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.693 min Scan# 3672
Delta R.T. -0.033 min
Lab File: BM037021.D
Acq: 13 Oct 2022 17:32

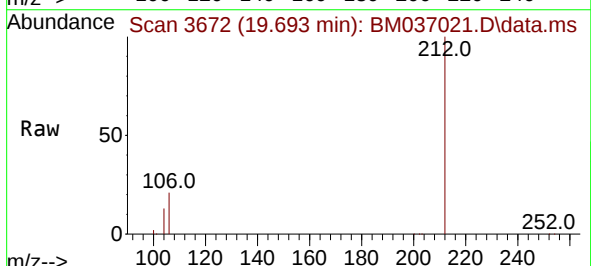


Tgt Ion: 202 Resp: 3812
Ion Ratio Lower Upper
202 100
101 160.5 12.0 18.0#
100 1217.7 9.8 14.6#

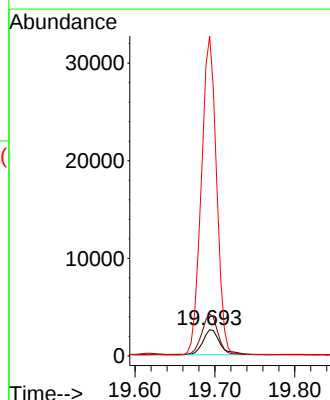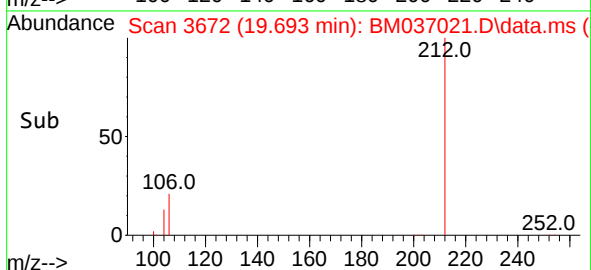

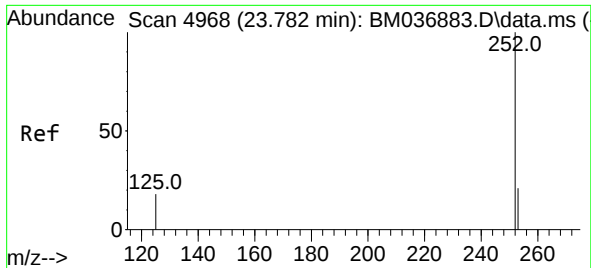

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.721 min Scan# 4947
Delta R.T. -0.050 min
Lab File: BM037021.D
Acq: 13 Oct 2022 17:32

Instrument :
BNA_M
ClientSampleId :
C0BX4

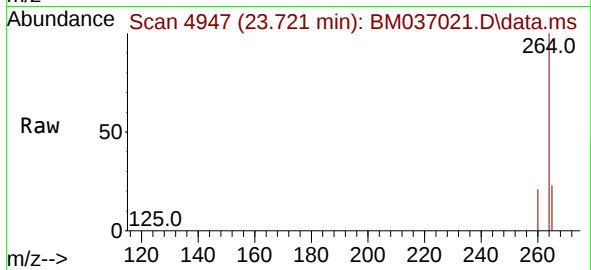

Tgt Ion:252 Resp: 5539
Ion Ratio Lower Upper
252 100
253 53.8 29.7 44.5#
125 60.6 23.6 35.4#

