

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037025.D
 Acq On : 13 Oct 2022 20:33
 Operator : CG/JU
 Sample : PB148252BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK252

Quant Time: Oct 13 23:36:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	7450	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	26937	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.567	164	14590	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.306	188	28167	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240	16065	0.400	ng/ul	0.00
23) Perylene-d12	23.872	264	13951	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	46932	4.467	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	12165	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.327	212	19565	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.557	166	3445	0.058	ng/ul#	15
20) Pyrene	19.694	202	2587	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.718	252	3776	0.075	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037025.D
Acq On : 13 Oct 2022 20:33
Operator : CG/JU
Sample : PB148252BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK252

Quant Time: Oct 13 23:36:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration




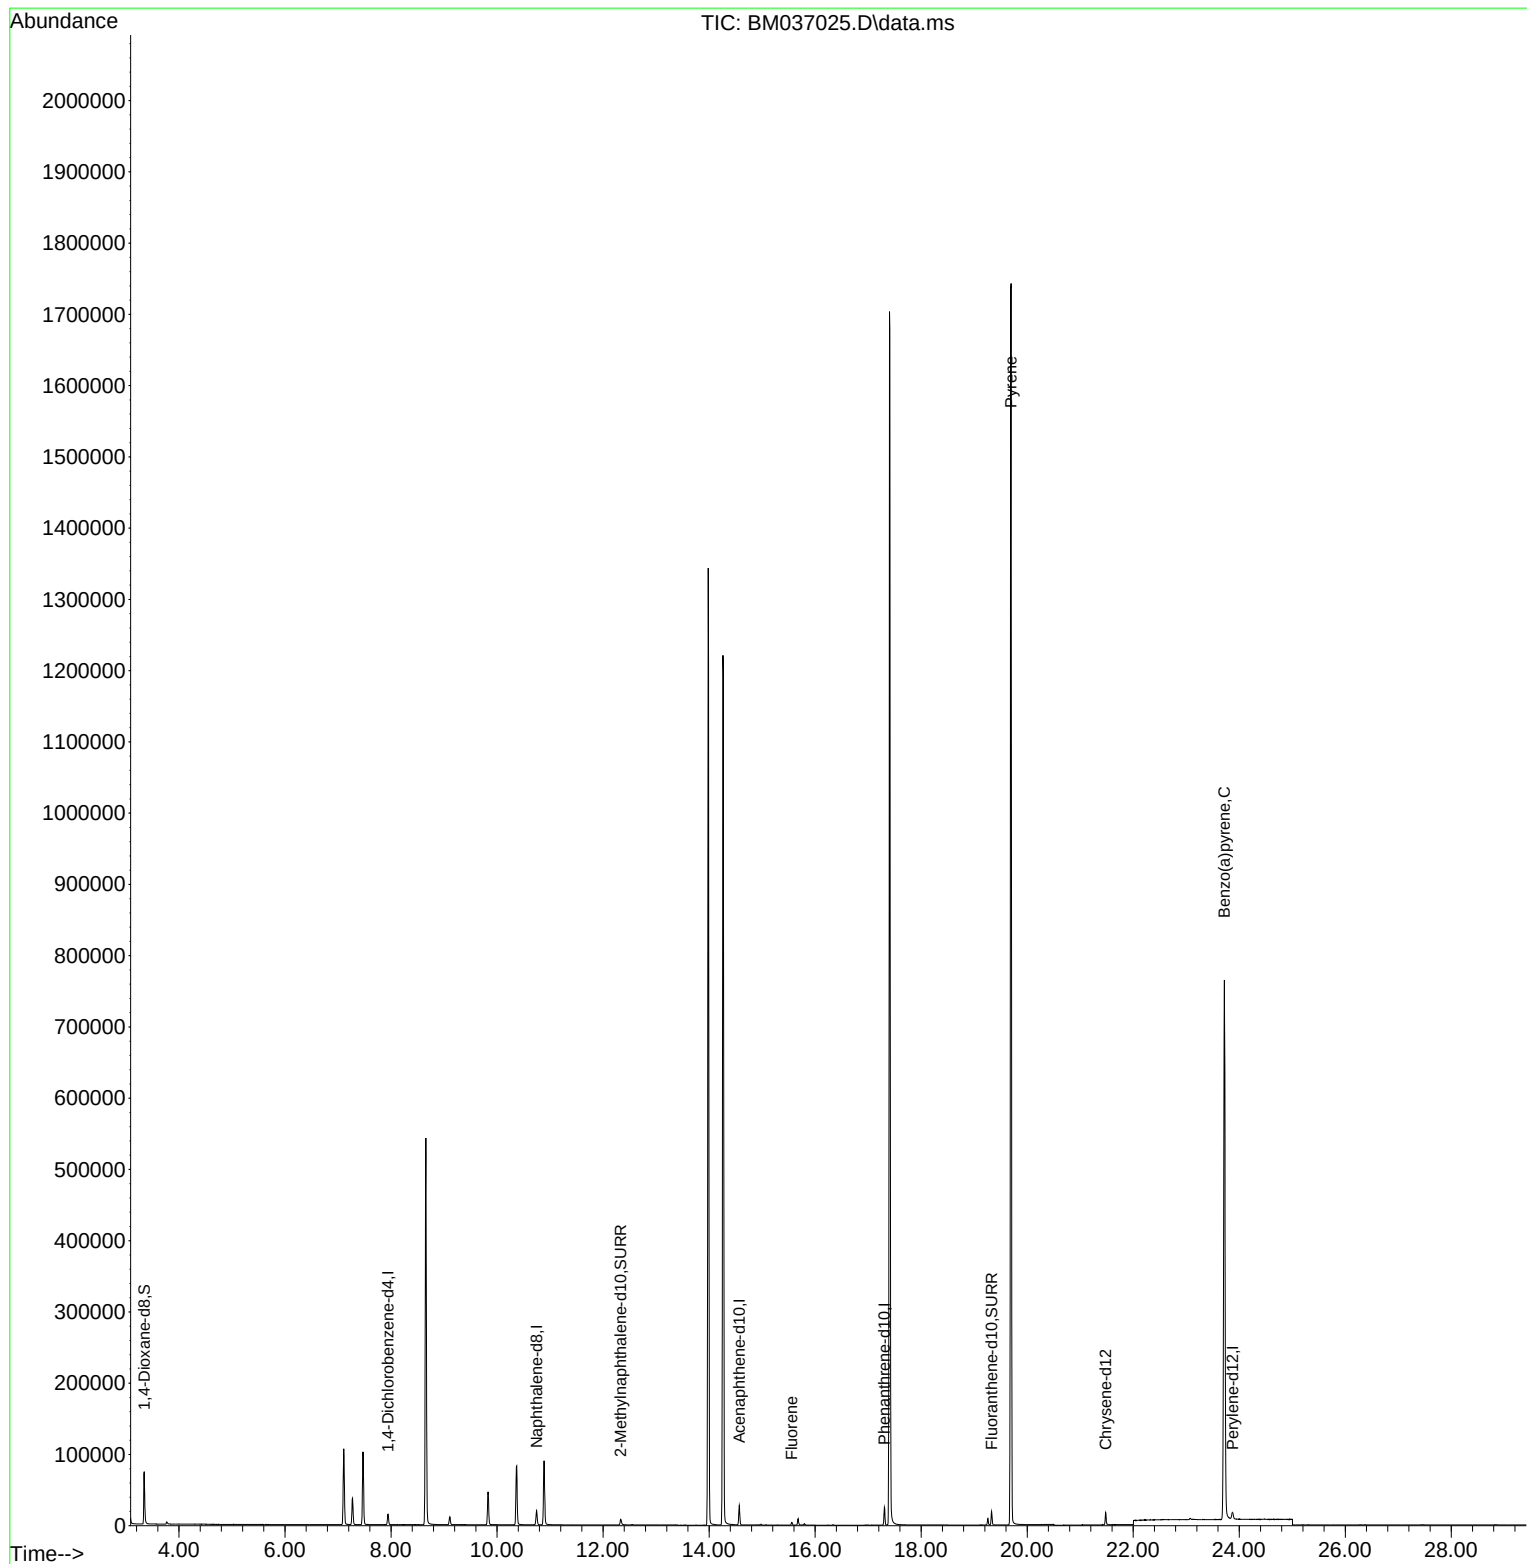


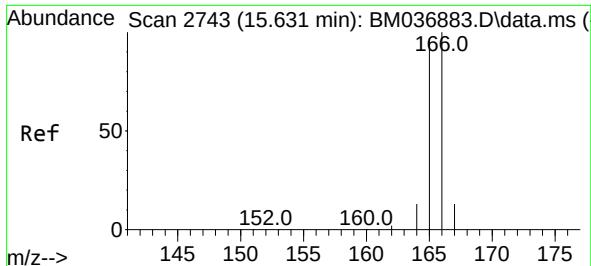

#12
Fluorene
Concen: 0.058 ng/ul
RT: 15.557 min Scan# 21
Delta R.T. -0.064 min
Lab File: BM037025.D
Acq: 13 Oct 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SBLK252


Tgt Ion:166 Resp: 3445
Ion Ratio Lower Upper
166 100
165 8.2 78.9 118.3#
167 30.6 11.3 16.9#

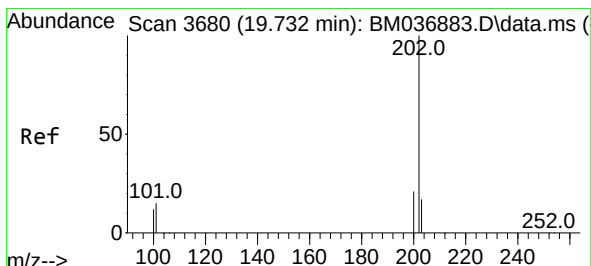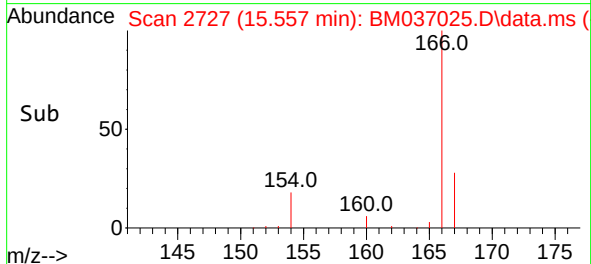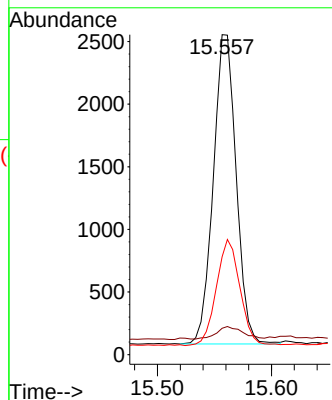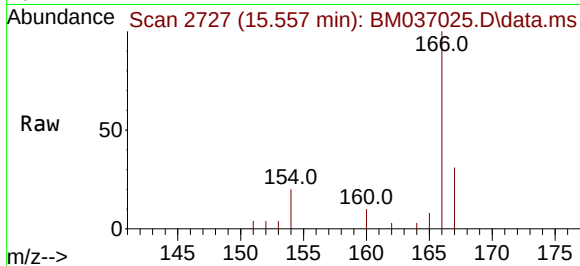

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.694 min Scan# 3672
Delta R.T. -0.032 min
Lab File: BM037025.D
Acq: 13 Oct 2022 20:33


Tgt Ion:202 Resp: 2587
Ion Ratio Lower Upper
202 100
101 157.0 12.0 18.0#
100 1103.3 9.8 14.6#

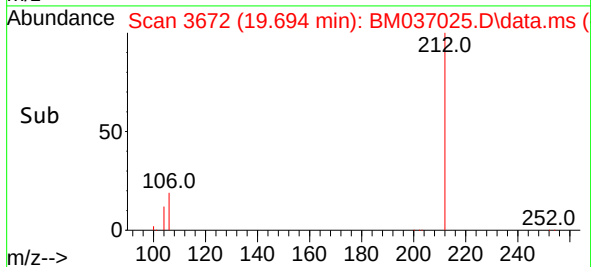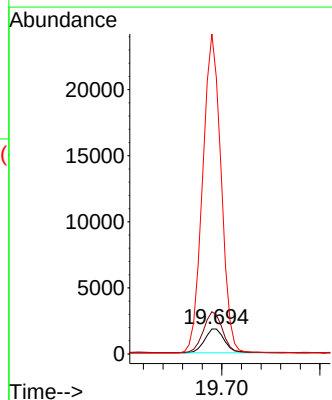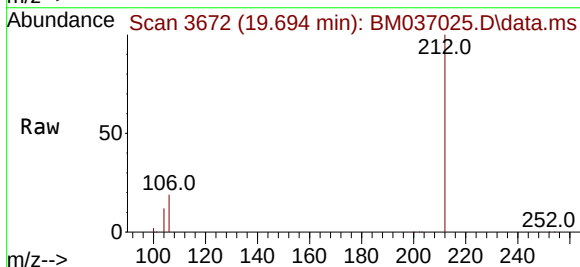

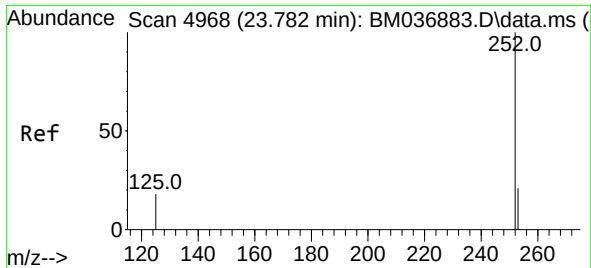

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.718 min Scan# 4946
Delta R.T. -0.053 min
Lab File: BM037025.D
Acq: 13 Oct 2022 20:33

Instrument :
BNA_M
ClientSampleId :
SBLK252

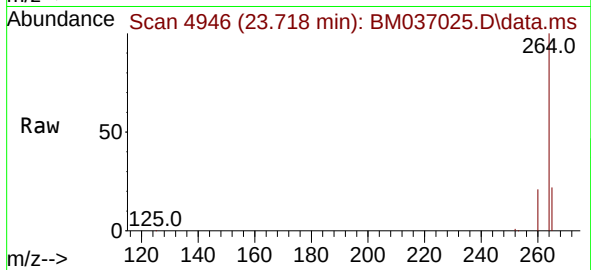

Tgt Ion:252 Resp: 3776
Ion Ratio Lower Upper
252 100
253 58.5 29.7 44.5#
125 68.0 23.6 35.4#

