

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037026.D
 Acq On : 13 Oct 2022 21:09
 Operator : CG/JU
 Sample : PB148291BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK291

Quant Time: Oct 13 23:37:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	6221	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	22699	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.570	164	12377	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.305	188	24189	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240	14793	0.400	ng/ul	0.00
23) Perylene-d12	23.870	264	12642	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	47650	5.431	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	11121	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	19267	0.435	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.560	166	3482	0.069	ng/ul#	14
20) Pyrene	19.694	202	2808	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.715	252	4221	0.092	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037026.D
Acq On : 13 Oct 2022 21:09
Operator : CG/JU
Sample : PB148291BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK291

Quant Time: Oct 13 23:37:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration




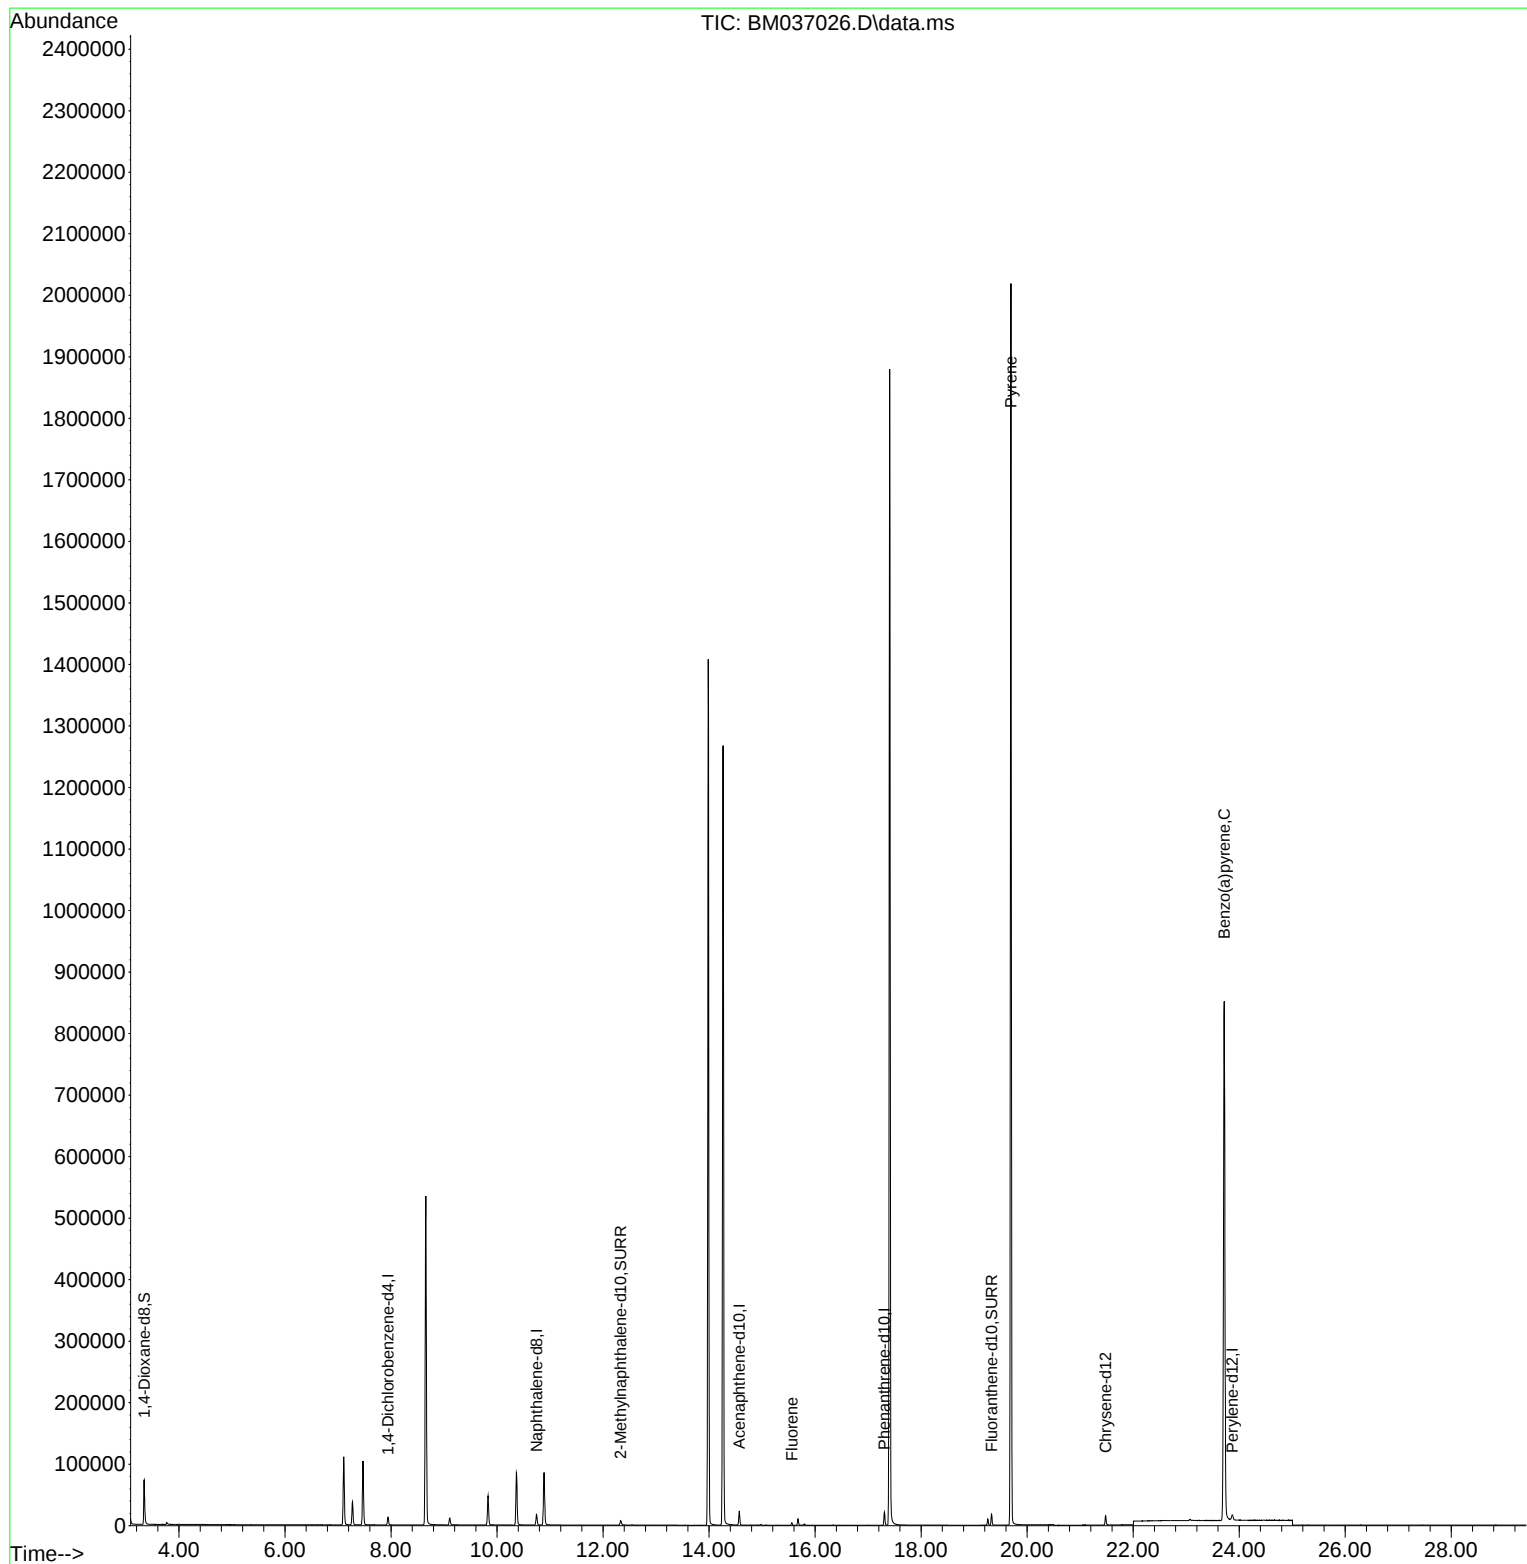


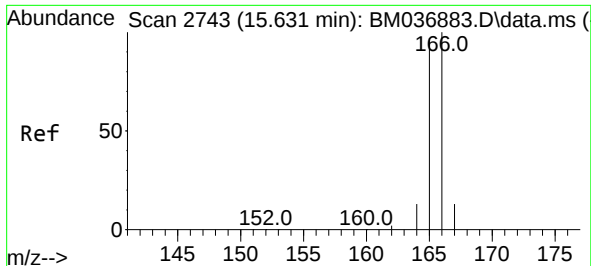

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.560 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM037026.D
Acq: 13 Oct 2022 21:09




Instrument :
BNA_M
ClientSampleId :
SBLK291


Tgt Ion:166 Resp: 3482
Ion Ratio Lower Upper
166 100
165 8.5 78.9 118.3#
167 34.8 11.3 16.9#

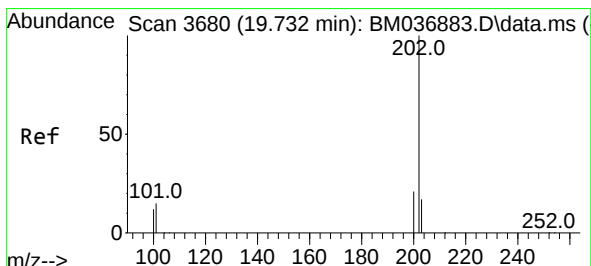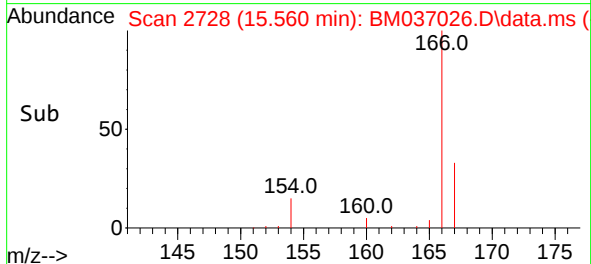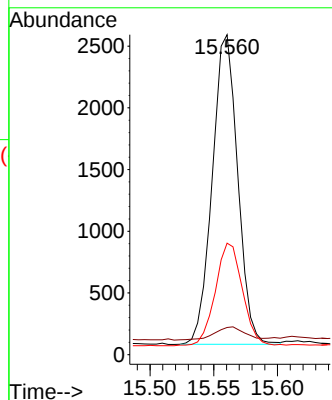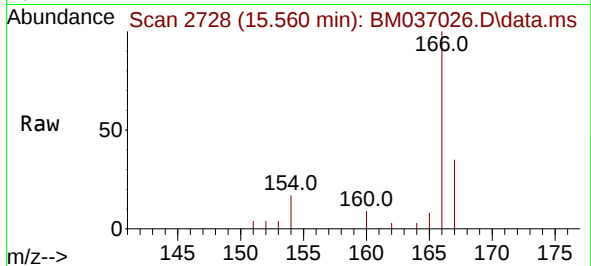

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.694 min Scan# 3672
Delta R.T. -0.032 min
Lab File: BM037026.D
Acq: 13 Oct 2022 21:09


Tgt Ion:202 Resp: 2808
Ion Ratio Lower Upper
202 100
101 157.1 12.0 18.0#
100 1140.2 9.8 14.6#

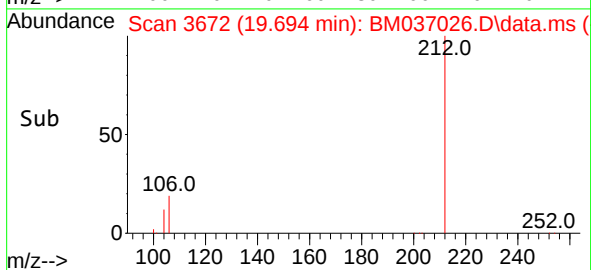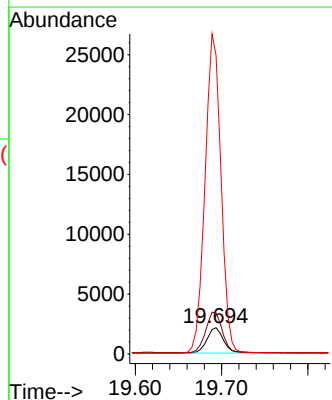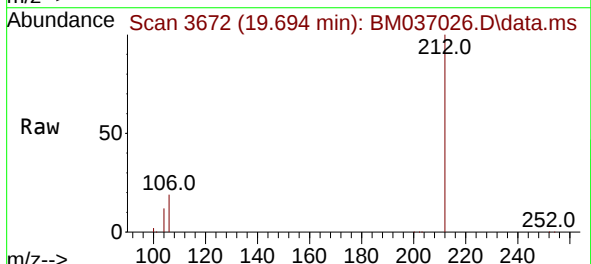

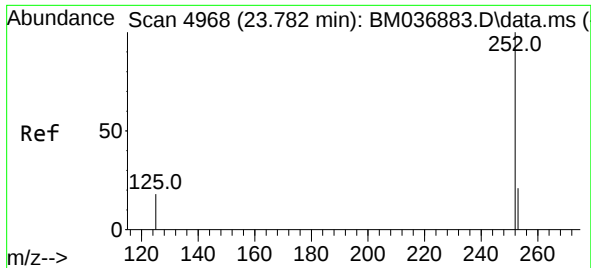

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.715 min Scan# 4945
Delta R.T. -0.055 min
Lab File: BM037026.D
Acq: 13 Oct 2022 21:09

Instrument :
BNA_M
ClientSampleId :
SBLK291

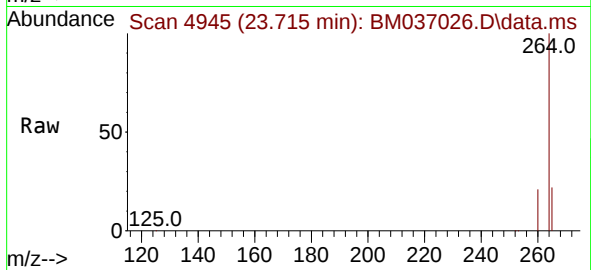

Tgt Ion:252 Resp: 4221
Ion Ratio Lower Upper
252 100
253 56.8 29.7 44.5#
125 63.3 23.6 35.4#

