

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037057.D
 Acq On : 14 Oct 2022 17:19
 Operator : CG/JU
 Sample : PB148218BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK218

Quant Time: Oct 14 23:03:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 14 07:11:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	6352	0.400	ng/ul	0.00
4) Naphthalene-d8	10.736	136	22730	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.560	164	12441	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.299	188	23842	0.400	ng/ul	0.00
17) Chrysene-d12	21.478	240	14099	0.400	ng/ul	0.00
23) Perylene-d12	23.869	264	12482	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	69063	7.710	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.320	152	16216	0.472	ng/ul	0.00
18) Fluoranthene-d10	19.325	212	26827	0.636	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.555	166	4782	0.094	ng/ul#	13
20) Pyrene	19.692	202	3846	0.066	ng/ul#	1
26) Benzo(a)pyrene	23.714	252	5801	0.128	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037057.D
Acq On : 14 Oct 2022 17:19
Operator : CG/JU
Sample : PB148218BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK218

Quant Time: Oct 14 23:03:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 07:11:07 2022
Response via : Initial Calibration




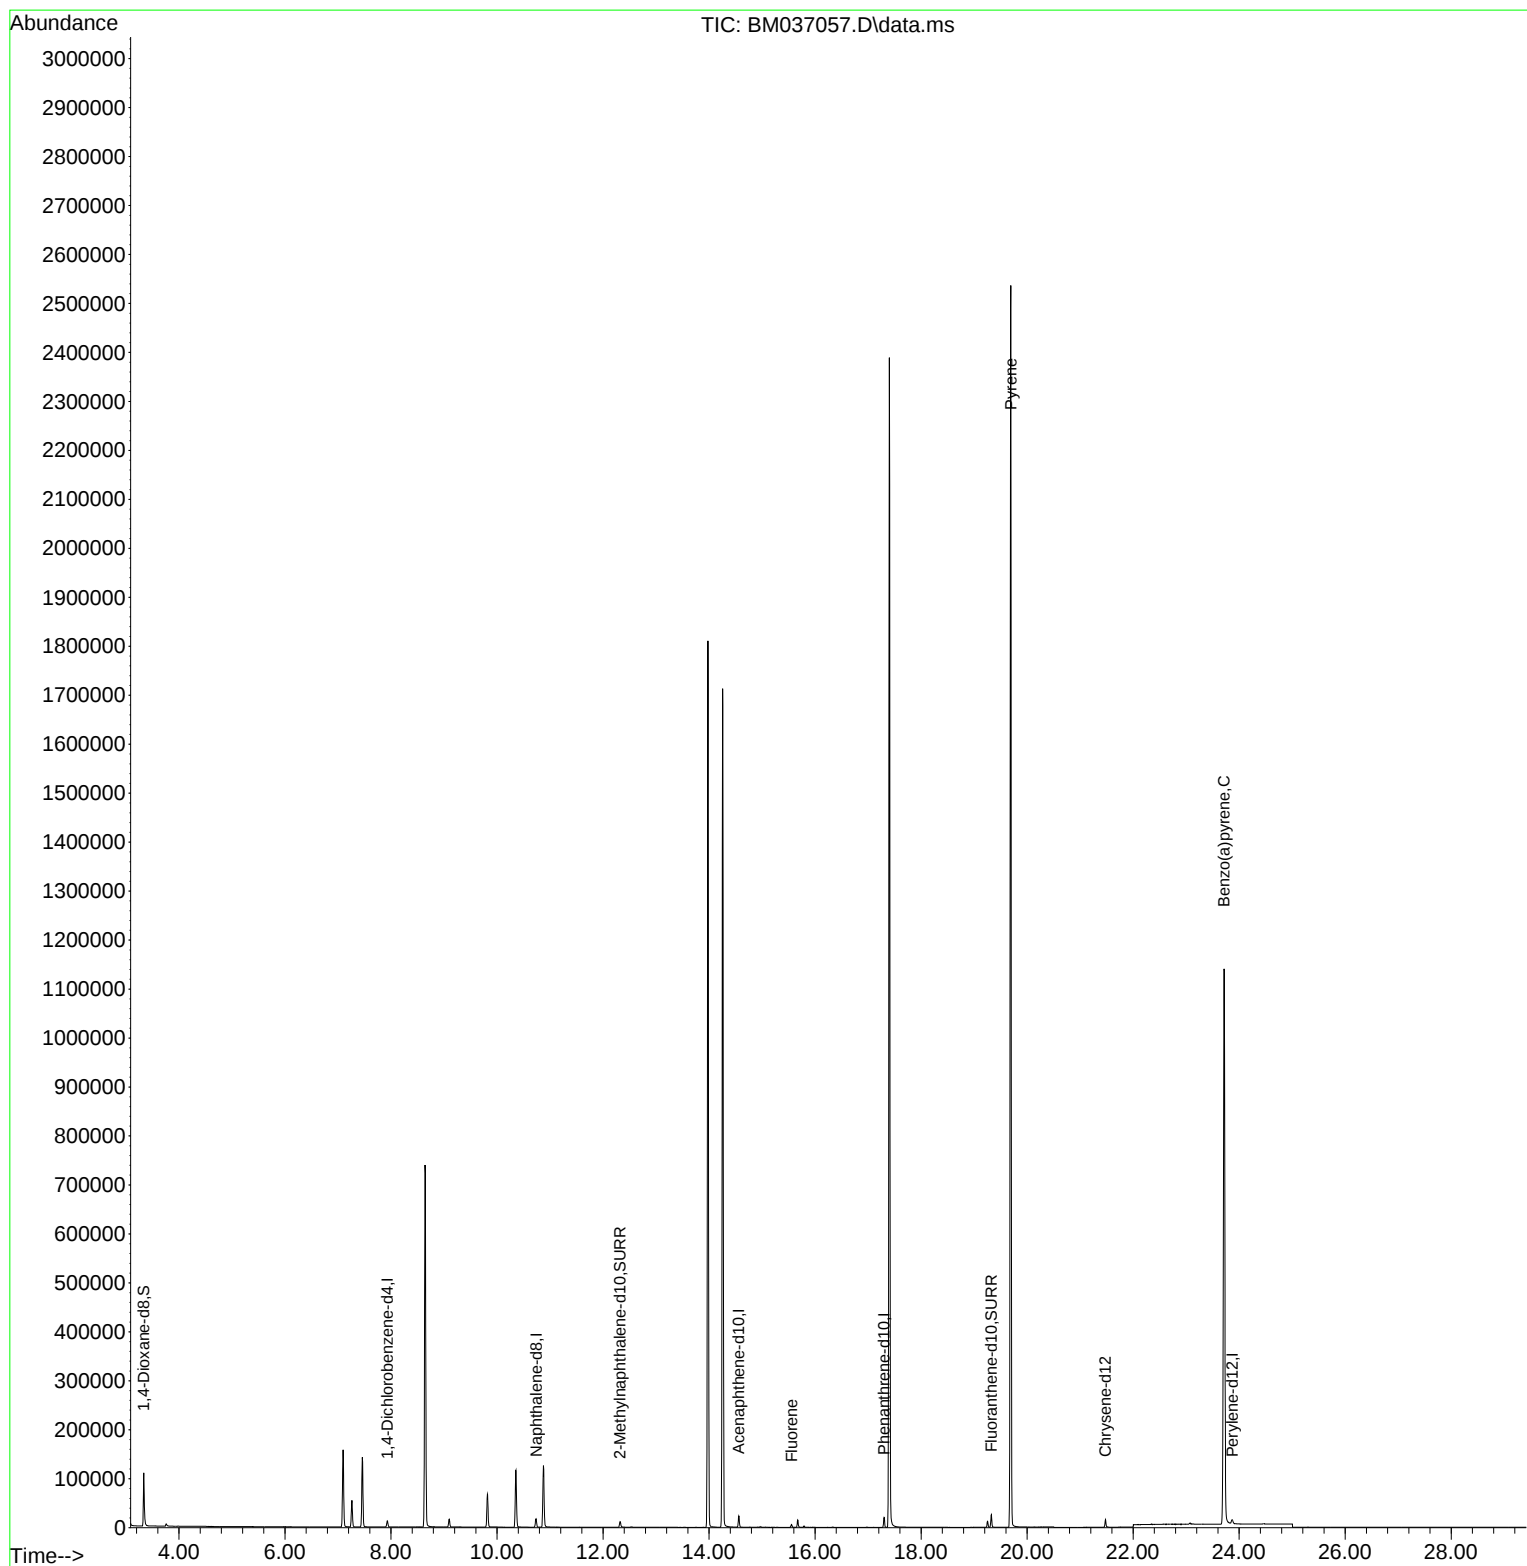


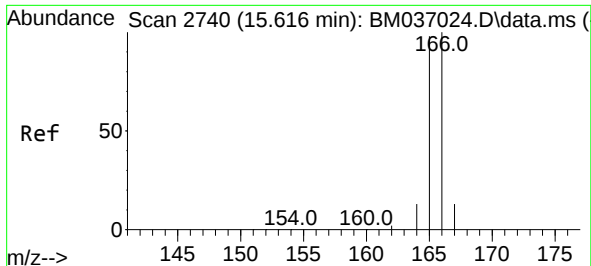

#12
Fluorene
Concen: 0.094 ng/ul
RT: 15.555 min Scan# 21
Delta R.T. -0.053 min
Lab File: BM037057.D
Acq: 14 Oct 2022 17:19




Instrument :
BNA_M
ClientSampleId :
SBLK218


Tgt Ion:166 Resp: 4782
Ion Ratio Lower Upper
166 100
165 6.9 78.9 118.3#
167 32.8 11.3 16.9#

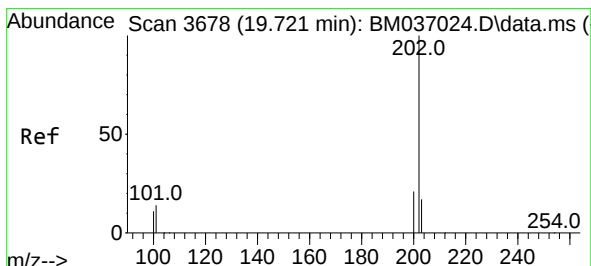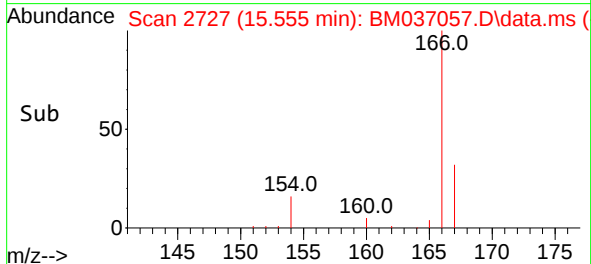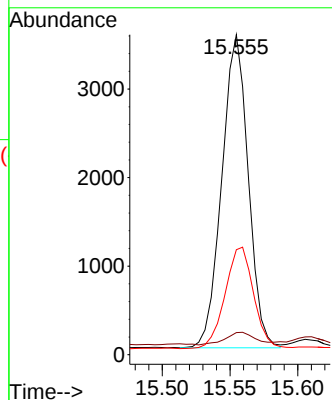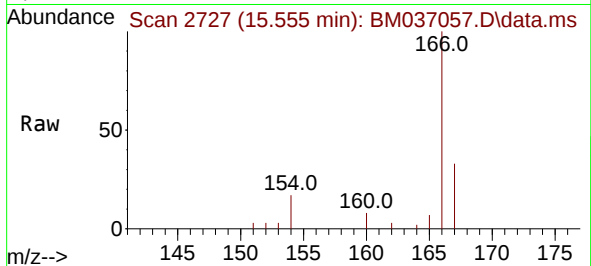

#20
Pyrene
Concen: 0.066 ng/ul
RT: 19.692 min Scan# 3672
Delta R.T. -0.026 min
Lab File: BM037057.D
Acq: 14 Oct 2022 17:19


Tgt Ion:202 Resp: 3846
Ion Ratio Lower Upper
202 100
101 163.0 12.0 18.0#
100 1153.0 9.8 14.6#

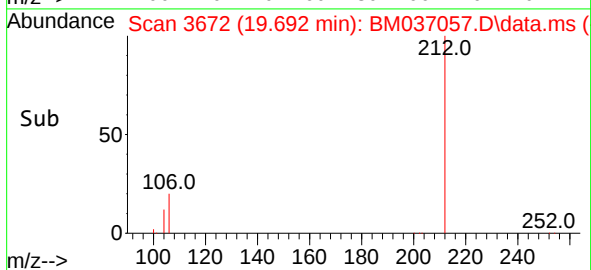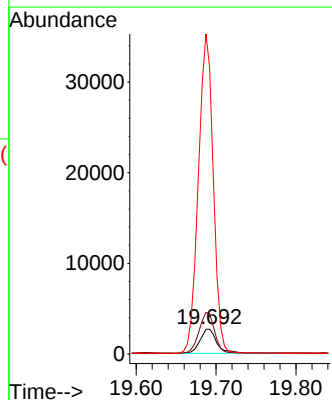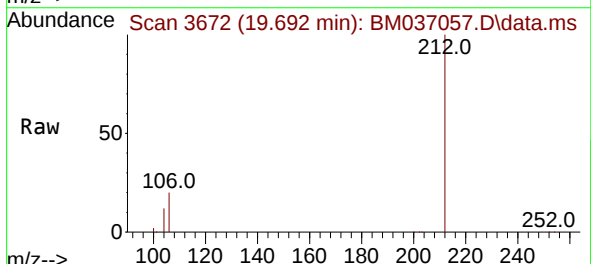

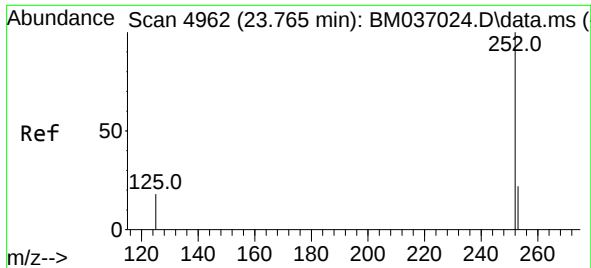

#26
 Benzo(a)pyrene
 Concen: 0.128 ng/ul
 RT: 23.714 min Scan# 4962
 Delta R.T. -0.044 min
 Lab File: BM037057.D
 Acq: 14 Oct 2022 17:19

Instrument :
 BNA_M
 ClientSampleId :
 SBLK218

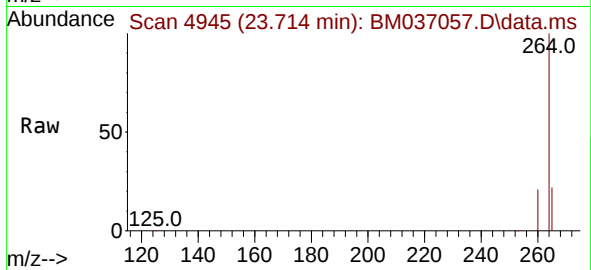

Tgt Ion:252 Resp: 5801
 Ion Ratio Lower Upper
 252 100
 253 46.8 29.7 44.5#
 125 54.1 23.6 35.4#

