

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037092.D
 Acq On : 15 Oct 2022 15:11
 Operator : CG/JU
 Sample : PB148218BL
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK218

Quant Time: Oct 17 00:56:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 15 04:13:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5007	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	17786	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.557	164	9412	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	17740	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	10274	0.400	ng/ul	0.00
23) Perylene-d12	23.856	264	9570	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.335	96	40185	5.691	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	9447	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	14651	0.477	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.547	166	2706	0.070	ng/ul#	15
20) Pyrene	19.684	202	2326	0.055	ng/ul#	1
26) Benzo(a)pyrene	23.701	252	3278	0.095	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037092.D
Acq On : 15 Oct 2022 15:11
Operator : CG/JU
Sample : PB148218BL
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK218

Quant Time: Oct 17 00:56:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 15 04:13:53 2022
Response via : Initial Calibration




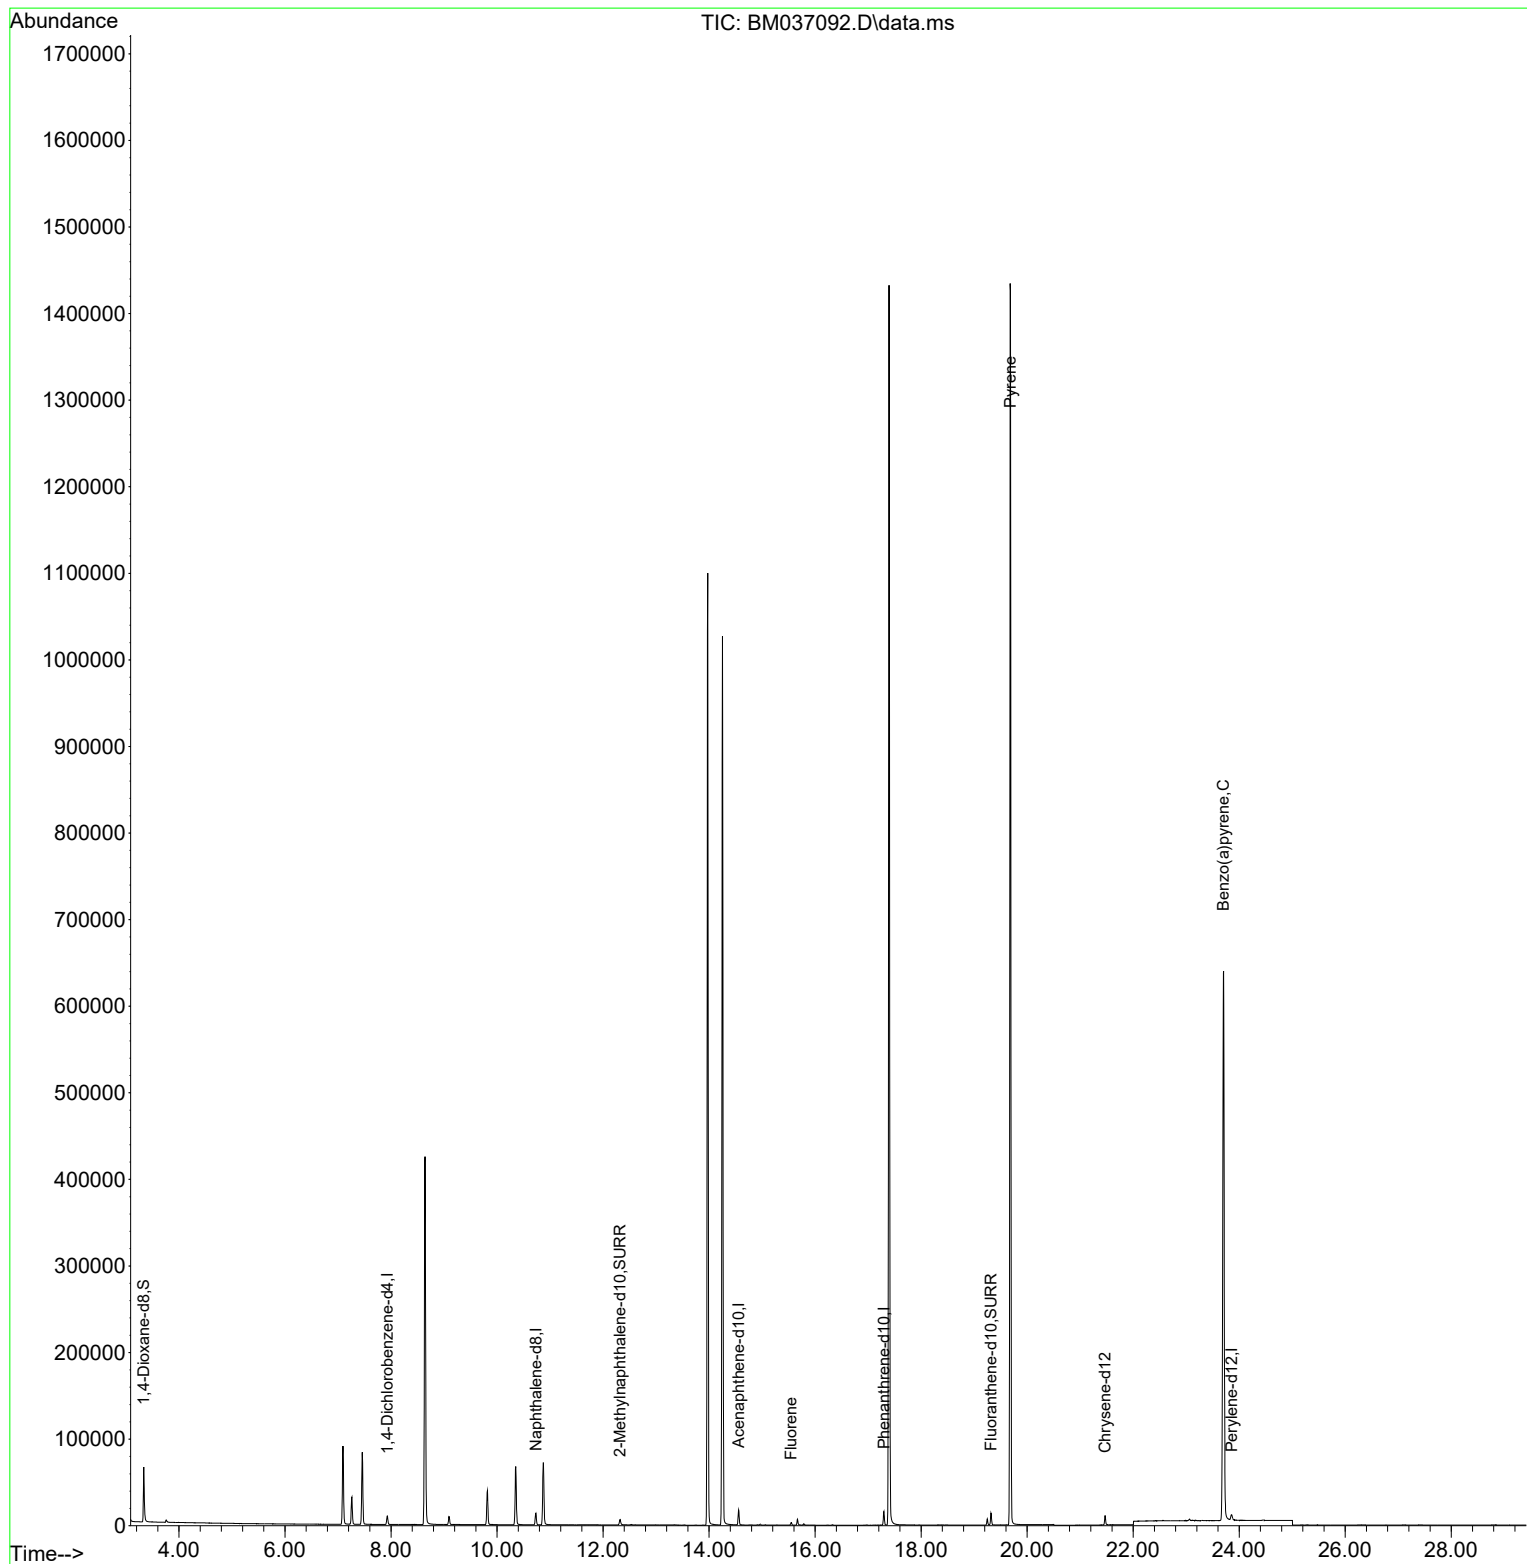


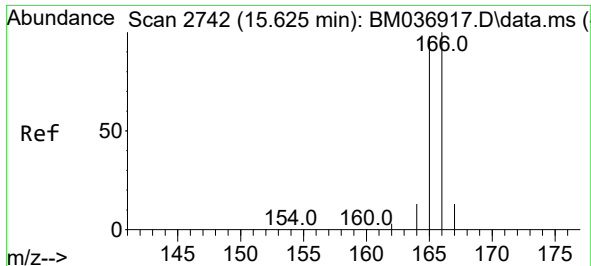

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.547 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM037092.D
Acq: 15 Oct 2022 15:11




Instrument :
BNA_M
ClientSampleId :
SBLK218


Tgt Ion:166 Resp: 2706
Ion Ratio Lower Upper
166 100
165 8.5 78.9 118.3#
167 31.2 11.3 16.9#

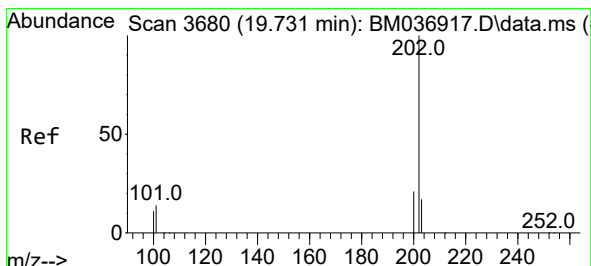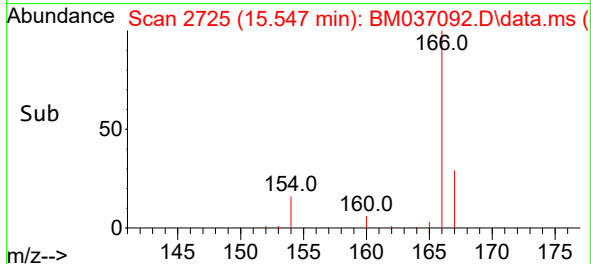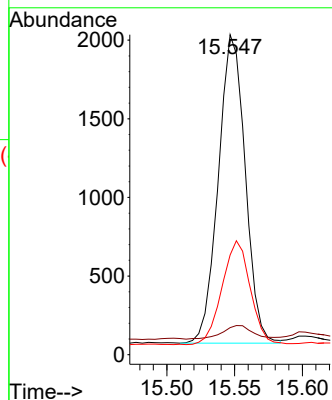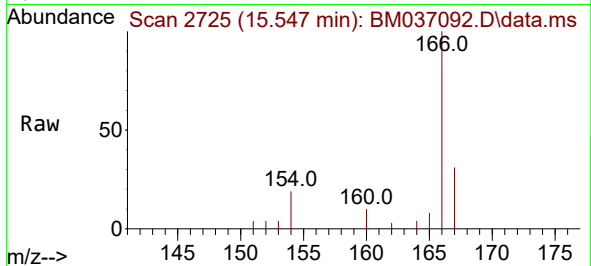

#20
Pyrene
Concen: 0.055 ng/ul
RT: 19.684 min Scan# 3670
Delta R.T. -0.023 min
Lab File: BM037092.D
Acq: 15 Oct 2022 15:11


Tgt Ion:202 Resp: 2326
Ion Ratio Lower Upper
202 100
101 156.7 12.0 18.0#
100 1109.5 9.8 14.6#

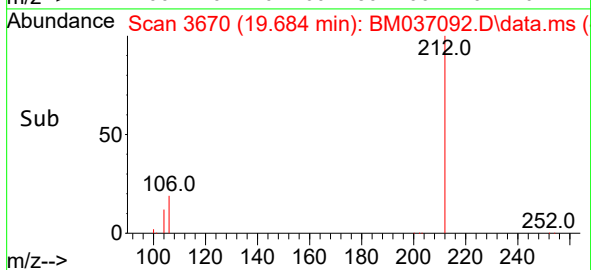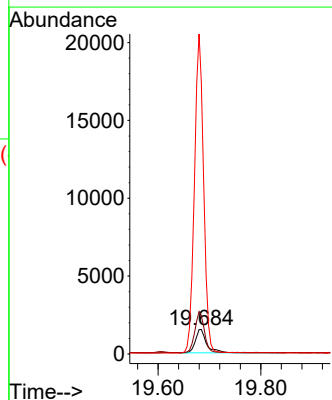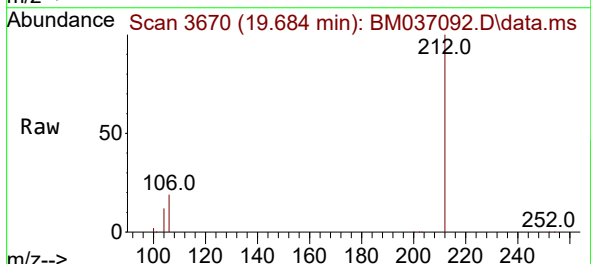

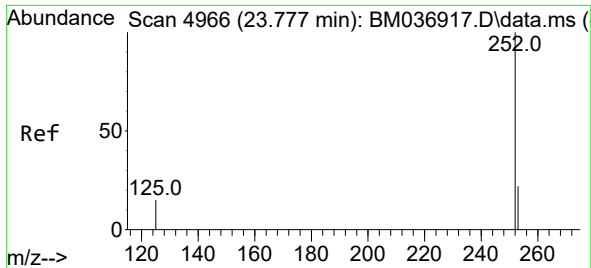

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.701 min Scan# 4940
Delta R.T. -0.044 min
Lab File: BM037092.D
Acq: 15 Oct 2022 15:11

Instrument :
BNA_M
ClientSampleId :
SBLK218

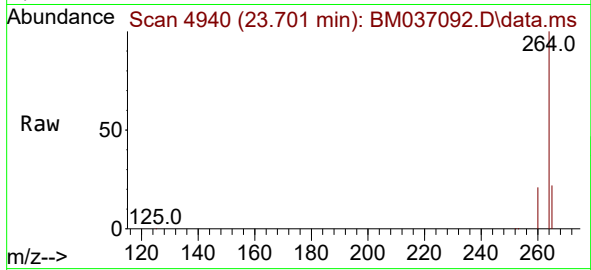

Tgt Ion:252 Resp: 3278
Ion Ratio Lower Upper
252 100
253 53.2 29.7 44.5#
125 63.0 23.6 35.4#

