




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037018.D
 Acq On : 13 Oct 2022 15:44
 Operator : CG/JU
 Sample : N4976-07DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 13 23:34:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/14/2022
 Supervised By :mohammad ahmed 10/16/2022

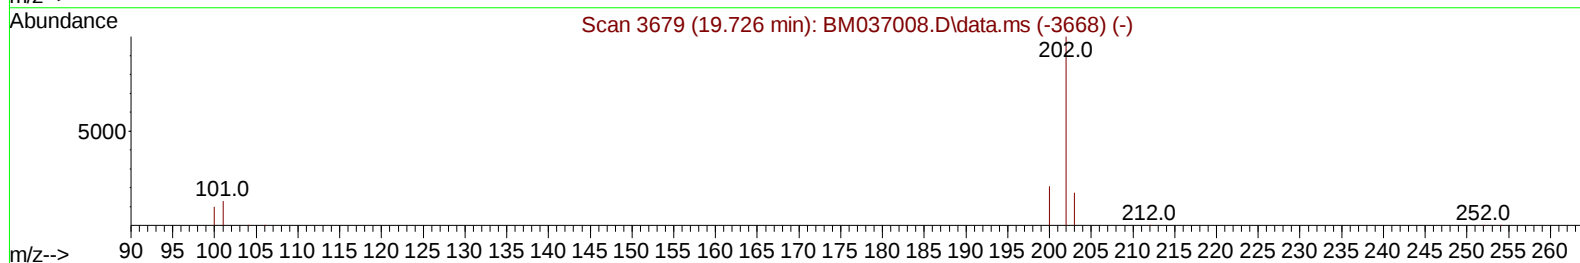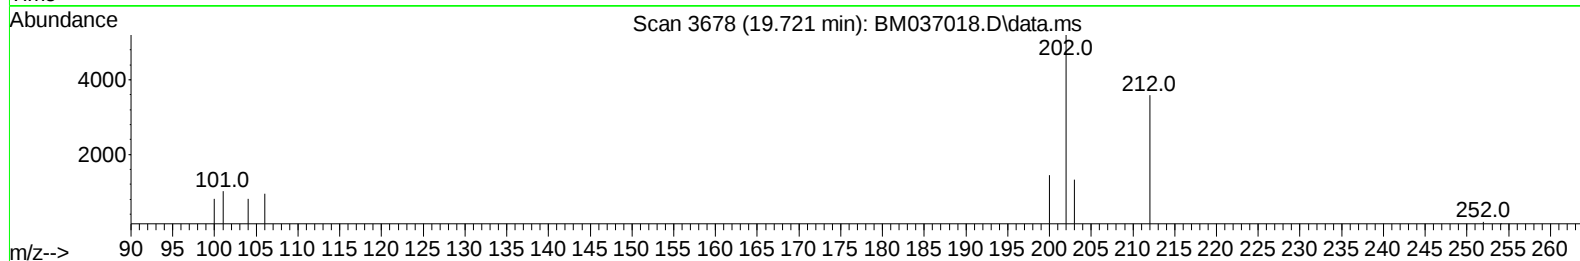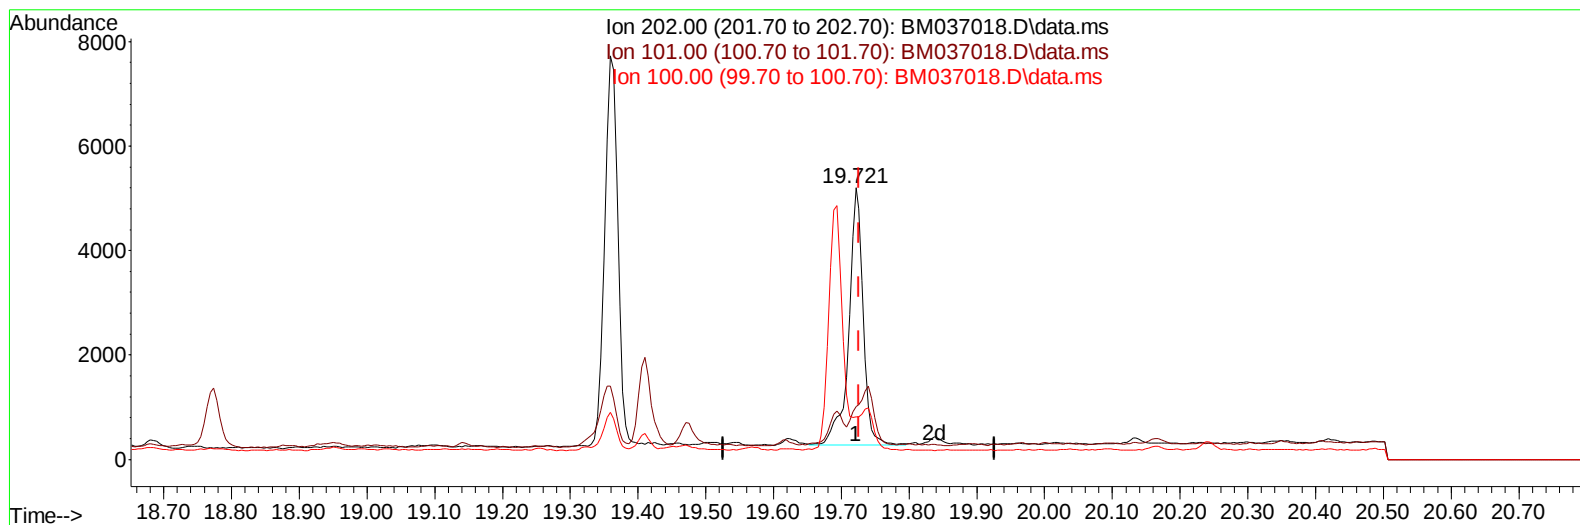

TIC: BM037018.D\data.ms

(20) Pyrene

19.721min (-0.005) 0.09 ng/u1

response 7405

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	19.52#
100.00	12.20	15.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037018.D
 Acq On : 13 Oct 2022 15:44
 Operator : CG/JU
 Sample : N4976-07DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 13 23:34:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/14/2022
 Supervised By :mohammad ahmed 10/16/2022

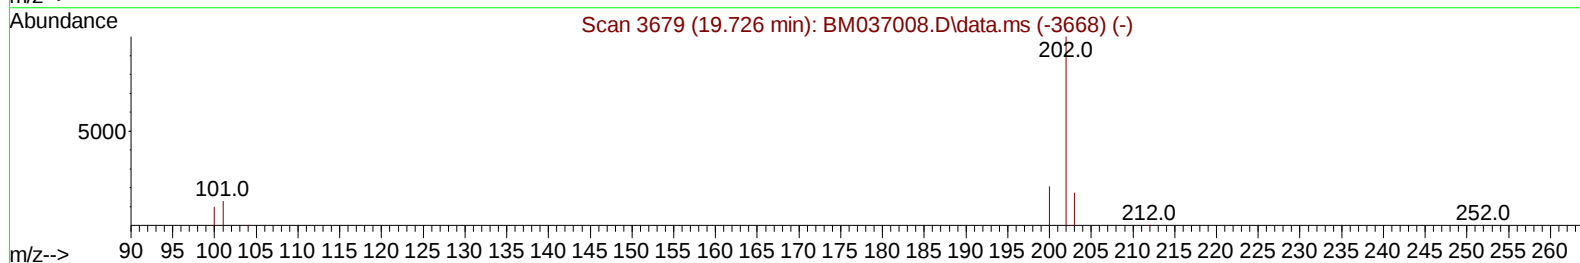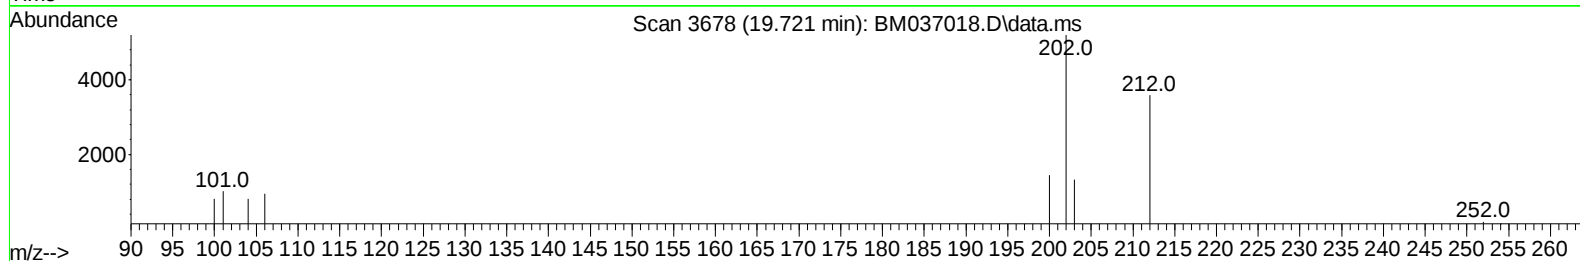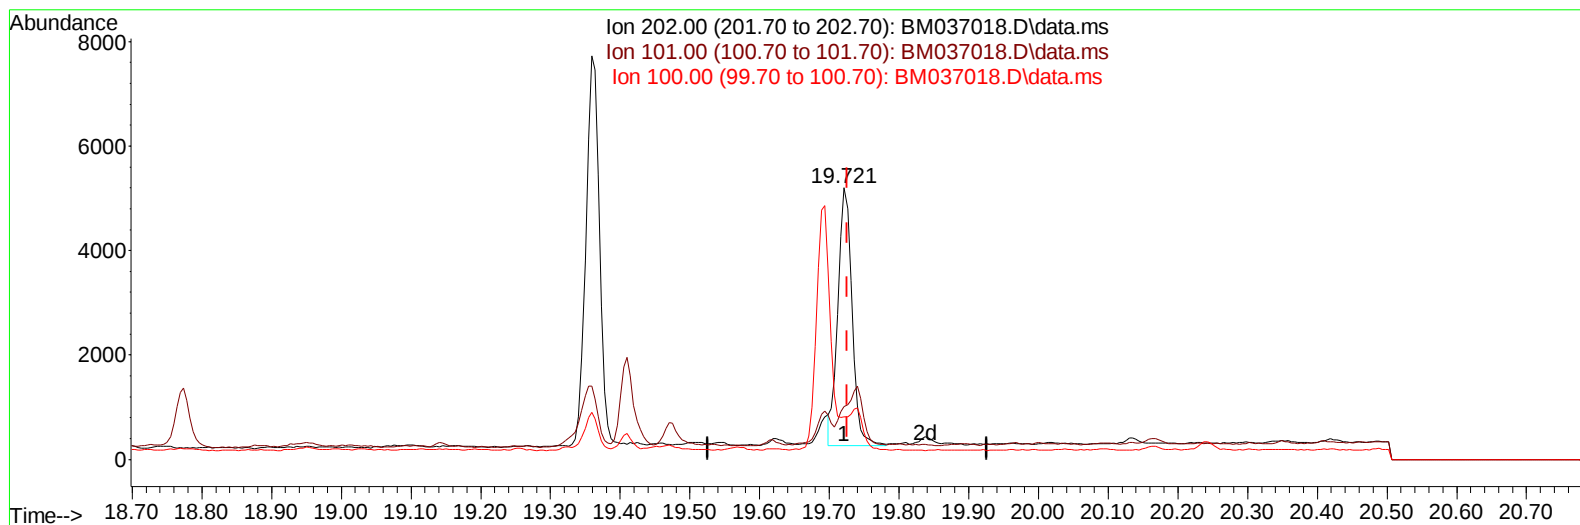

TIC: BM037018.D\data.ms

(20) Pyrene

19.721min (-0.005) 0.09 ng/ul m

response 6828

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	19.52#
100.00	12.20	15.73#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037018.D
 Acq On : 13 Oct 2022 15:44
 Operator : CG/JU
 Sample : N4976-07DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Y3DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/14/2022
 Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 13 23:34:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.943	152		7429	0.400	ng/ul	0.00
4) Naphthalene-d8	10.749	136		27463	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.570	164		15371	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188		30852	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240		18836	0.400	ng/ul	0.00
23) Perylene-d12	23.876	264		14267	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.344	96		3480	0.332	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152		1890	0.046	ng/ul	0.00
18) Fluoranthene-d10	19.331	212		3912	0.069	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.798	128		5940	0.076	ng/ul#	94
7) 2-Methylnaphthalene	12.404	142		1601	0.033	ng/ul	91
8) 1-Methylnaphthalene	12.624	142		2752	0.056	ng/ul	99
10) Acenaphthylene	14.293	152		1712	0.027	ng/ul#	24
11) Acenaphthene	14.631	153		110663	1.996	ng/ul	98
12) Fluorene	15.616	166		63476	1.010	ng/ul	98
15) Phenanthrene	17.351	178		19169	0.195	ng/ul	97
16) Anthracene	17.440	178		10524	0.128	ng/ul	93
19) Fluoranthene	19.359	202		10117	0.135	ng/ul#	90
20) Pyrene	19.721	202		6828m	0.087	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037018.D
Acq On : 13 Oct 2022 15:44
Operator : CG/JU
Sample : N4976-07DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Y3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 13 23:34:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/14/2022
Supervised By :mohammad ahmed 10/16/2022

