

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101322\  
 Data File : BM037048.D  
 Acq On : 14 Oct 2022 10:44  
 Operator : CG/JU  
 Sample : N4984-12  
 Misc :  
 ALS Vial : 43 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BGNM1

Quant Time: Oct 14 23:01:28 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM100622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Oct 14 07:11:07 2022  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|--------|------|----------|-------|---------|----------|
| -----                       |        |      |          |       |         |          |
| Internal Standards          |        |      |          |       |         |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.934  | 152  | 4372     | 0.400 | ng/ul   | 0.00     |
| 4) Naphthalene-d8           | 10.738 | 136  | 15788    | 0.400 | ng/ul # | 0.00     |
| 9) Acenaphthene-d10         | 14.561 | 164  | 9081     | 0.400 | ng/ul   | 0.00     |
| 13) Phenanthrene-d10        | 17.301 | 188  | 16140    | 0.400 | ng/ul   | 0.00     |
| 17) Chrysene-d12            | 21.474 | 240  | 8445     | 0.400 | ng/ul # | 0.00     |
| 23) Perylene-d12            | 23.862 | 264  | 8032     | 0.400 | ng/ul   | 0.00     |
| System Monitoring Compounds |        |      |          |       |         |          |
| 3) 1,4-Dioxane-d8           | 3.340  | 96   | 39893    | 6.470 | ng/ul   | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.322 | 152  | 13018    | 0.546 | ng/ul   | 0.00     |
| 18) Fluoranthene-d10        | 19.322 | 212  | 20658    | 0.818 | ng/ul   | 0.00     |
| Target Compounds            |        |      |          |       |         |          |
|                             |        |      |          |       | Qvalue  |          |
| 5) Naphthalene              | 10.787 | 128  | 1387     | 0.031 | ng/ul#  | 81       |
| -----                       |        |      |          |       |         |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101322\  
Data File : BM037048.D  
Acq On : 14 Oct 2022 10:44  
Operator : CG/JU  
Sample : N4984-12  
Misc :  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BGNM1


Quant Time: Oct 14 23:01:28 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM100622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 14 07:11:07 2022  
Response via : Initial Calibration

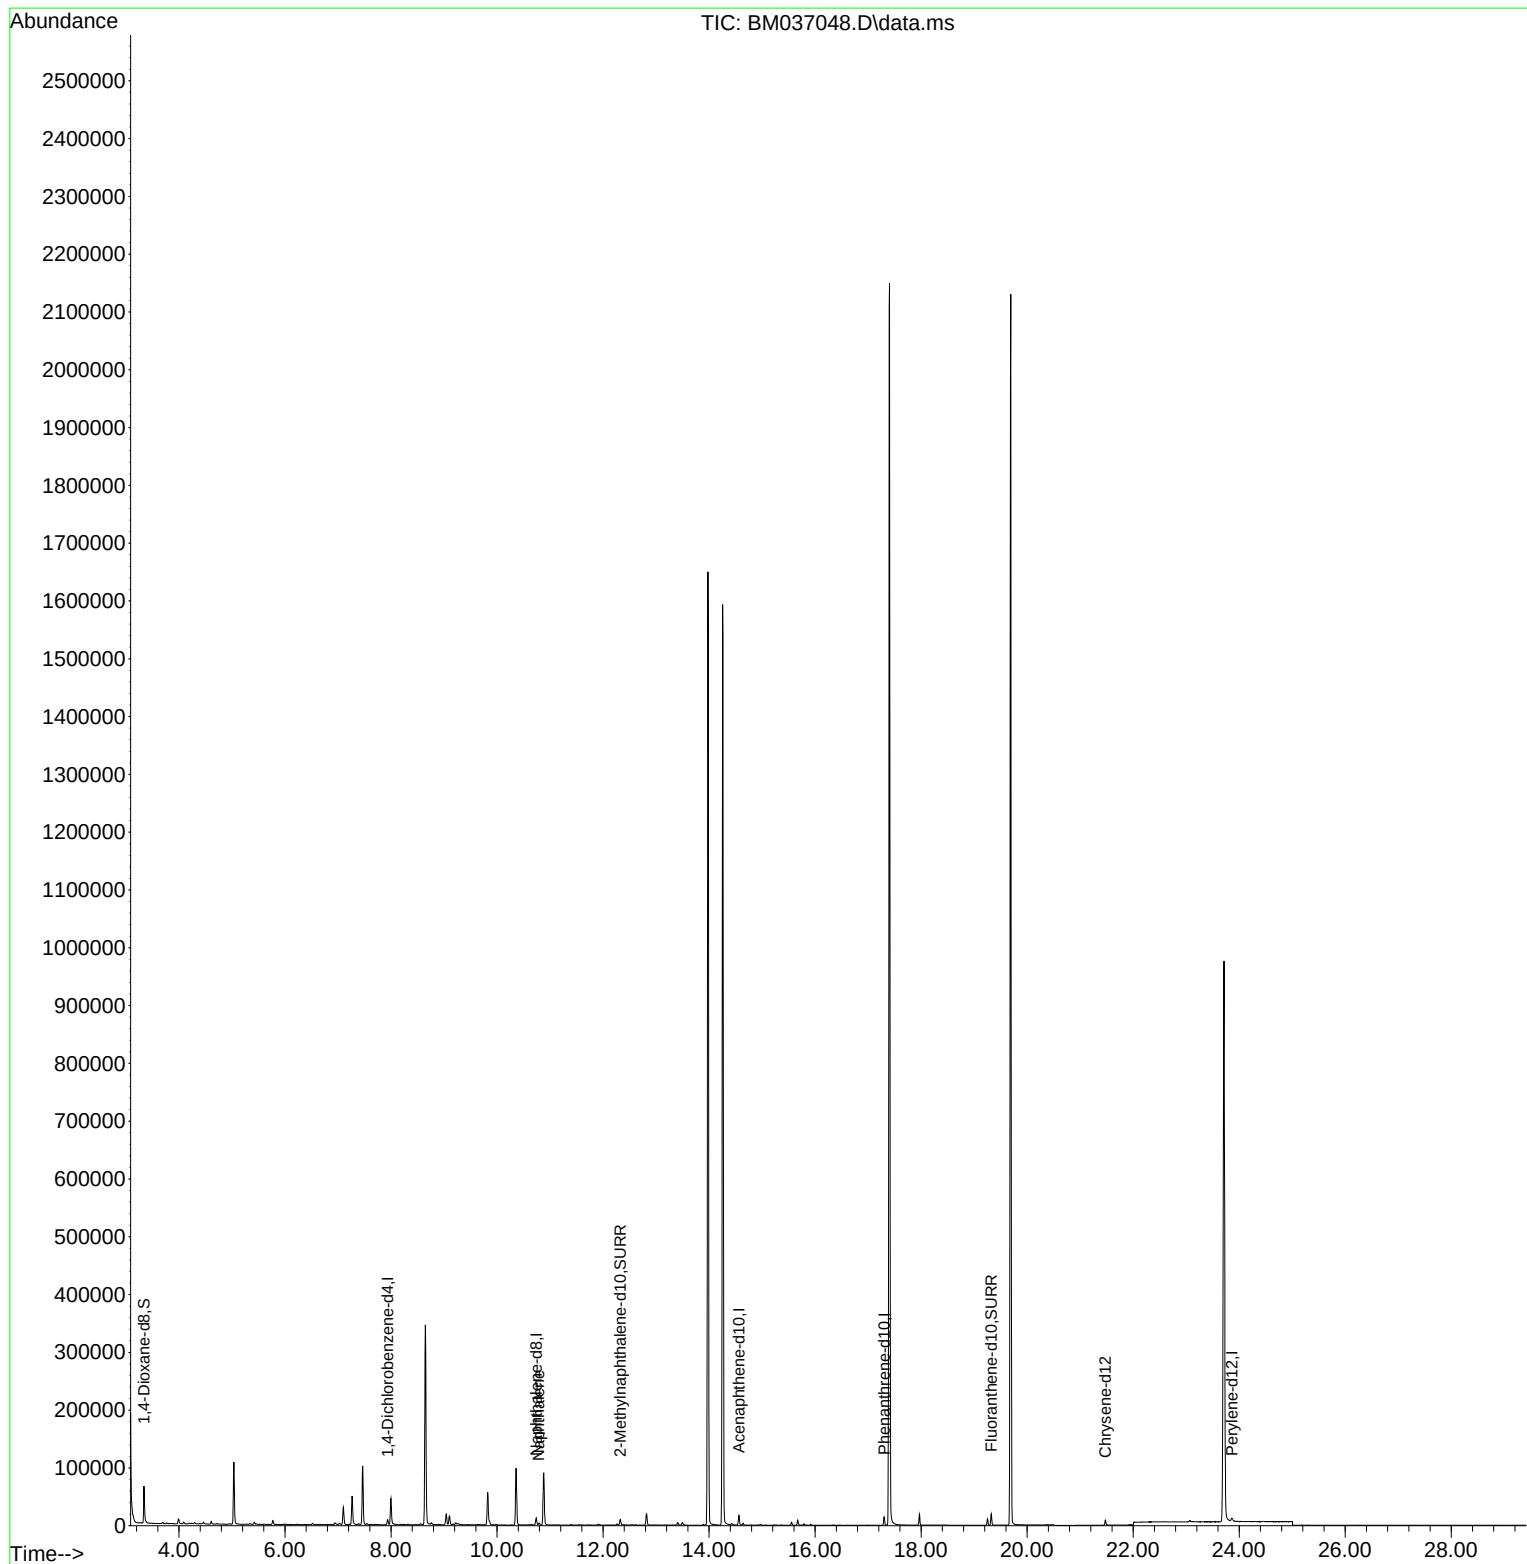

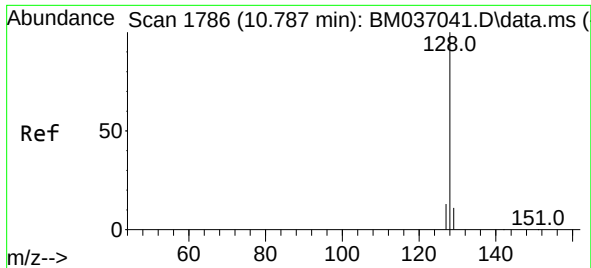

#5  
Naphthalene  
Concen: 0.031 ng/ul  
RT: 10.787 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: BM037048.D  
Acq: 14 Oct 2022 10:44

Instrument :  
BNA\_M  
ClientSampleId :  
BGNM1

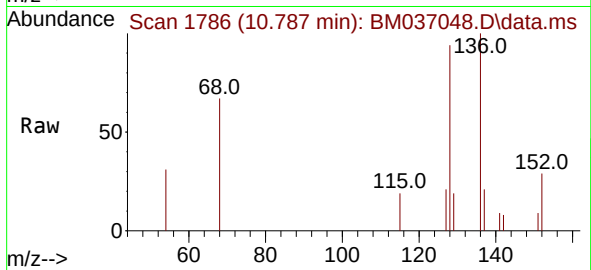

Tgt Ion:128 Resp: 1387  
Ion Ratio Lower Upper  
128 100  
129 20.2 10.2 15.2#  
127 22.5 11.7 17.5#

