

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037049.D
 Acq On : 14 Oct 2022 11:19
 Operator : CG/JU
 Sample : N4984-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGNM4

Quant Time: Oct 14 23:01:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 14 07:11:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	5909	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	21551	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.561	164	11727	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.301	188	21679	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	12100	0.400	ng/ul	0.00
23) Perylene-d12	23.864	264	10775	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	33979	4.078	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	9807	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	17869	0.494	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.787	128	3770	0.061	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037049.D
Acq On : 14 Oct 2022 11:19
Operator : CG/JU
Sample : N4984-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGNM4


Quant Time: Oct 14 23:01:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 07:11:07 2022
Response via : Initial Calibration

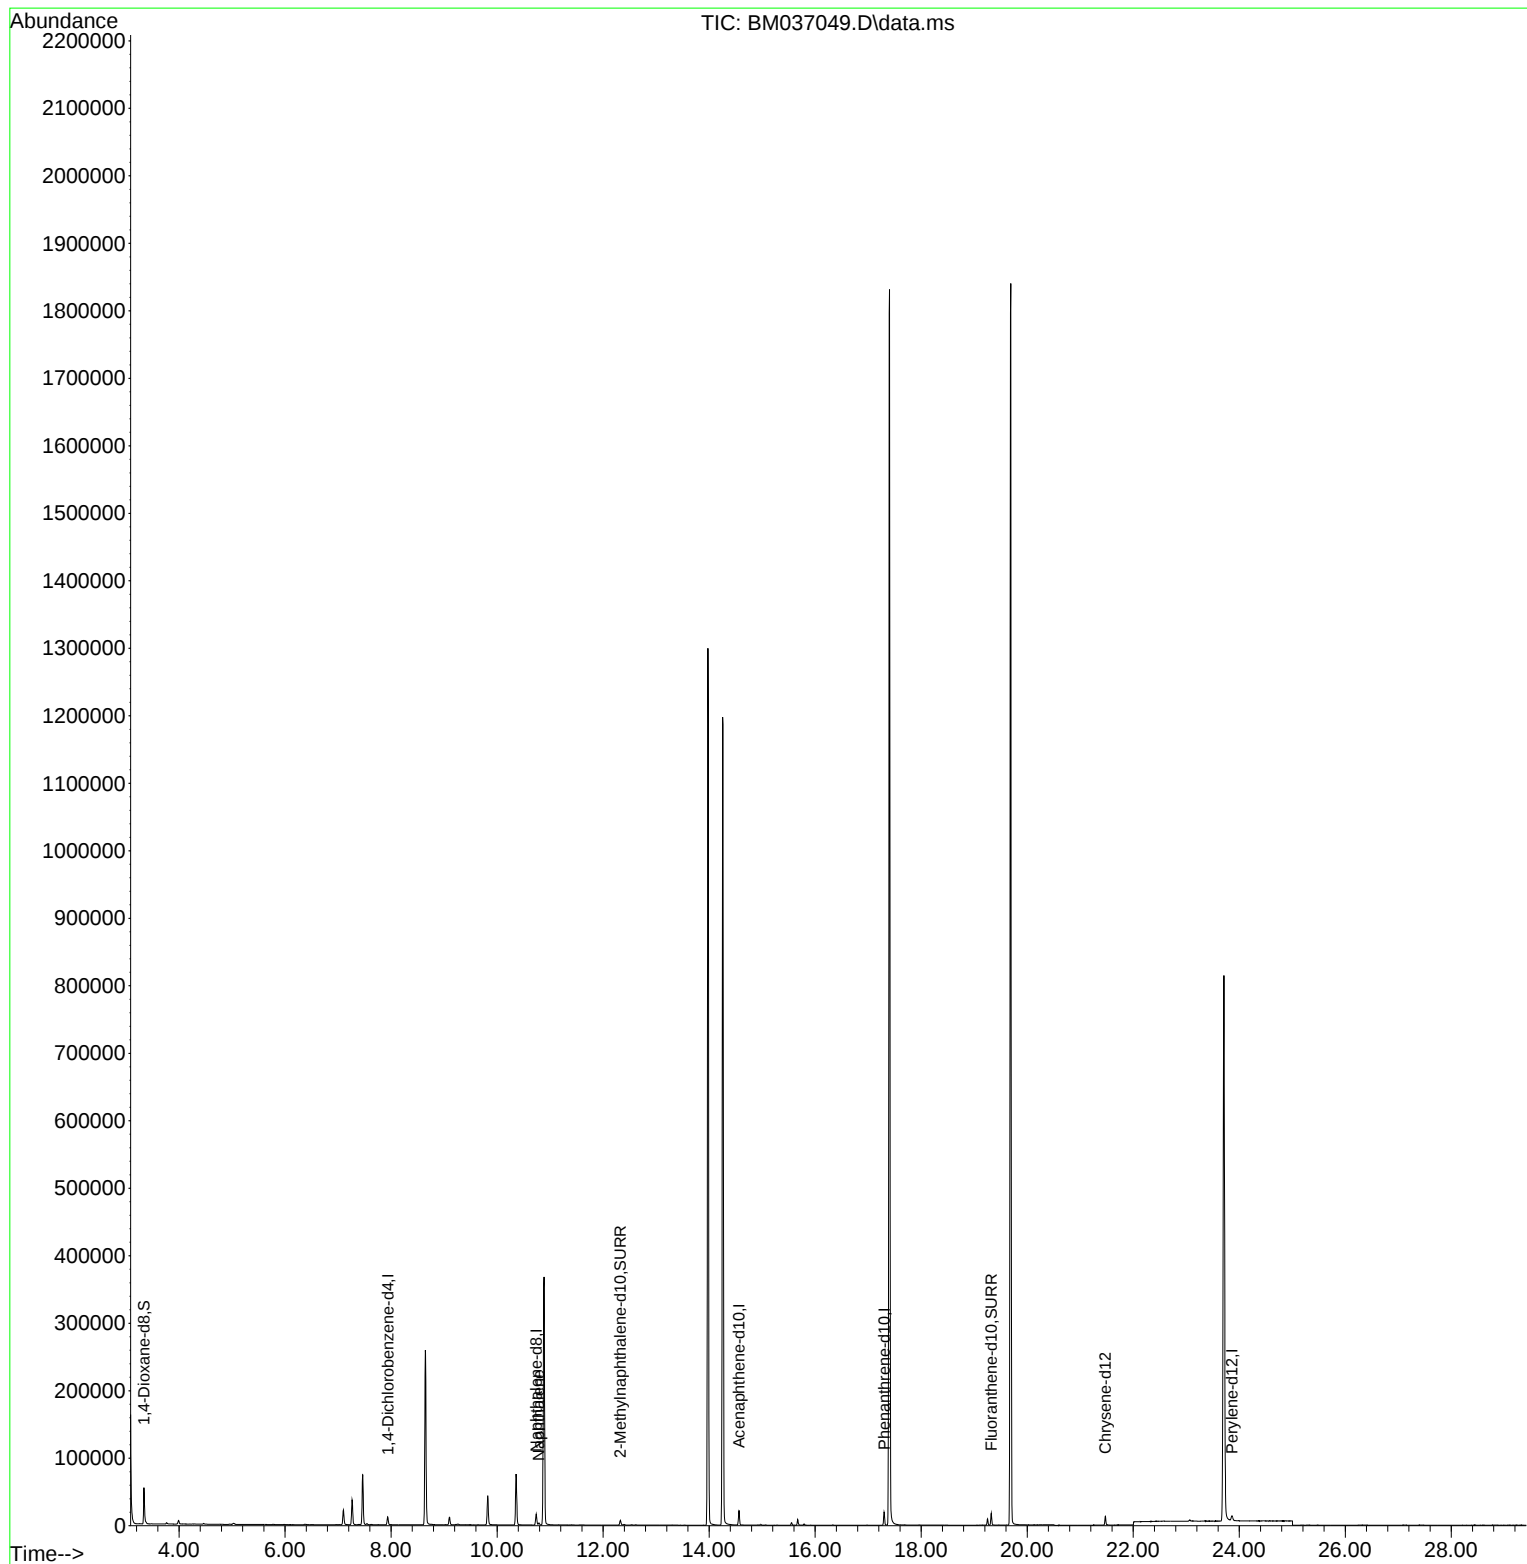

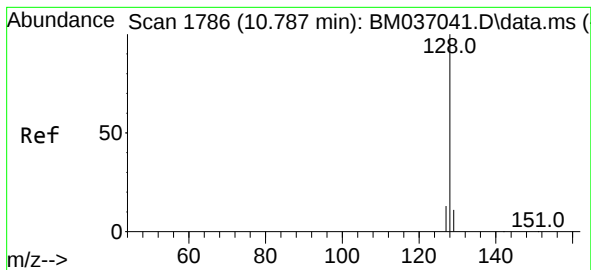

#5
Naphthalene
Concen: 0.061 ng/ul
RT: 10.787 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM037049.D
Acq: 14 Oct 2022 11:19

Instrument :
BNA_M
ClientSampleId :
BGNM4

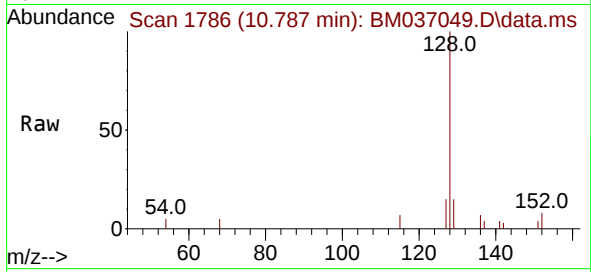

Tgt Ion:	128	Resp:	3770
Ion	Ratio	Lower	Upper
128	100		
129	15.1	10.2	15.2
127	15.4	11.7	17.5

