

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
 Data File : BM037052.D
 Acq On : 14 Oct 2022 13:06
 Operator : CG/JU
 Sample : N4980-12
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Z2

Quant Time: Oct 14 23:02:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 14 07:11:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7151	0.400	ng/ul	0.00
4) Naphthalene-d8	10.738	136	25830	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.561	164	16486	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.301	188	28718	0.400	ng/ul #	0.00
17) Chrysene-d12	21.473	240	15708	0.400	ng/ul #	0.00
23) Perylene-d12	23.864	264	13901	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	62781	6.225	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	12631	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.321	212	21861	0.465	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.373	88	378149	38.359	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101322\
Data File : BM037052.D
Acq On : 14 Oct 2022 13:06
Operator : CG/JU
Sample : N4980-12
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Z2

Quant Time: Oct 14 23:02:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 07:11:07 2022
Response via : Initial Calibration

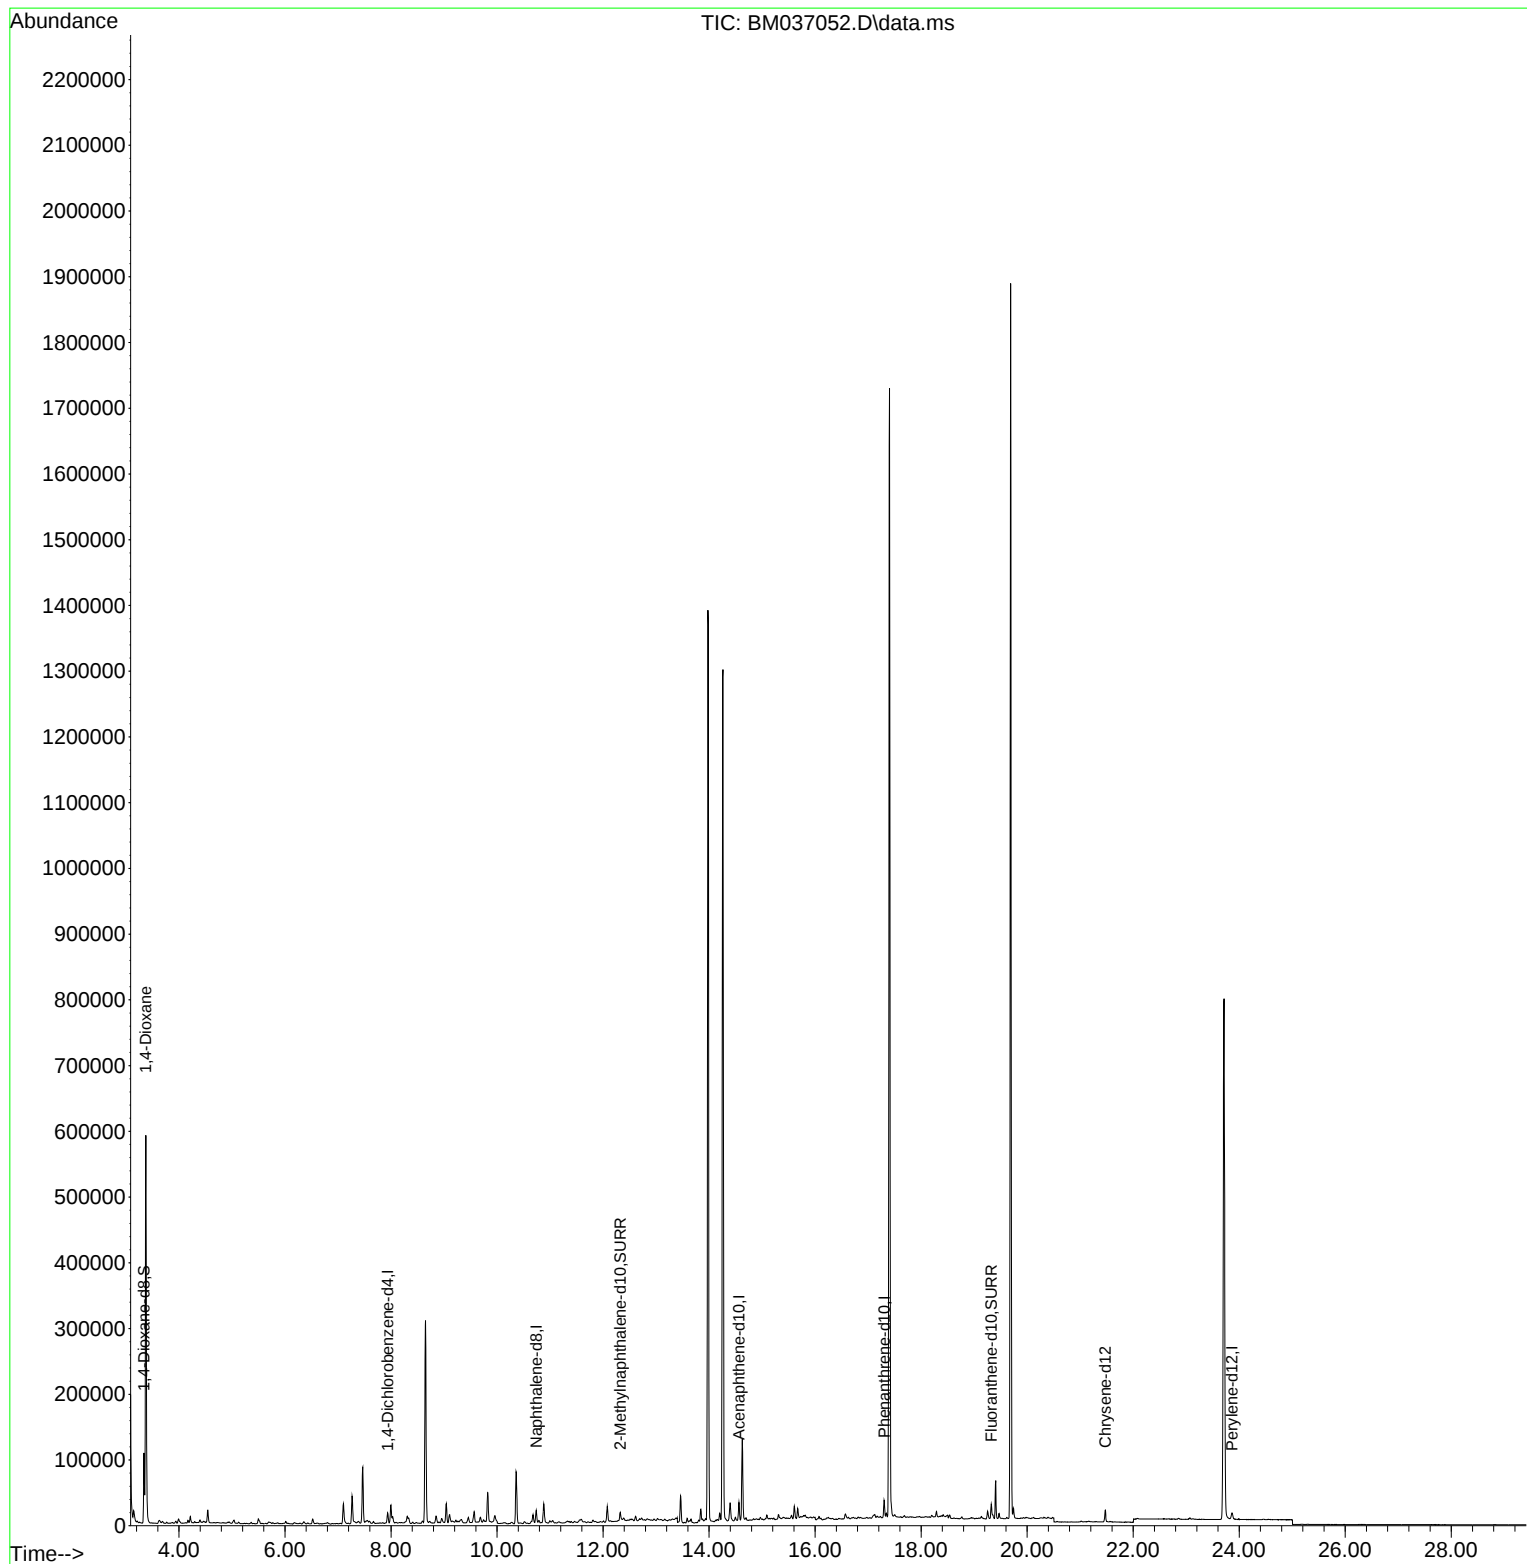

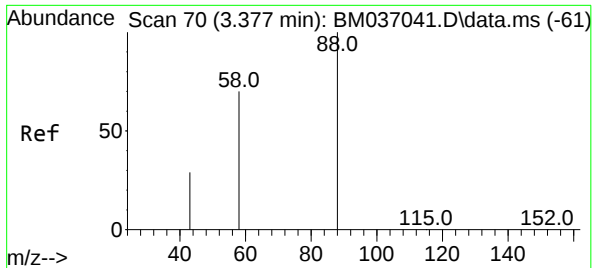

#2
 1,4-Dioxane
 Concen: 38.359 ng/ul
 RT: 3.373 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BM037052.D
 Acq: 14 Oct 2022 13:06

Instrument :
 BNA_M
 ClientSampleId :
 CB8Z2

Tgt Ion: 88 Resp: 378149
 Ion Ratio Lower Upper
 88 100
 43 28.3 37.8 56.6#
 58 70.4 42.6 63.8#

